


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
 Data File : BF127310.D
 Acq On : 14 Mar 2022 09:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 16:51:53 2022

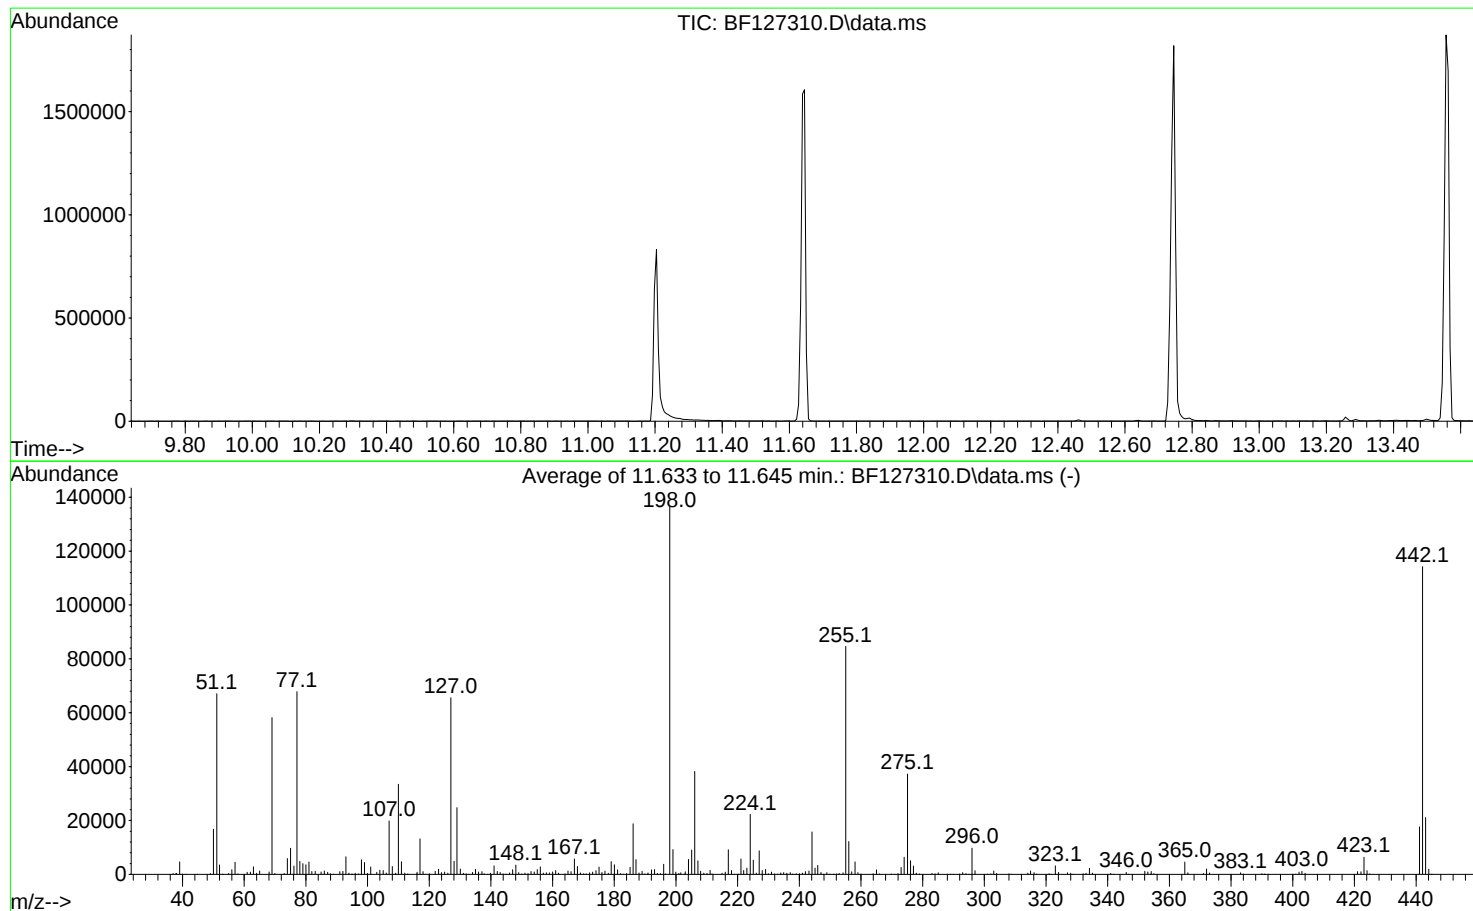

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	67056	PASS
68	69	0.00	2	1.5	896	PASS
69	198	0.00	100	42.6	58219	PASS
70	69	0.00	2	0.6	349	PASS
127	198	10	80	48.0	65600	PASS
197	198	0.00	2	0.1	175	PASS
198	198	100	100	100.0	136555	PASS
199	198	5	9	6.7	9189	PASS
275	198	10	60	27.3	37238	PASS
365	198	1	100	3.4	4599	PASS
441	198	0.01	100	12.9	17662	PASS
442	442	50	100	100.0	114240	PASS
443	442	15	24	18.5	21102	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/14/2022	BNA_F	<u>BF127310.D</u>
Compound Name	Response	Retention Time
DDT	354768	13.56
DDD	3860	13.26
DDE	389	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4249	359017	1.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
Data File : BF127310.D
Acq On : 14 Mar 2022 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 14 12:15:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

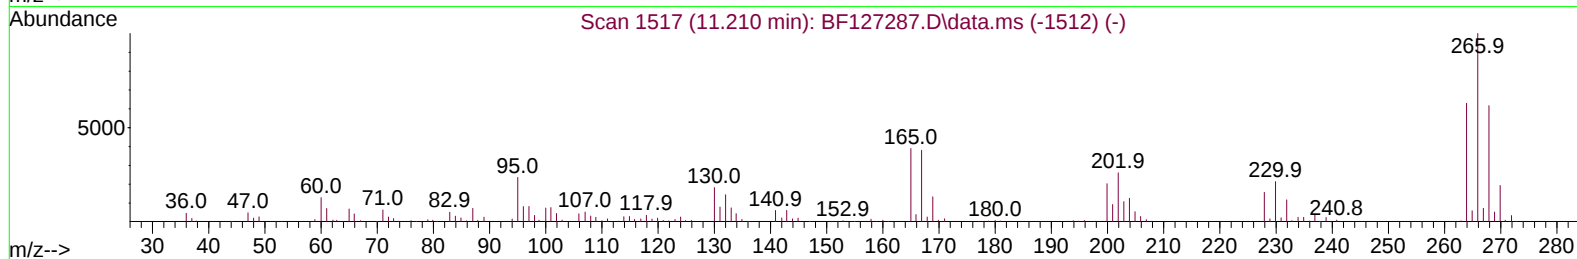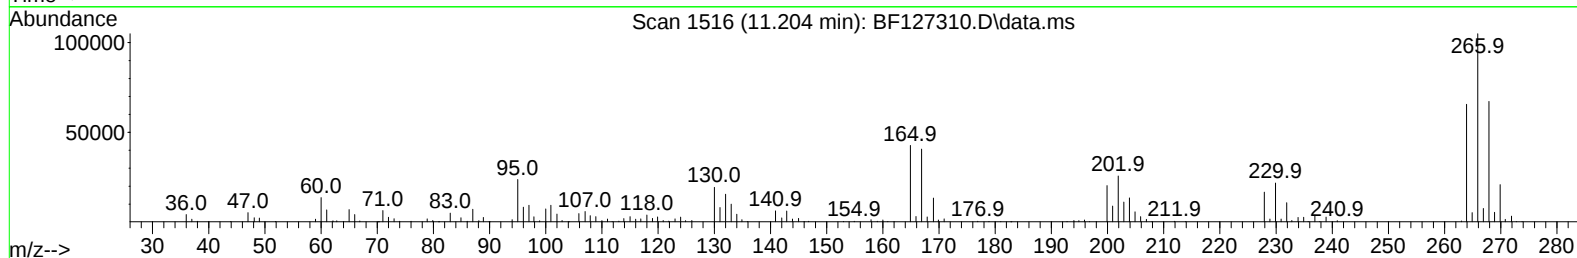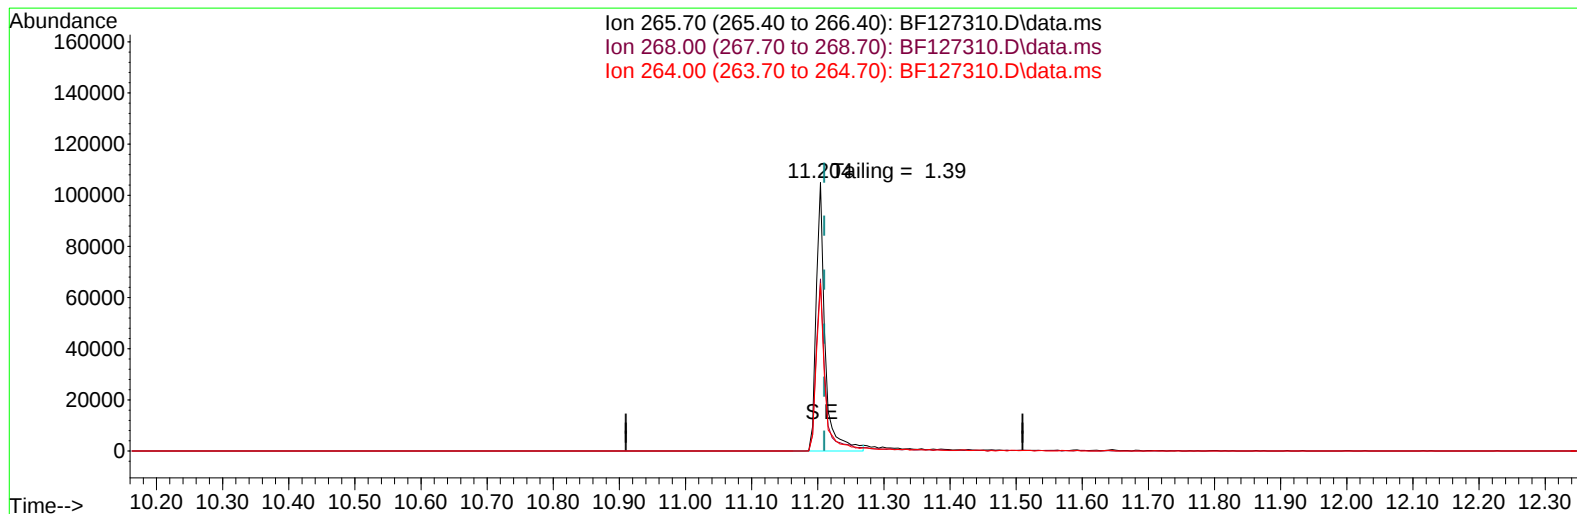

TIC: BF127310.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 29666.83 ng




response 104645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.08
264.00	63.00	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031422\
 Data File : BF127310.D
 Acq On : 14 Mar 2022 09:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 14 12:15:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 16:51:53 2022
 Response via : Initial Calibration

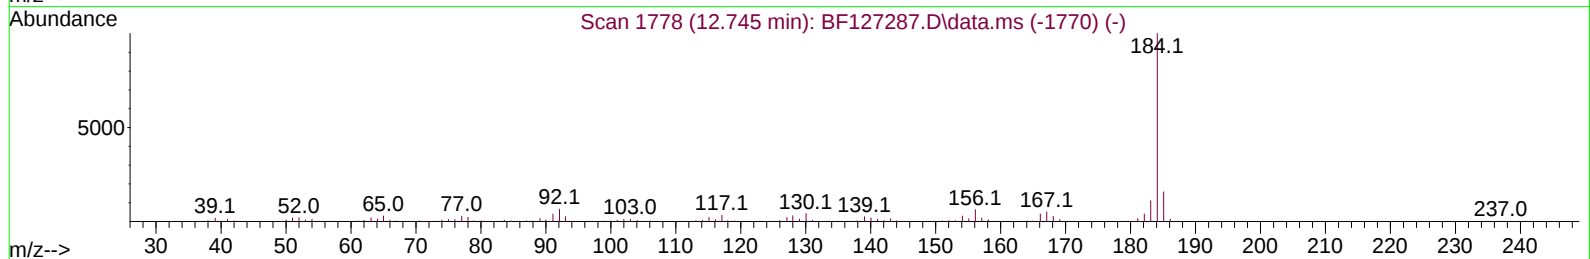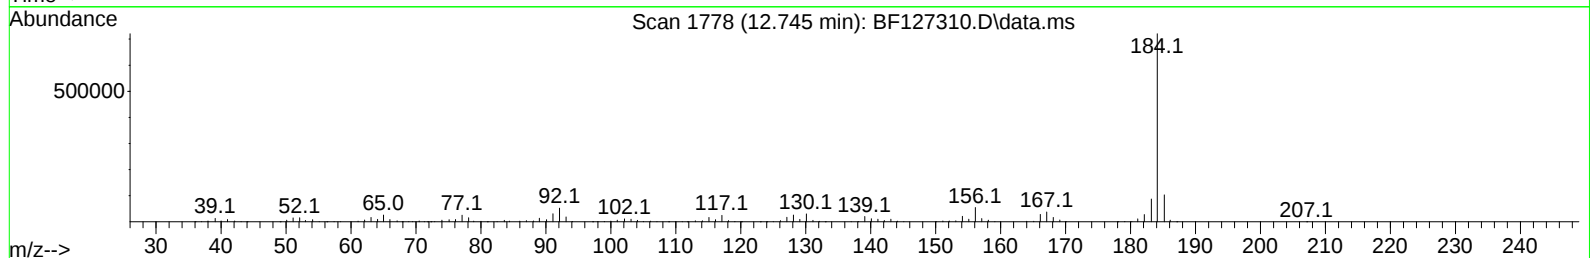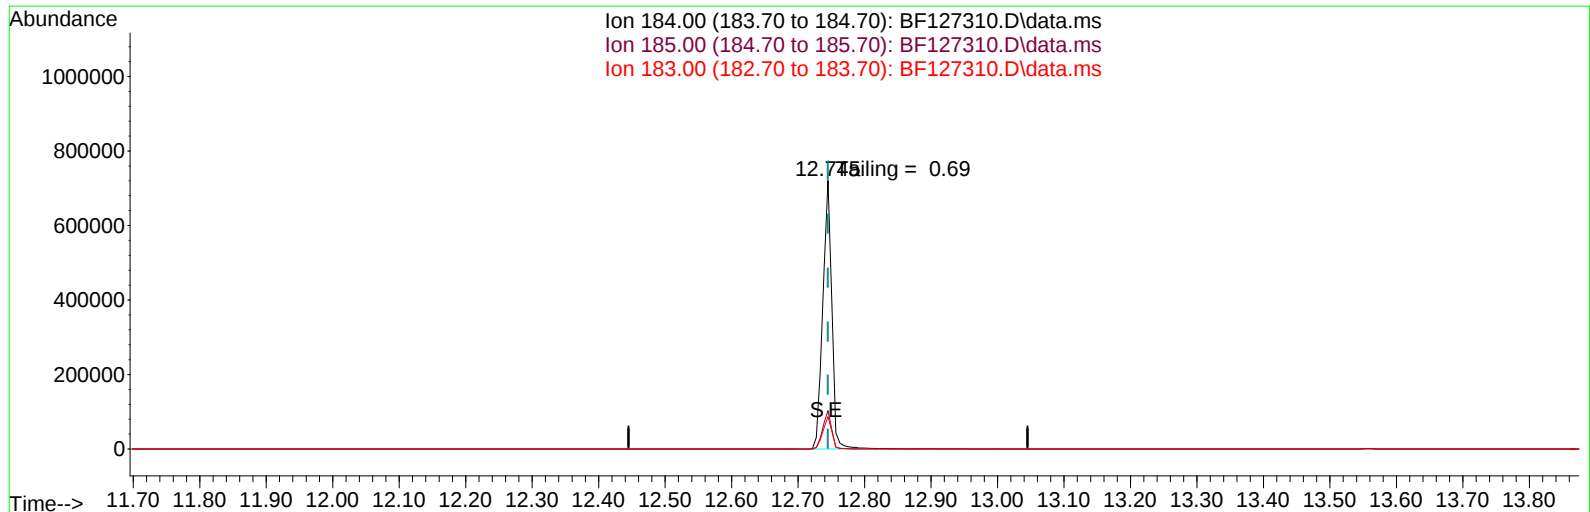

TIC: BF127310.D\data.ms

(77) Benzidine

12.745min (-0.000) 0.00 ng

response 681856

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.30
183.00	10.20	12.08
0.00	0.00	0.00