
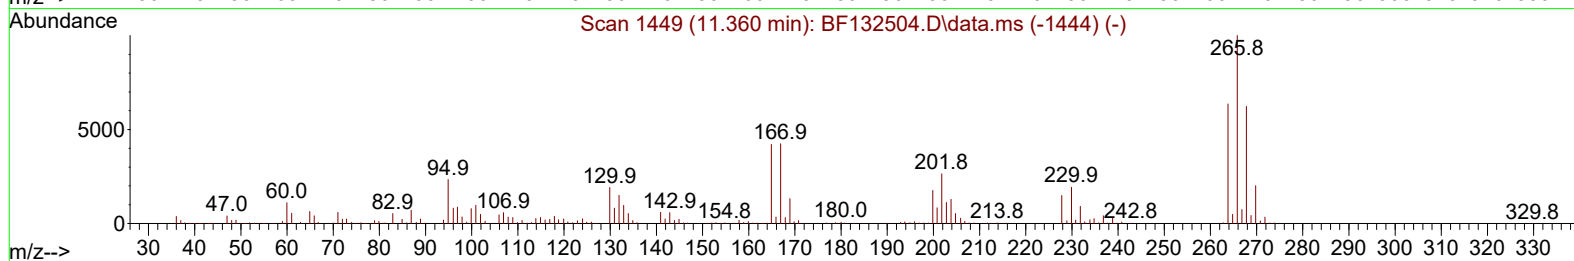
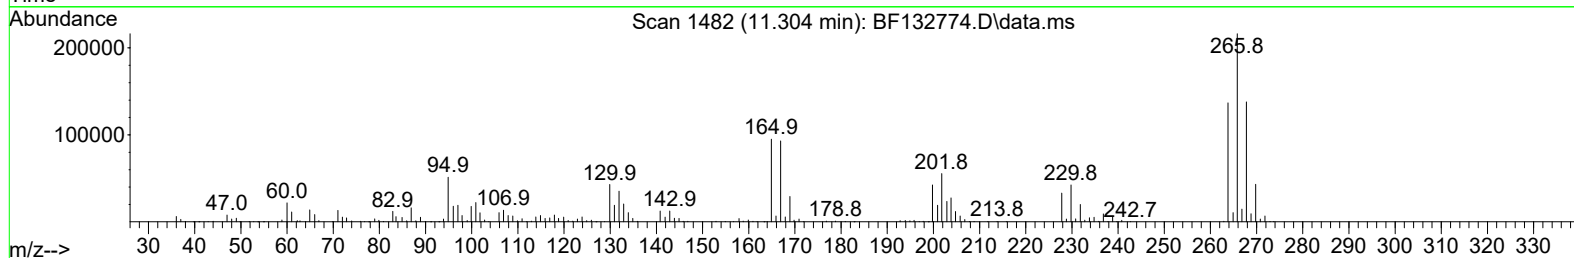


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031423\
Data File : BF132774.D
Acq On : 14 Mar 2023 12:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:56:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 15:35:42 2023
Response via : Initial Calibration

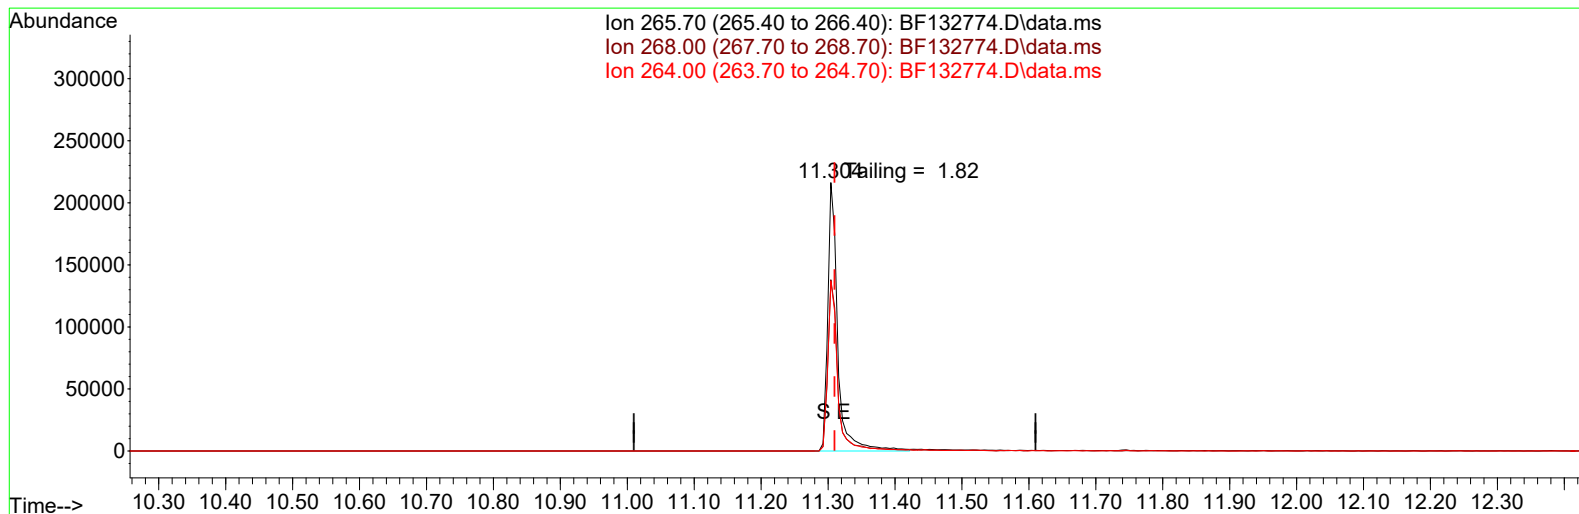

TIC: BF132774.D\data.ms

(70) Pentachlorophenol (C)




11.304min (-0.006) 23915.20 ng

response 225751

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.78
264.00	63.60	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031423\
 Data File : BF132774.D
 Acq On : 14 Mar 2023 12:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:56:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 15:35:42 2023
 Response via : Initial Calibration

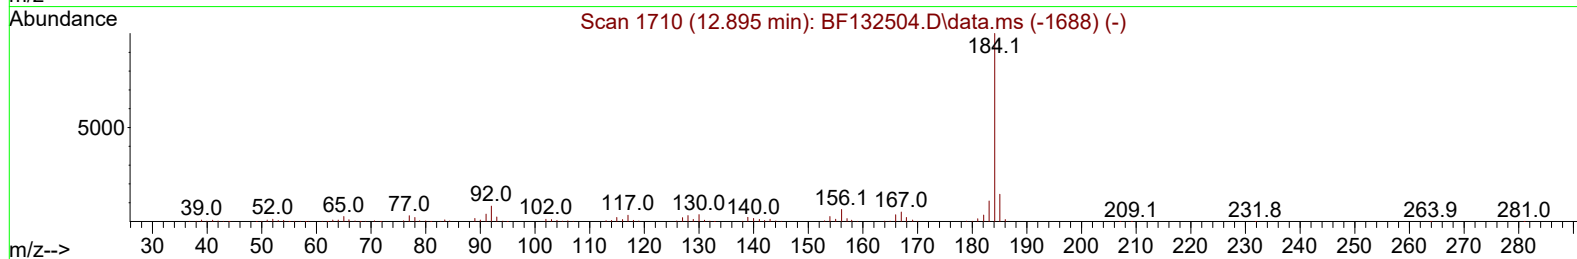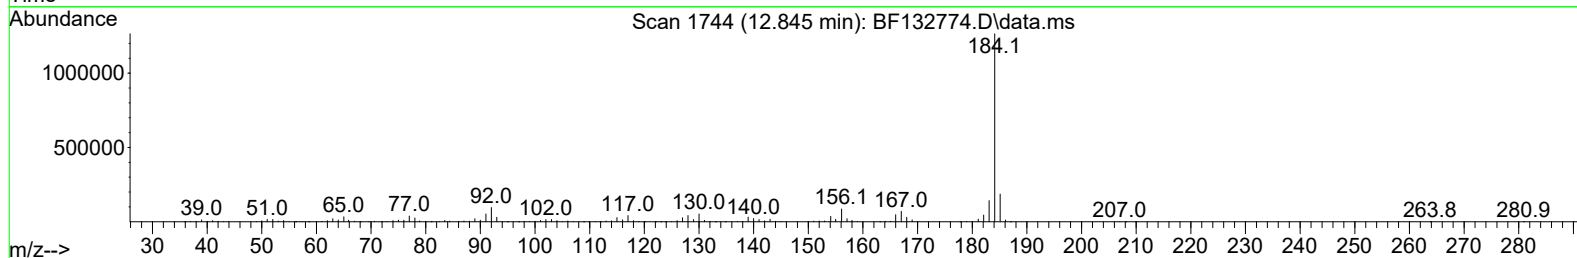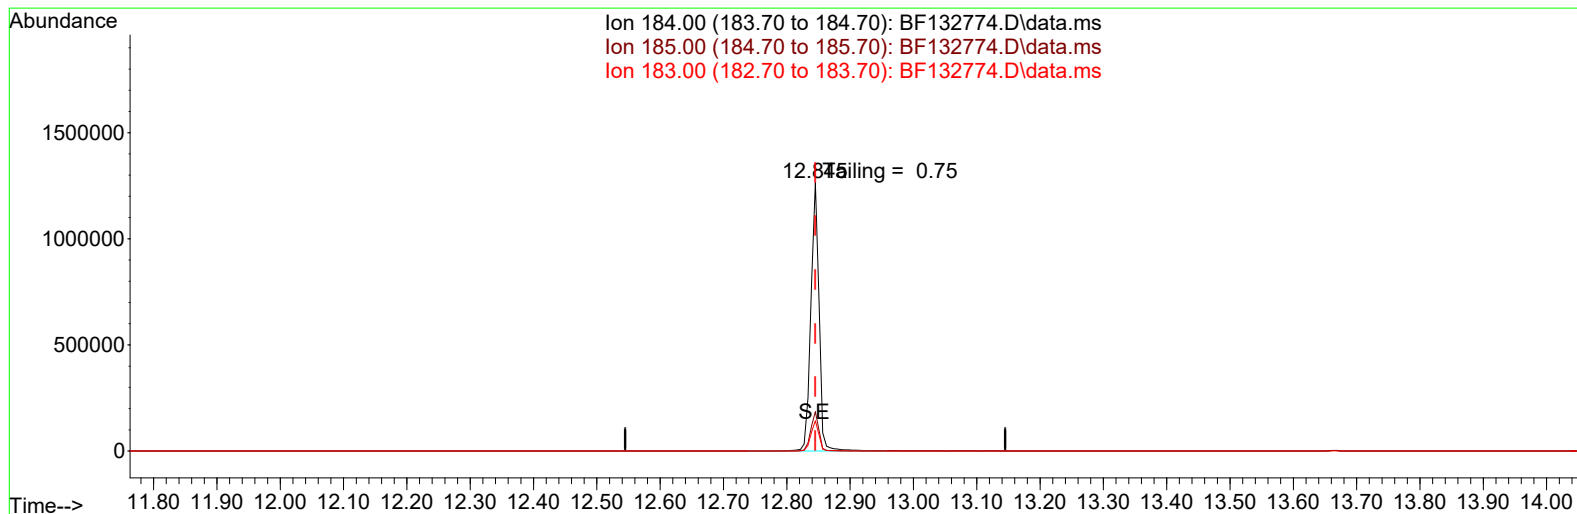

TIC: BF132774.D\data.ms

(77) Benzidine**12.845min (+ 0.000) 195264.69 ng****response 1155052**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.71
183.00	10.90	11.27
0.00	0.00	0.00