


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031423\  
Data File : BF132774.D  
Acq On : 14 Mar 2023 12:51  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF022223.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Mar 14 15:35:42 2023

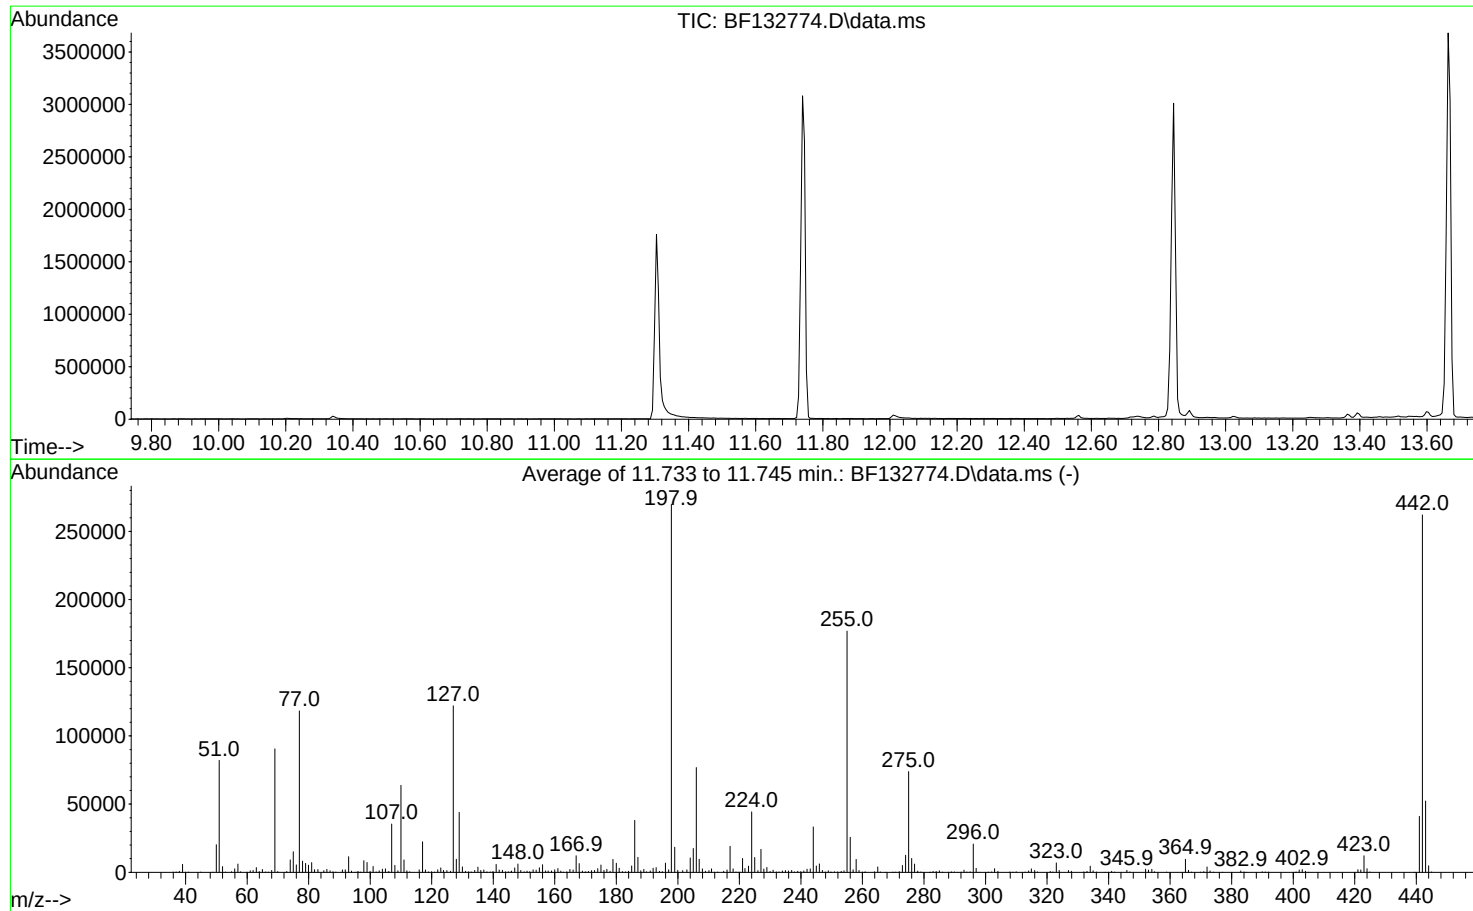




AutoFind: Scans 1555, 1556, 1557; Background Corrected with Scan 1550

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 30.4         | 82037      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 1403       | PASS                |
| 69             | 198             | 0.00            | 100             | 33.6         | 90571      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 527        | PASS                |
| 127            | 198             | 10              | 80              | 45.3         | 122088     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.7          | 1781       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 269781     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 18371      | PASS                |
| 275            | 198             | 10              | 60              | 27.4         | 73864      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 9575       | PASS                |
| 441            | 198             | 0.01            | 100             | 15.2         | 41068      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 262032     | PASS                |
| 443            | 442             | 15              | 24              | 20.0         | 52296      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031423\  
Data File : BF132774.D  
Acq On : 14 Mar 2023 12:51  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Mar 15 05:56:51 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF022223.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 14 15:35:42 2023  
Response via : Initial Calibration

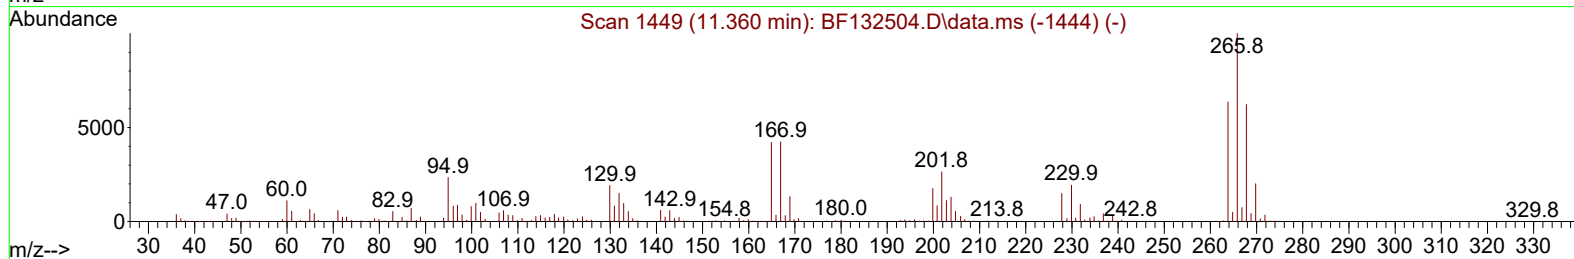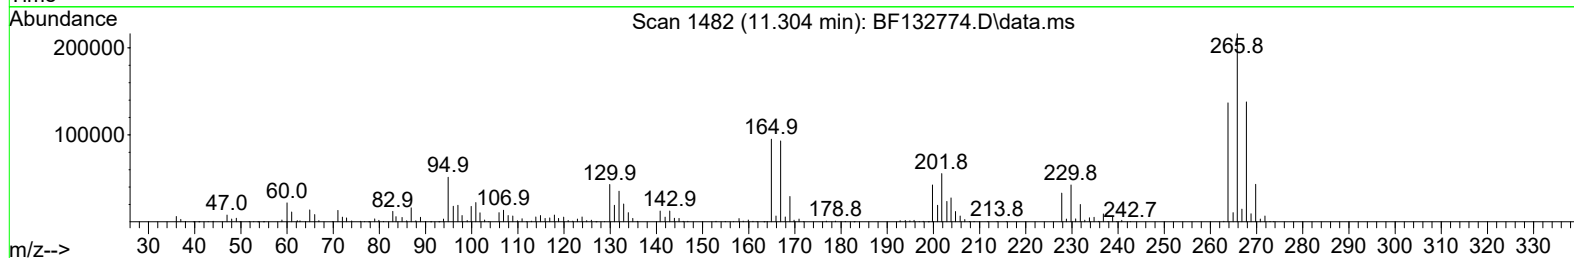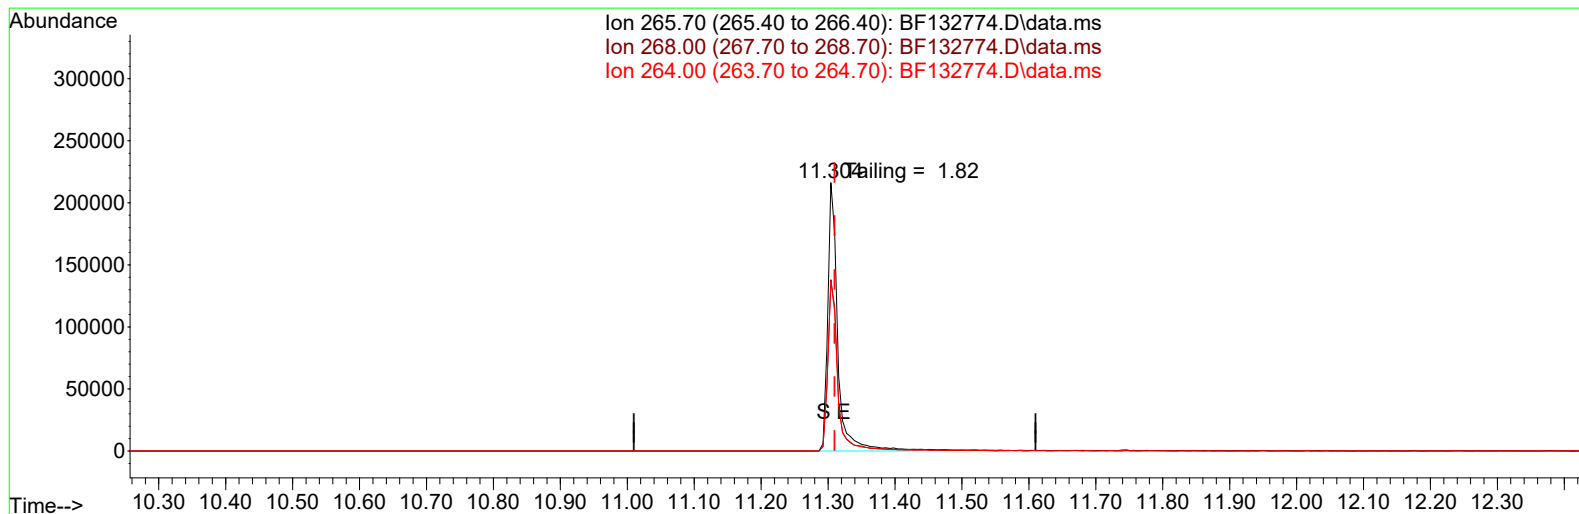

TIC: BF132774.D\data.ms

**(70) Pentachlorophenol (C)**

**11.304min (-0.006) 23915.20 ng**




**response 225751**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.78  |
| 264.00 | 63.60  | 63.27  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031423\  
Data File : BF132774.D  
Acq On : 14 Mar 2023 12:51  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Mar 15 05:56:51 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF022223.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 14 15:35:42 2023  
Response via : Initial Calibration

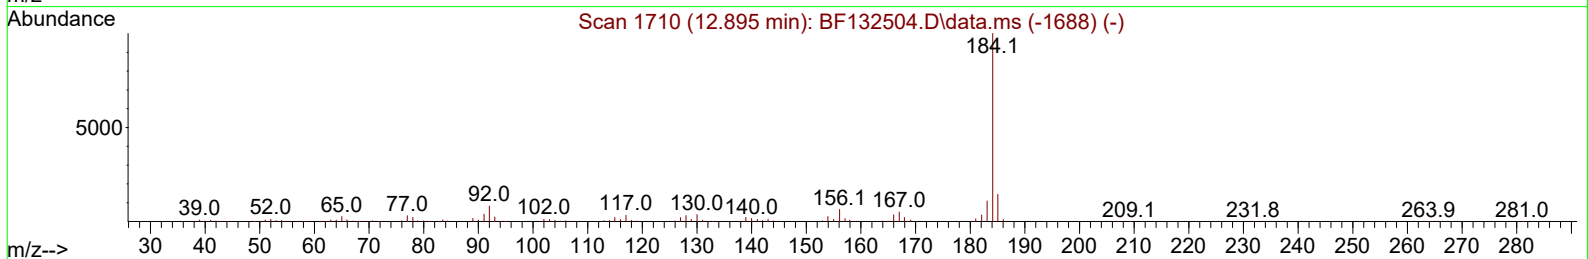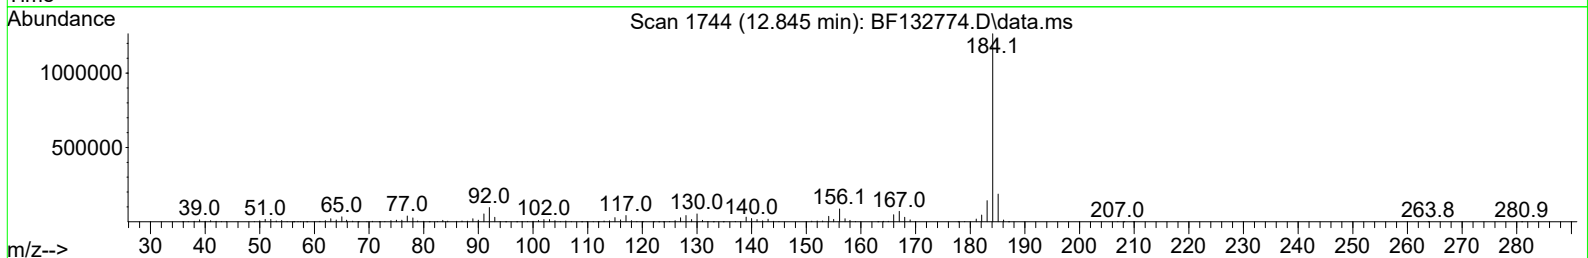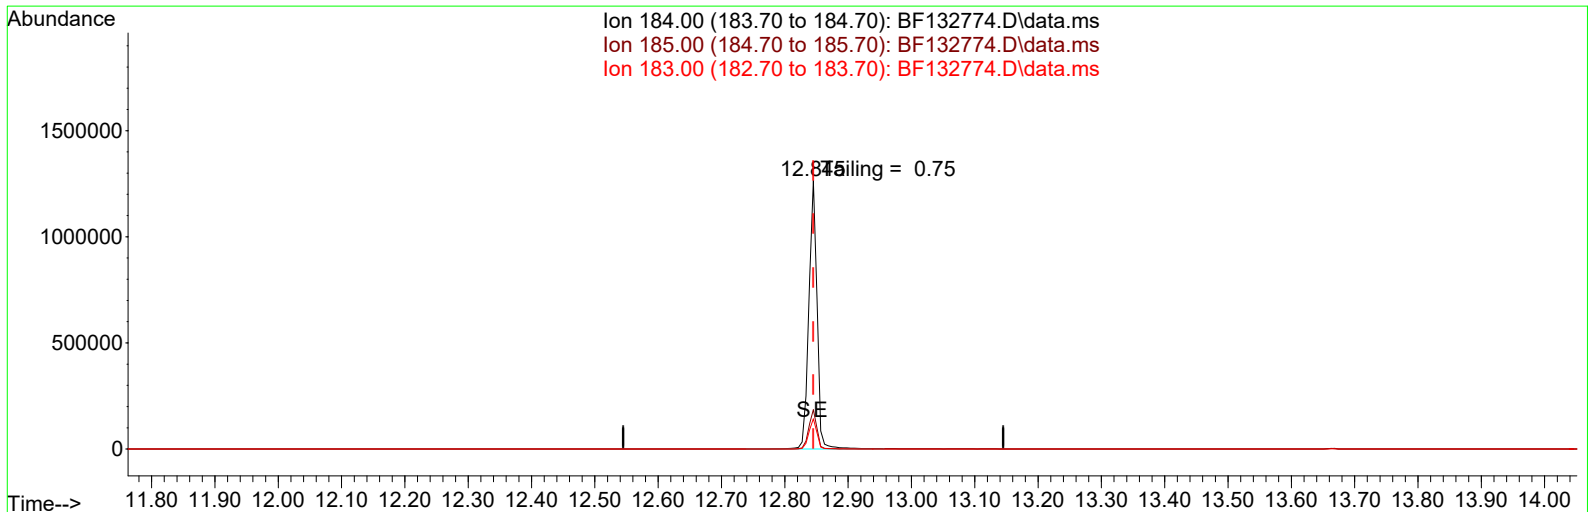

TIC: BF132774.D\data.ms

**(77) Benzidine**

**12.845min (+ 0.000) 195264.69 ng**

**response 1155052**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 14.71  |
| 183.00 | 10.90  | 11.27  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/14/2023     | BNA_F            | <u>BF132774.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 685967           | 13.663             |
| DDD           | 14822            | 13.392             |
| DDE           | 3097             | 13.027             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 17919         | 703886           | 2.55               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP