
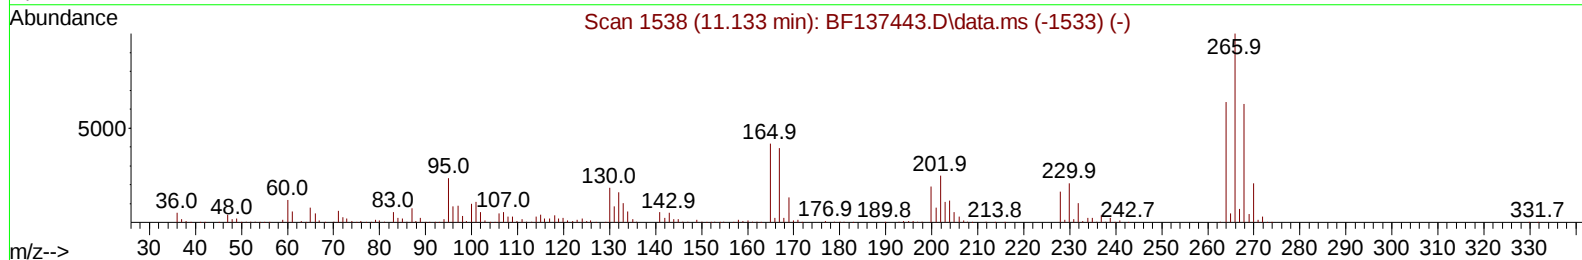
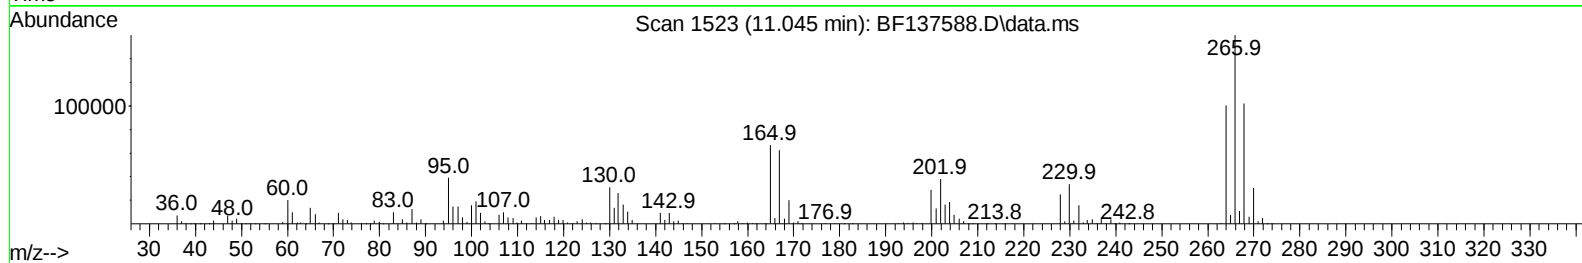


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031424\
Data File : BF137588.D
Acq On : 14 Mar 2024 13:33
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 15:46:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

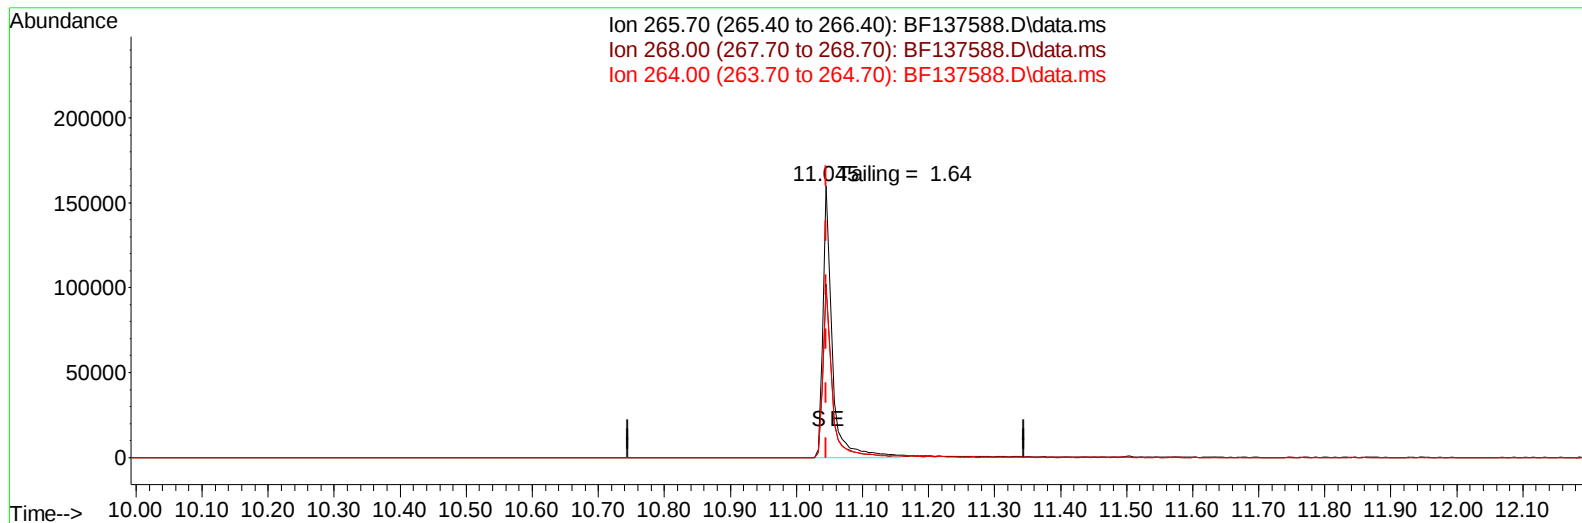

TIC: BF137588.D\data.ms

(70) Pentachlorophenol (C)




11.045min (-0.000) 25693.75 ng

response 157029

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.71
264.00	63.60	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031424\
Data File : BF137588.D
Acq On : 14 Mar 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 15:46:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

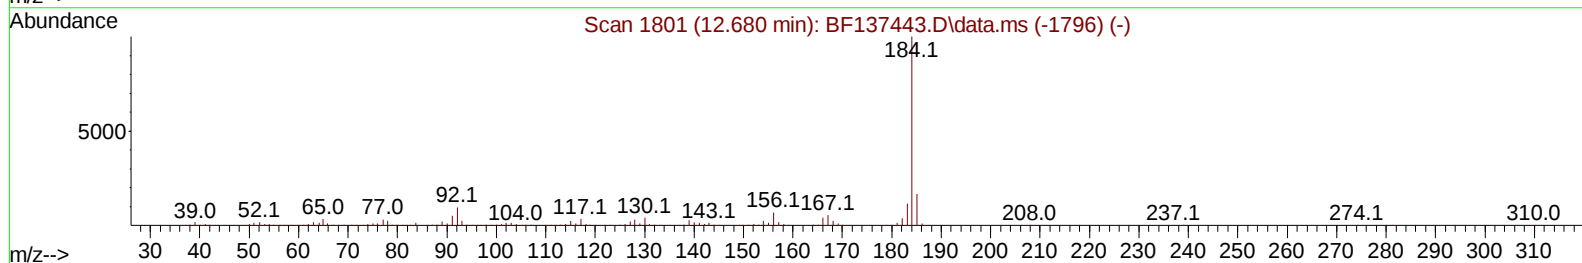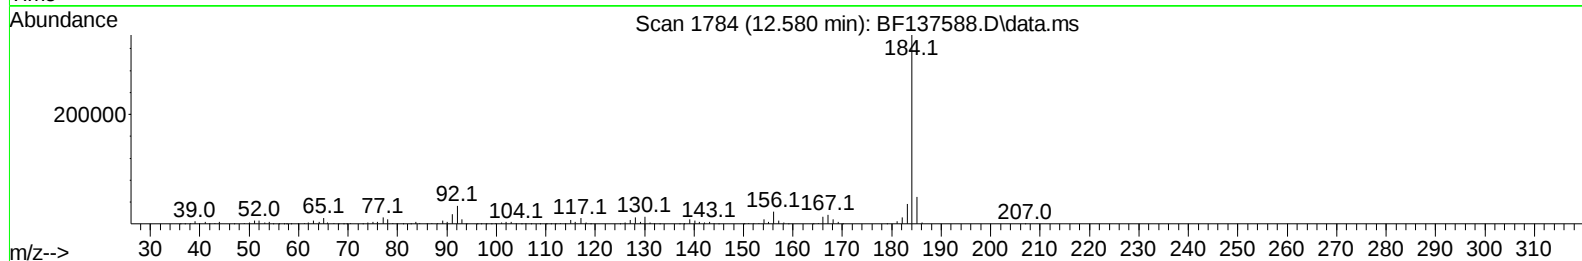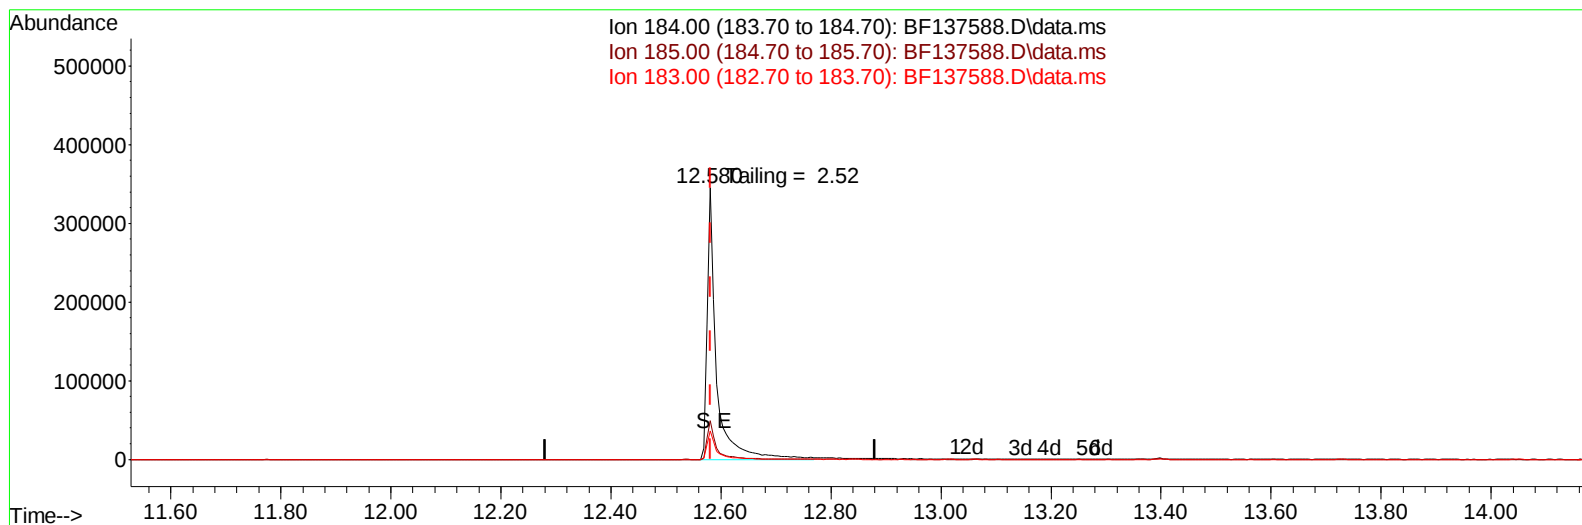

TIC: BF137588.D\data.ms

(77) Benzidine

12.580min (-0.000) 328079.03 ng m

response 433557

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.30
183.00	11.60	10.52
0.00	0.00	0.00