
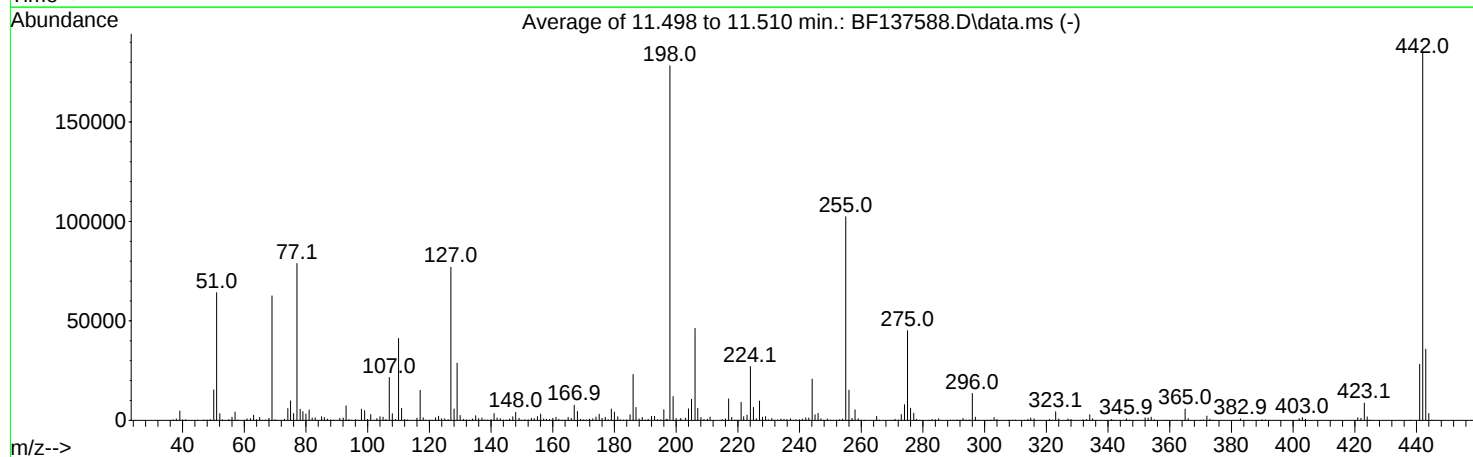


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031424\
Data File : BF137588.D
Acq On : 14 Mar 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 14:45:20 2024

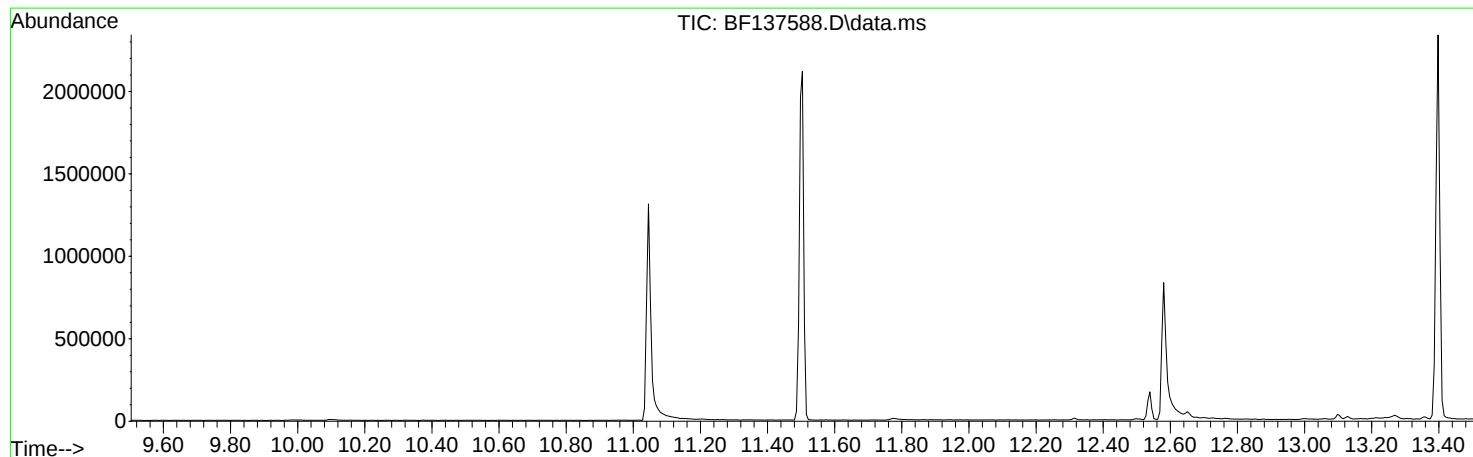




AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	64171	PASS
68	69	0.00	2	1.7	1046	PASS
69	198	0.00	100	35.1	62563	PASS
70	69	0.00	2	0.5	316	PASS
127	198	10	80	43.2	76960	PASS
197	198	0.00	2	0.3	539	PASS
198	198	100	100	100.0	178251	PASS
199	198	5	9	6.7	12013	PASS
275	198	10	60	25.3	45157	PASS
365	198	1	100	3.2	5721	PASS
441	198	0.01	100	15.8	28216	PASS
442	442	50	100	100.0	184891	PASS
443	442	15	24	19.3	35755	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031424\
Data File : BF137588.D
Acq On : 14 Mar 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 14 15:46:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

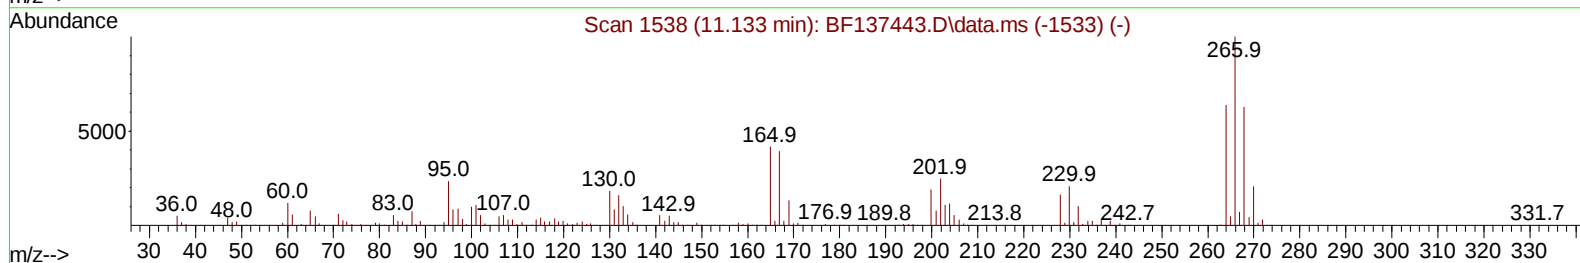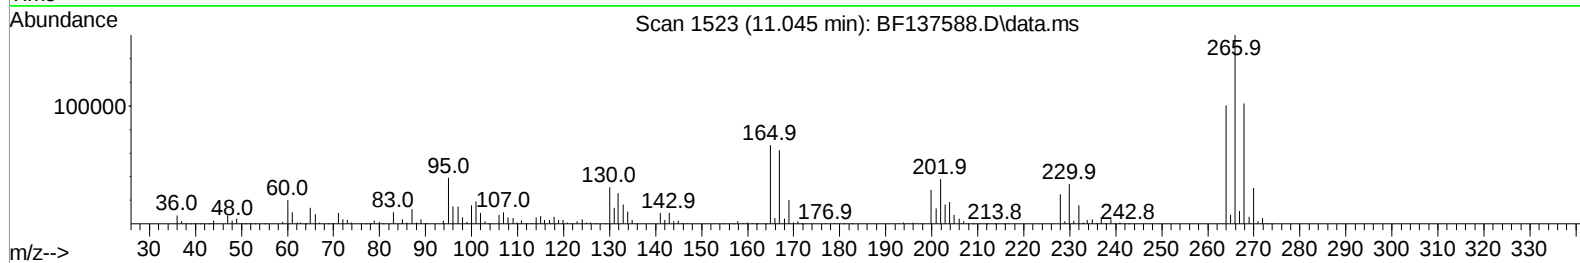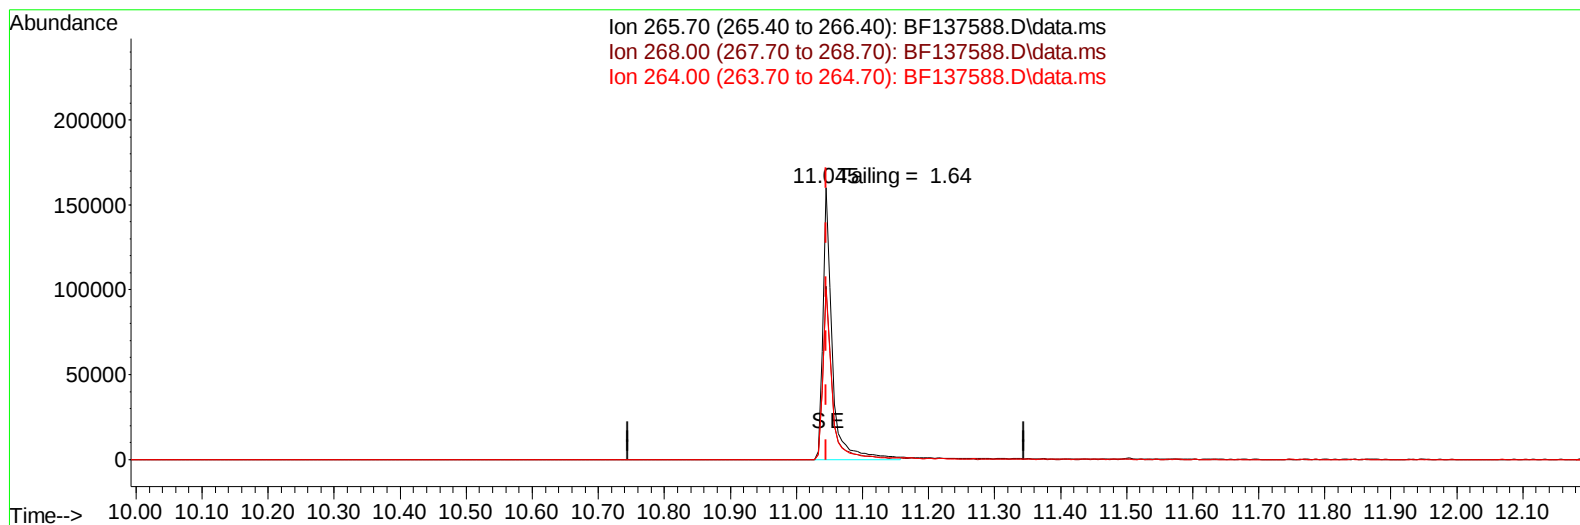

TIC: BF137588.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.000) 25693.75 ng




response 157029

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.71
264.00	63.60	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031424\
Data File : BF137588.D
Acq On : 14 Mar 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 14 15:46:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

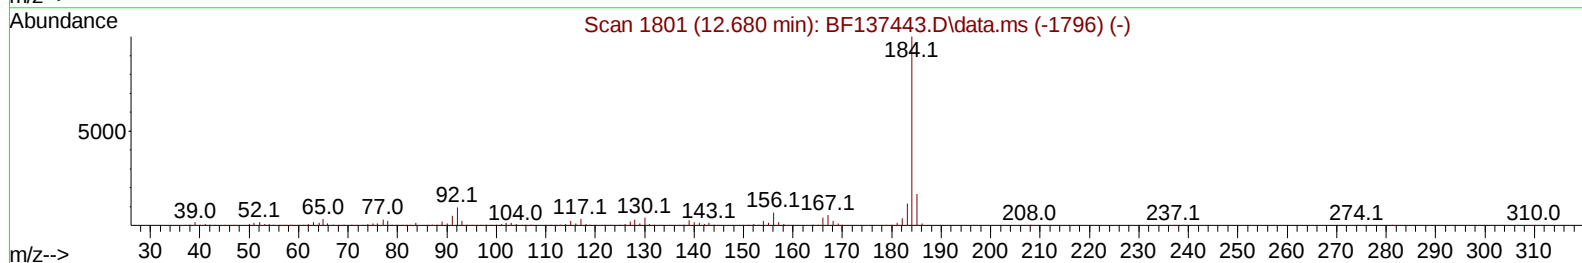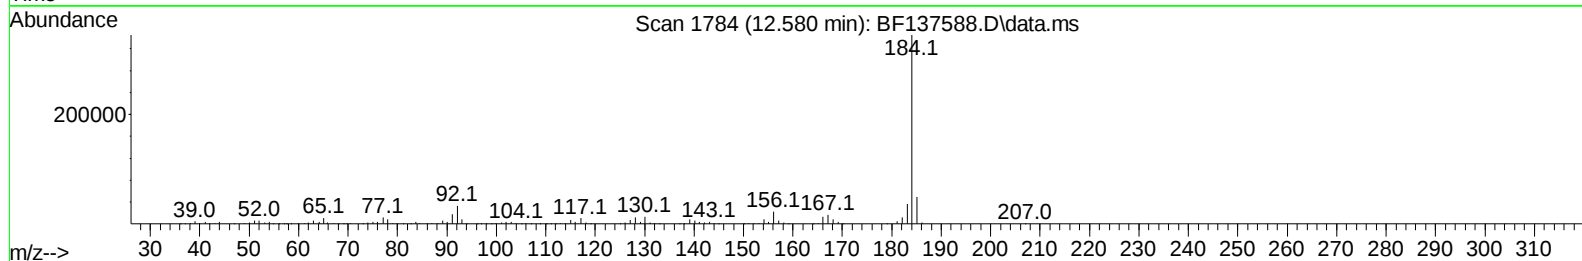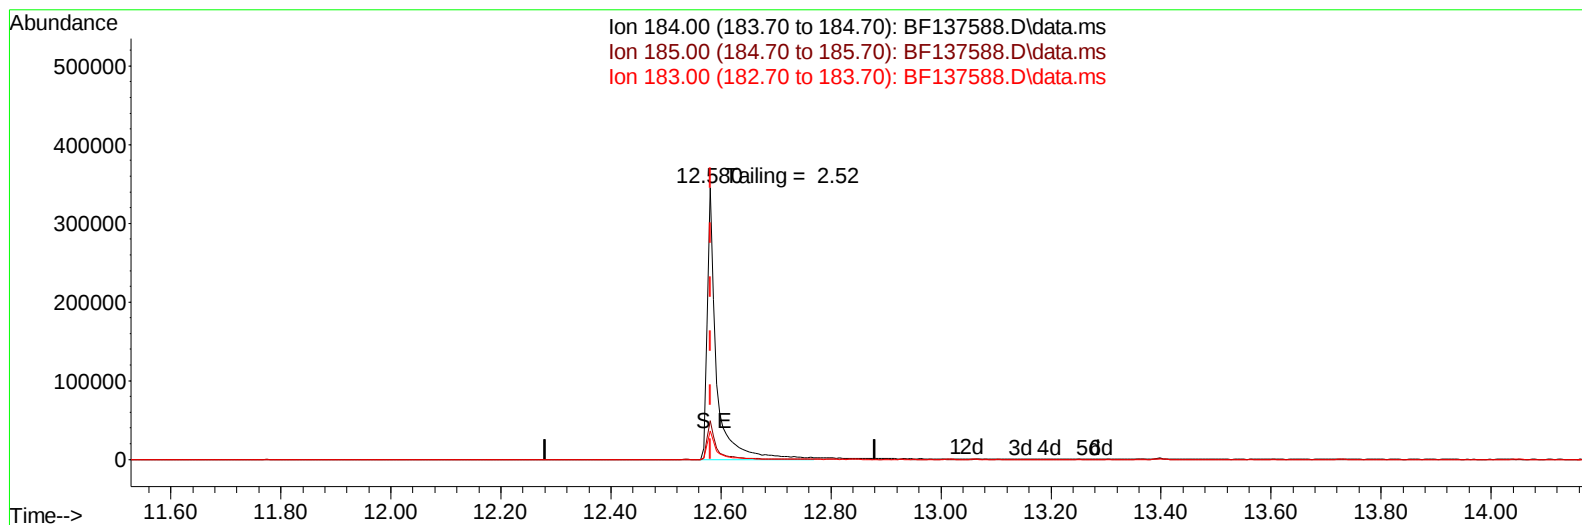

TIC: BF137588.D\data.ms

(77) Benzidine

12.580min (-0.000) 328079.03 ng m

response 433557

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.30
183.00	11.60	10.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2024	BNA_F	<u>BF137588.D</u>
Compound Name	Response	Retention Time
DDT	359524	13.398
DDD	8980	13.098
DDE	681	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9661	369185	2.62

Instrument :
BNA_F
ClientSampleId :
DFTPP