

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031425\
 Data File : BF141958.D
 Acq On : 14 Mar 2025 11:39
 Operator : RC/JU
 Sample : PB167123BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167123BL

Quant Time: Mar 14 12:18:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 10 15:46:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	149023	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	593343	20.000	ng	0.00
39) Acenaphthene-d10	9.910	164	338386	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	598649	20.000	ng	0.00
76) Chrysene-d12	14.033	240	348554	20.000	ng	0.00
86) Perylene-d12	15.504	264	326717	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	1375162	154.009	ng	0.01
7) Phenol-d6	6.498	99	1648990	145.046	ng	0.00
23) Nitrobenzene-d5	7.434	82	1102015	104.521	ng	-0.01
42) 2,4,6-Tribromophenol	10.698	330	684546	159.461	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	2277051	102.338	ng	0.00
79) Terphenyl-d14	12.980	244	2840101	120.468	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031425\
Data File : BF141958.D
Acq On : 14 Mar 2025 11:39
Operator : RC/JU
Sample : PB167123BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167123BL

Quant Time: Mar 14 12:18:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration




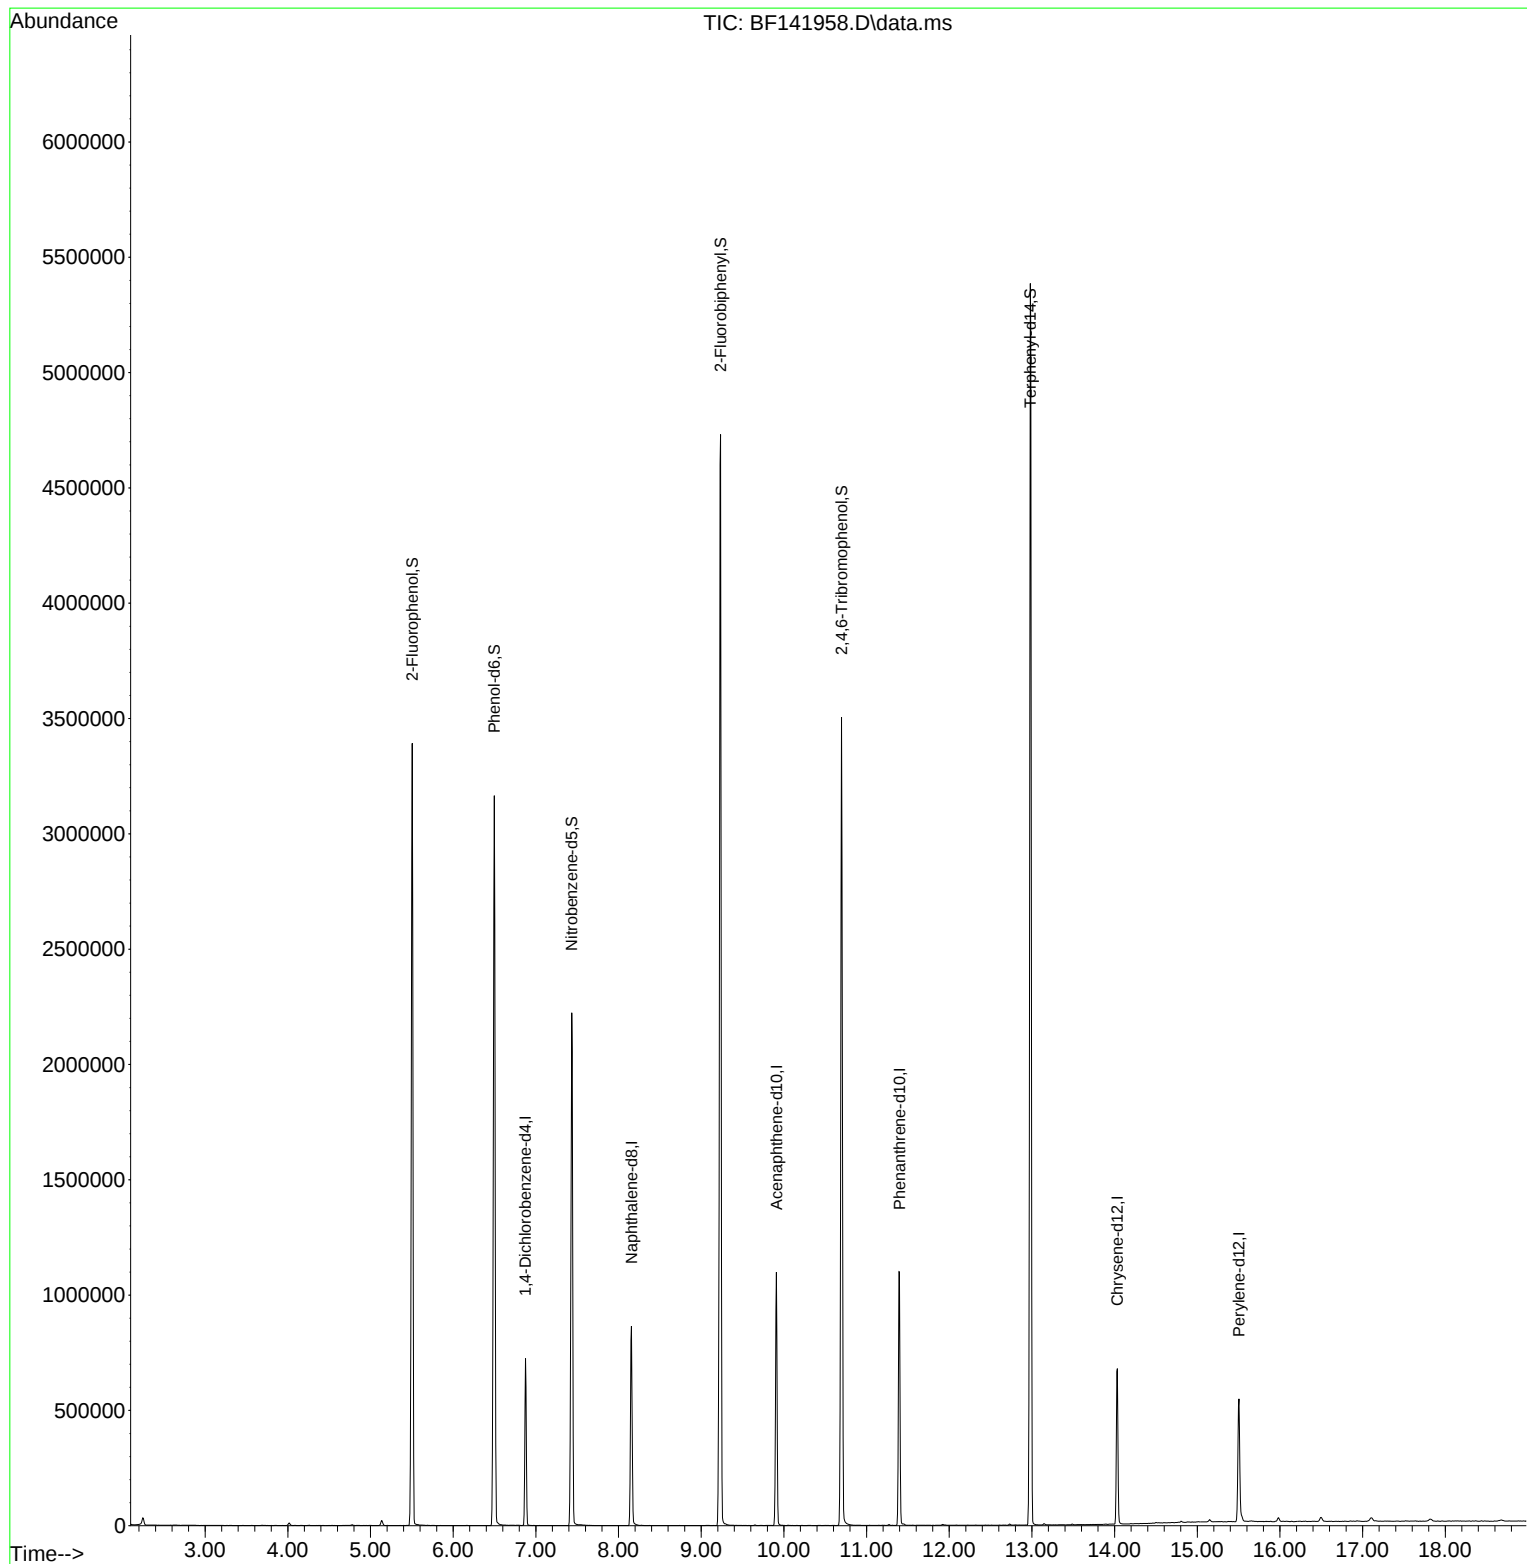




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.875 min Scan# 814
 Delta R.T. -0.006 min
 Lab File: BF141958.D
 Acq: 14 Mar 2025 11:39




Instrument :
 BNA_F
 ClientSampleId :
 PB167123BL


Tgt Ion:152 Resp: 149023
 Ion Ratio Lower Upper
 152 100
 150 156.4 127.4 191.2
 115 65.7 51.9 77.9

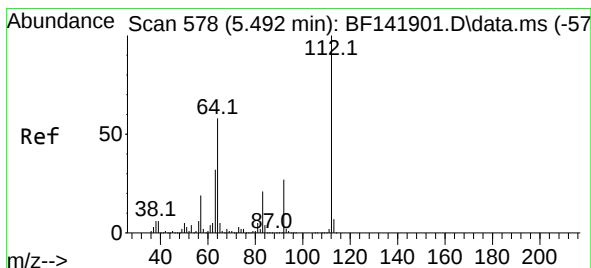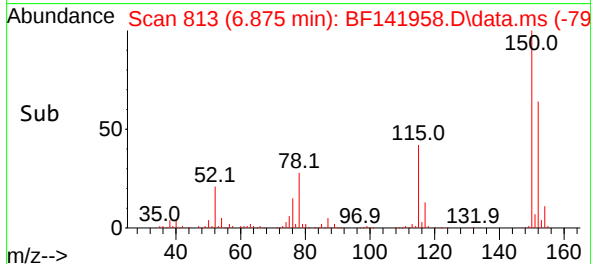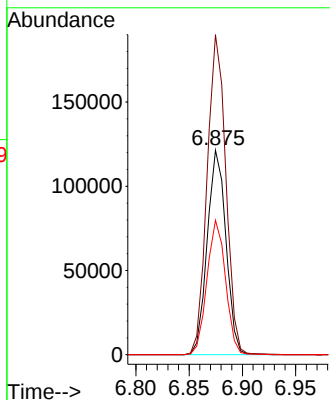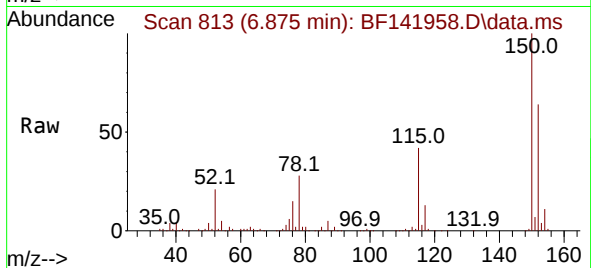

#5
 2-Fluorophenol
 Concen: 154.009 ng
 RT: 5.504 min Scan# 580
 Delta R.T. 0.012 min
 Lab File: BF141958.D
 Acq: 14 Mar 2025 11:39

Tgt Ion:112 Resp: 1375162
 Ion Ratio Lower Upper
 112 100
 64 56.0 46.5 69.7
 63 31.1 25.4 38.2


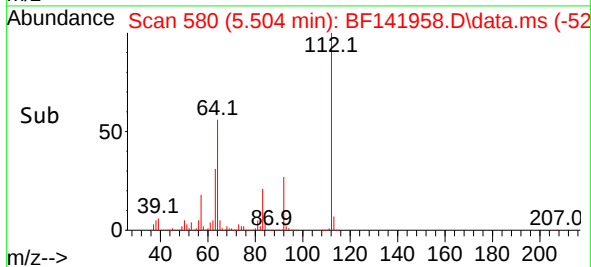
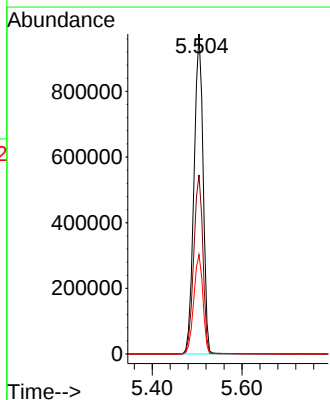
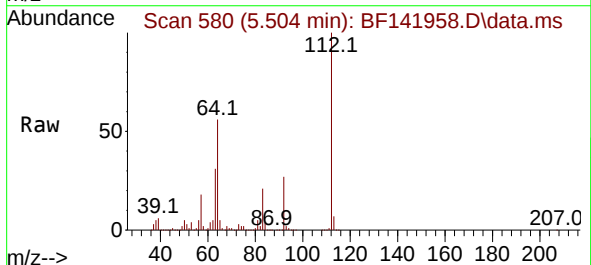


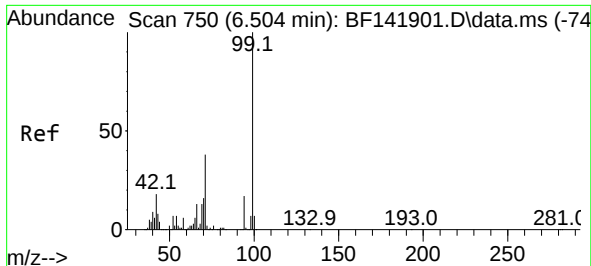

#7
Phenol-d6
Concen: 145.046 ng
RT: 6.498 min Scan# 74
Delta R.T. -0.006 min
Lab File: BF141958.D
Acq: 14 Mar 2025 11:39




Instrument :
BNA_F
ClientSampleId :
PB167123BL


Tgt Ion: 99 Resp: 1648990
Ion Ratio Lower Upper
99 100
42 17.5 14.6 21.8
71 38.8 30.8 46.2

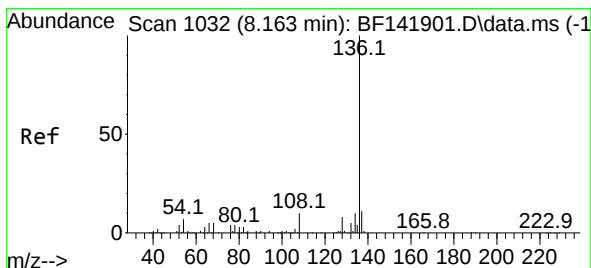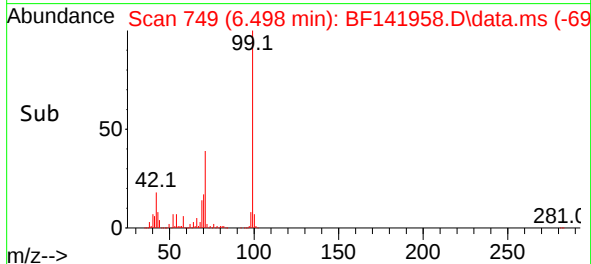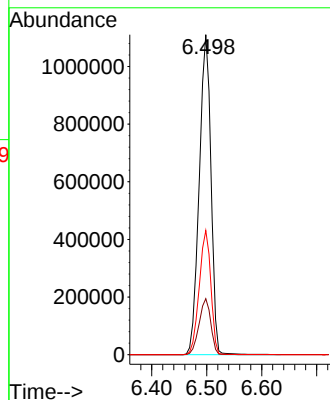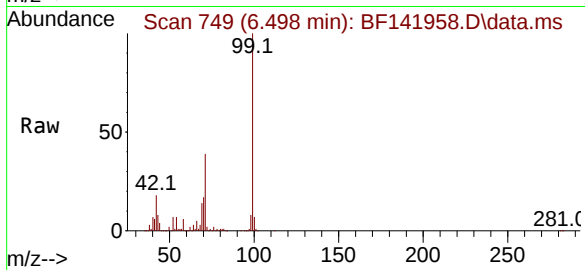

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BF141958.D
Acq: 14 Mar 2025 11:39

Tgt Ion:136 Resp: 593343
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 6.5 5.8 8.8
68 4.6 4.1 6.1

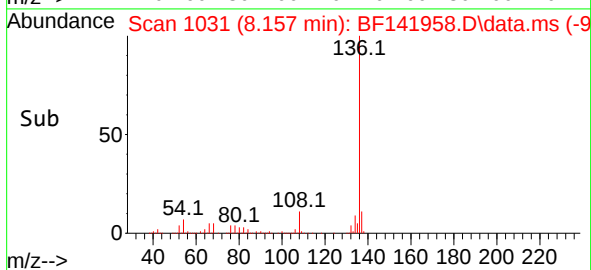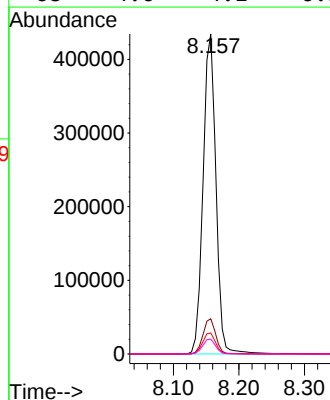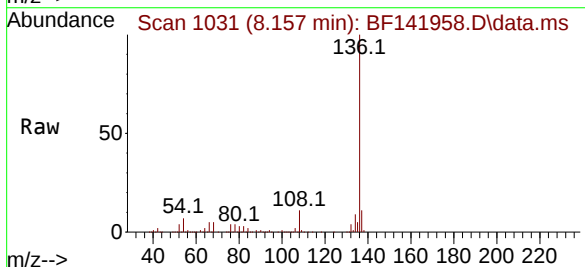

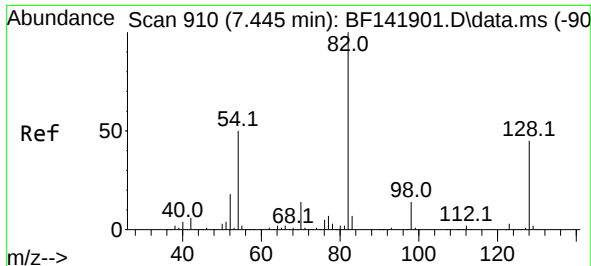

#23

Nitrobenzene-d5

Concen: 104.521 ng

RT: 7.434 min Scan# 90

Delta R.T. -0.012 min

Lab File: BF141958.D

Acq: 14 Mar 2025 11:39

Instrument :





BNA_F

ClientSampleId :

PB167123BL

Tgt Ion: 82 Resp: 1102015

Ion	Ratio	Lower	Upper
82	100		
128	44.7	36.0	54.0
54	48.5	39.6	59.4

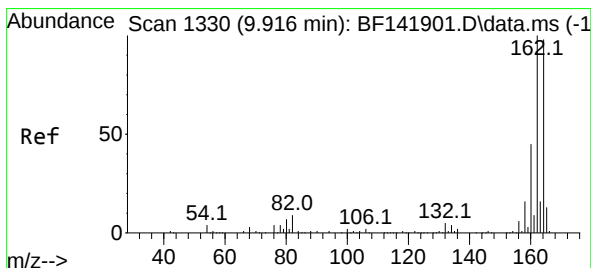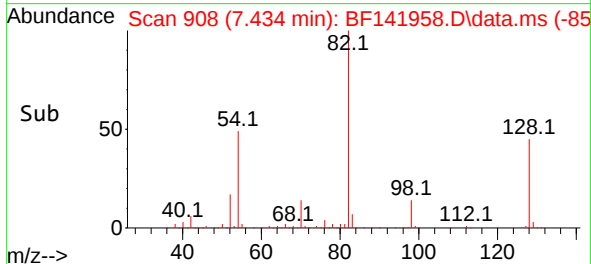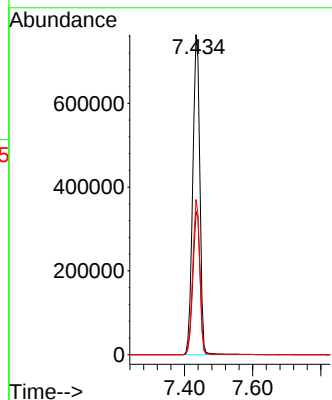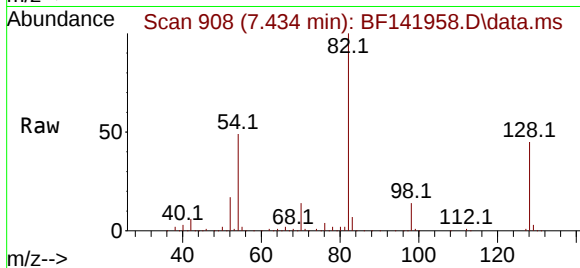

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.910 min Scan# 1329




Delta R.T. -0.006 min

Lab File: BF141958.D

Acq: 14 Mar 2025 11:39

Tgt Ion:164 Resp: 338386

Ion	Ratio	Lower	Upper
164	100		
162	102.2	81.8	122.6
160	45.4	36.7	55.1

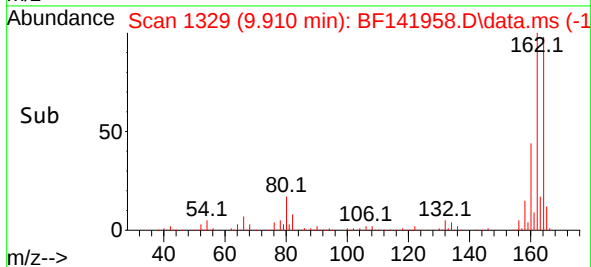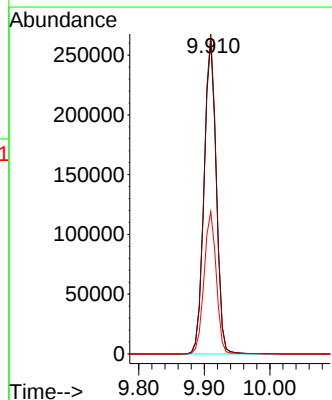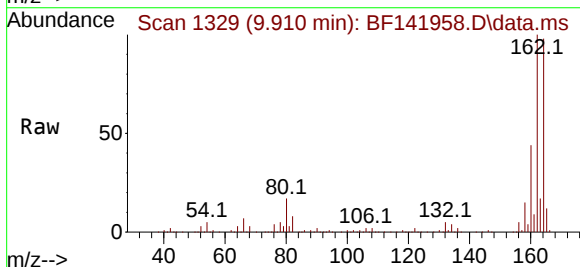



#42

2,4,6-Tribromophenol

Concen: 159.461 ng

RT: 10.698 min Scan# 1463

Delta R.T. -0.006 min

Lab File: BF141958.D

Acq: 14 Mar 2025 11:39

Instrument :

BNA_F

ClientSampleId :

PB167123BL





Tgt Ion:330 Resp: 684546

Ion Ratio Lower Upper

330 100

332 95.9 77.6 116.4

141 27.8 24.7 37.1

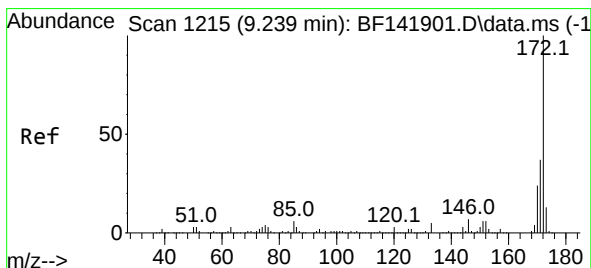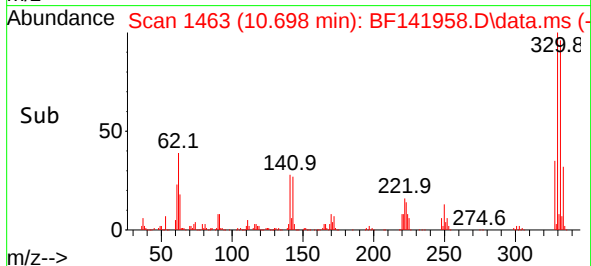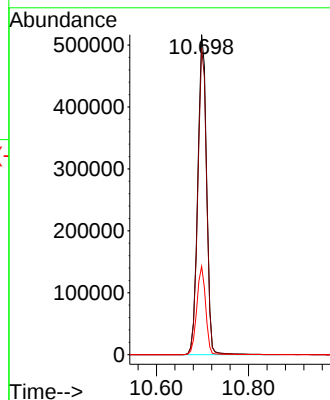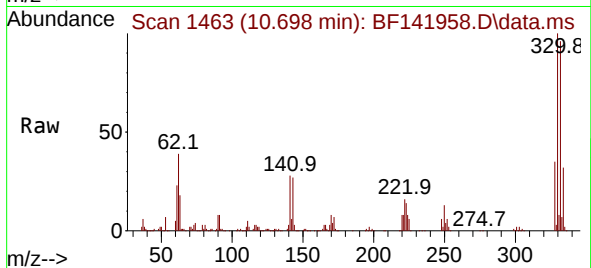

#45

2-Fluorobiphenyl

Concen: 102.338 ng

RT: 9.233 min Scan# 1214

Delta R.T. -0.006 min

Lab File: BF141958.D

Acq: 14 Mar 2025 11:39




Tgt Ion:172 Resp: 2277051

Ion Ratio Lower Upper

172 100

171 36.1 29.3 43.9

170 24.0 19.4 29.0


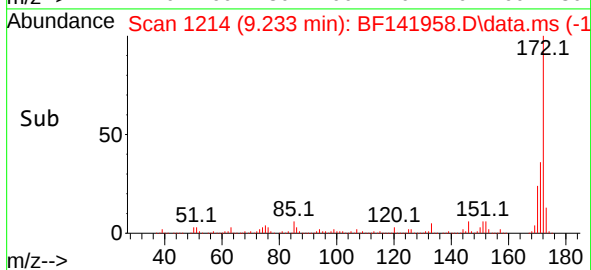
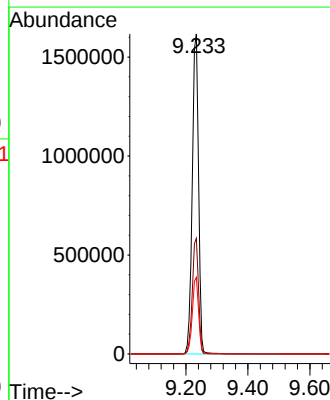
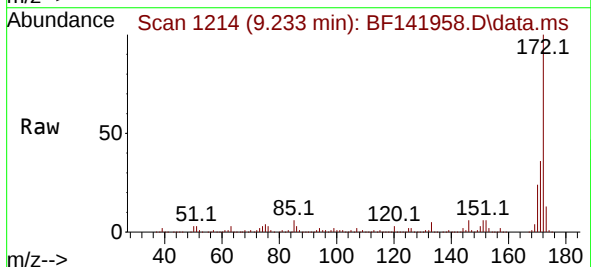




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF141958.D
Acq: 14 Mar 2025 11:39




Instrument :
BNA_F
ClientSampleId :
PB167123BL


Tgt Ion:188 Resp: 598649
Ion Ratio Lower Upper
188 100
94 7.9 6.8 10.2
80 8.9 7.6 11.4

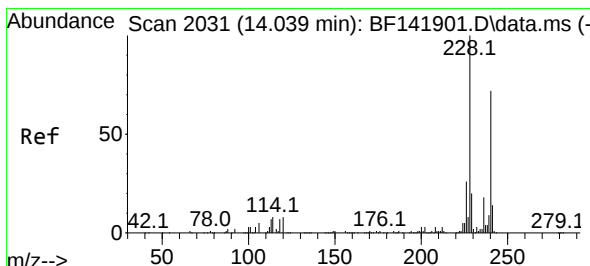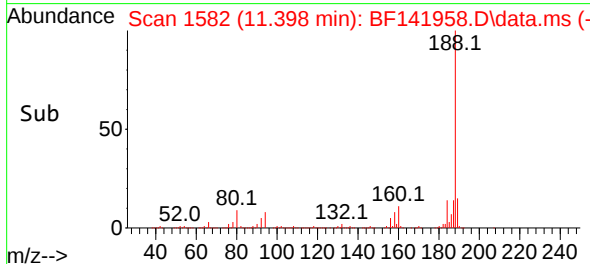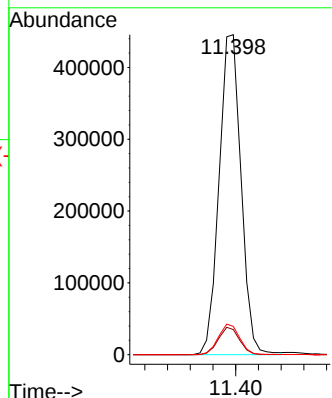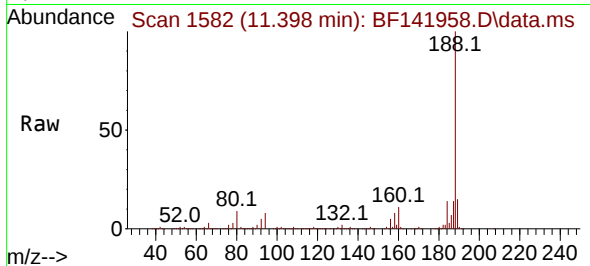

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.033 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BF141958.D
Acq: 14 Mar 2025 11:39


Tgt Ion:240 Resp: 348554
Ion Ratio Lower Upper
240 100
120 9.1 8.4 12.6
236 25.1 20.5 30.7

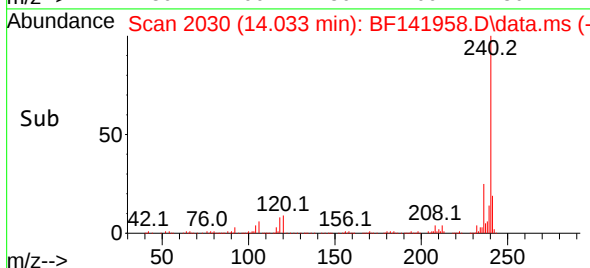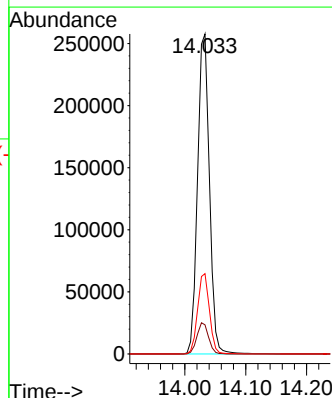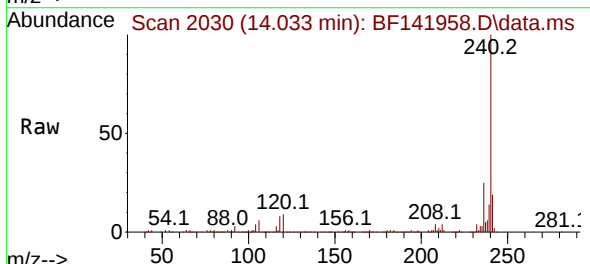



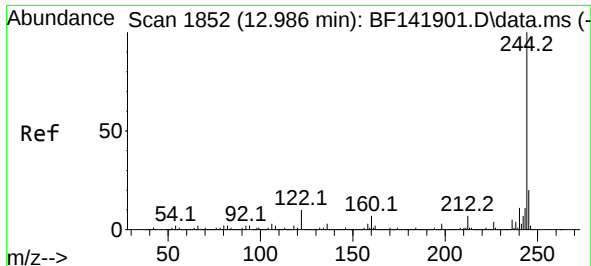


#79
 Terphenyl-d14
 Concen: 120.468 ng
 RT: 12.980 min Scan# 1851
 Delta R.T. -0.006 min
 Lab File: BF141958.D
 Acq: 14 Mar 2025 11:39

Instrument :
 BNA_F
 ClientSampleId :
 PB167123BL

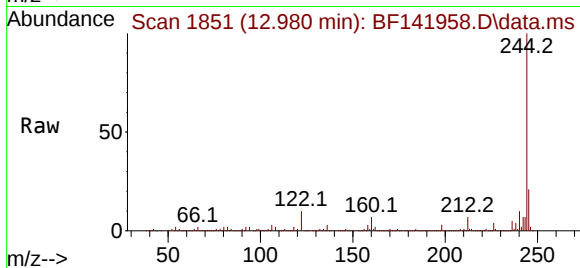

Tgt Ion:244 Resp: 2840101
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 9.6 7.7 11.5

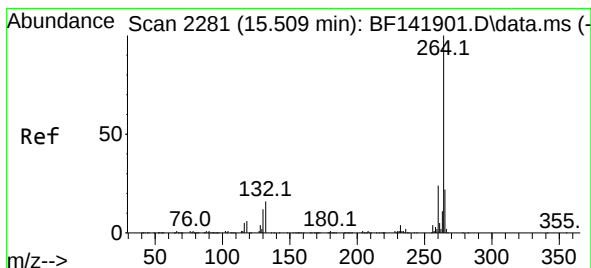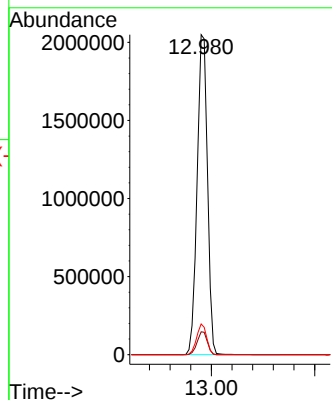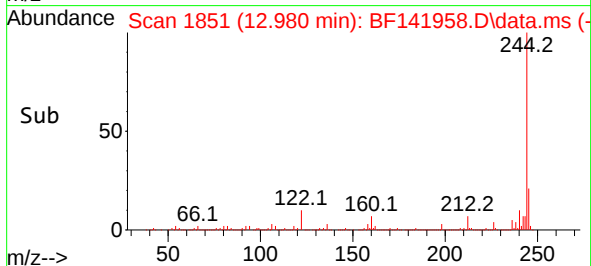

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.504 min Scan# 2280
 Delta R.T. -0.006 min
 Lab File: BF141958.D
 Acq: 14 Mar 2025 11:39

Tgt Ion:264 Resp: 326717
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.1 28.7
 265 21.5 17.5 26.3

