
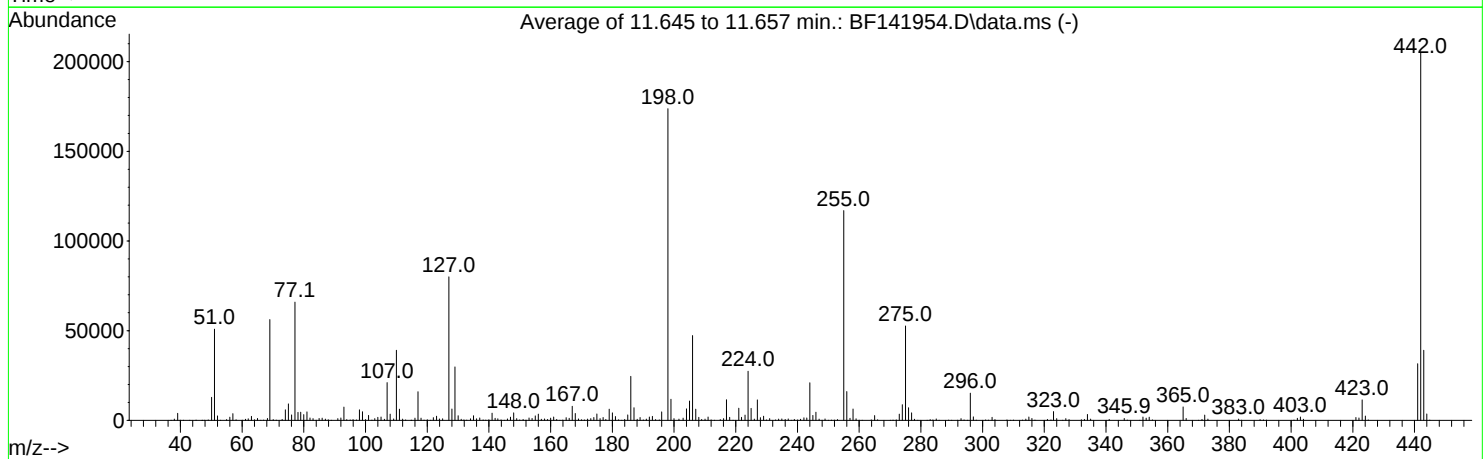


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031425\
Data File : BF141954.D
Acq On : 14 Mar 2025 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

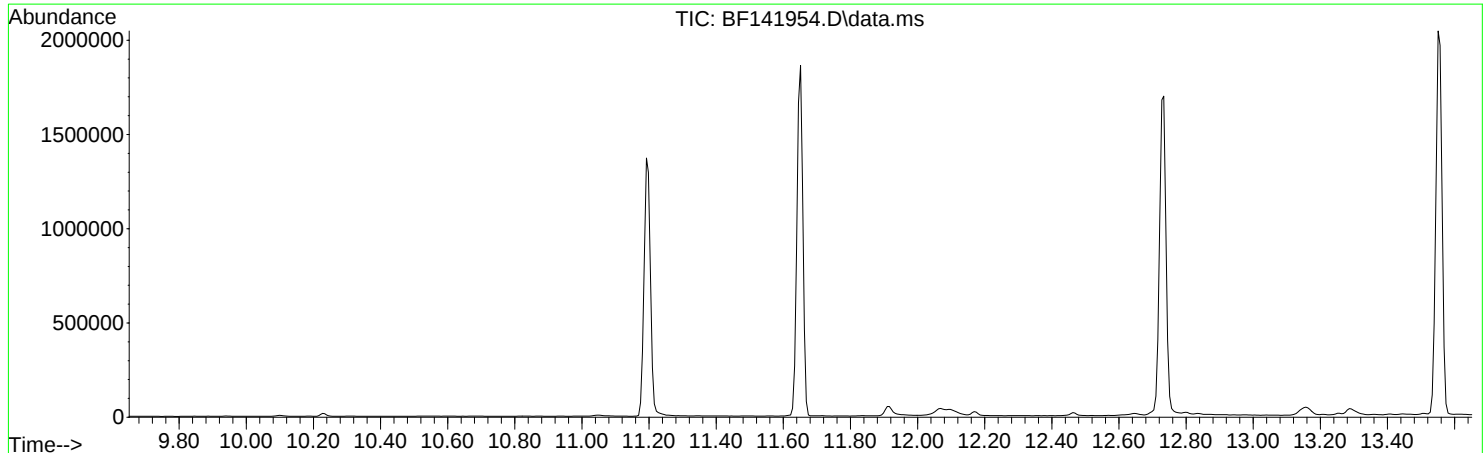

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	50899	PASS
68	69	0.00	2	2.0	1111	PASS
69	198	0.00	100	32.4	56244	PASS
70	69	0.00	2	0.8	424	PASS
127	198	10	80	46.0	80016	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	173803	PASS
199	198	5	9	6.8	11788	PASS
275	198	10	60	30.3	52683	PASS
365	198	1	100	4.3	7524	PASS
441	198	0.01	100	18.2	31589	PASS
442	442	50	100	100.0	205099	PASS
443	442	15	24	19.0	39064	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/14/2025	BNA_F	<u>BF141954.D</u>
Compound Name	Response	Retention Time
DDT	528547	13.557
DDD	7387	13.286
DDE	377	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7764	536311	1.45

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031425\  
Data File : BF141954.D  
Acq On    : 14 Mar 2025  09:08  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 14 11:49:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

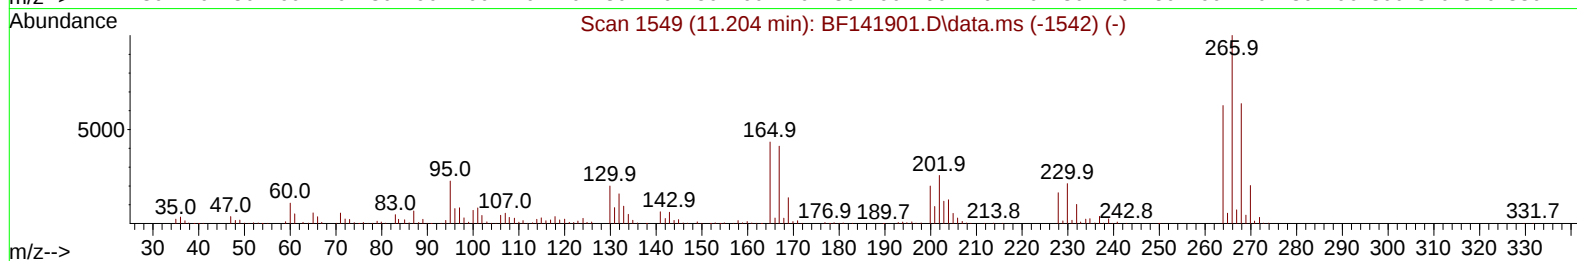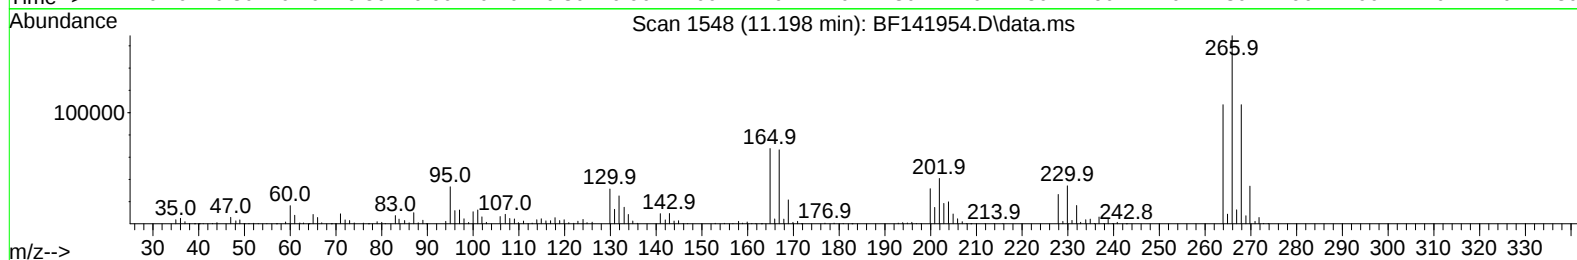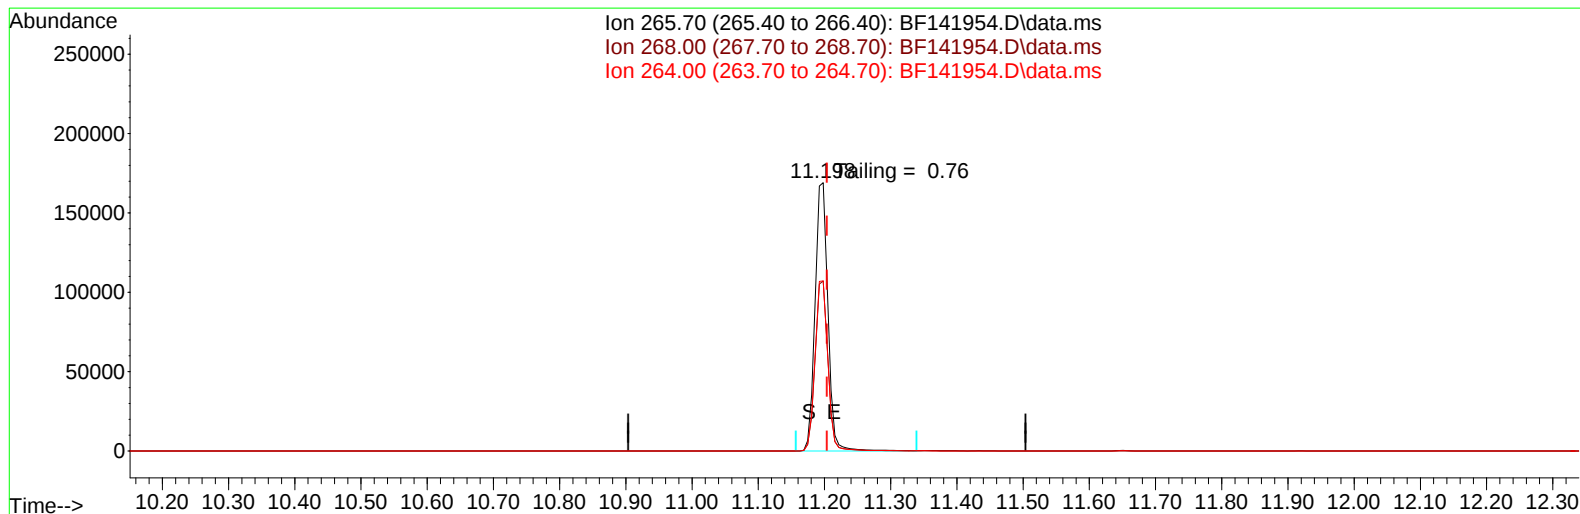

TIC: BF141954.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 97299.40 ng




response **229558**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.38
264.00	62.70	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031425\
Data File : BF141954.D
Acq On : 14 Mar 2025 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 14 11:49:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

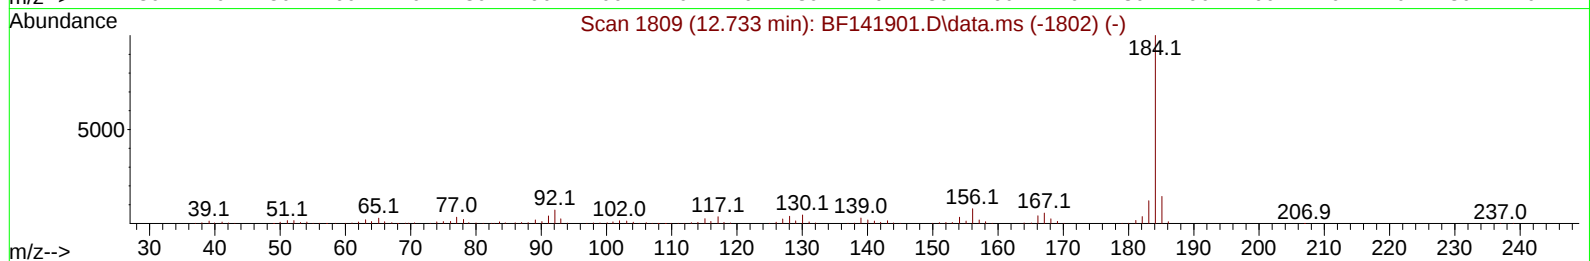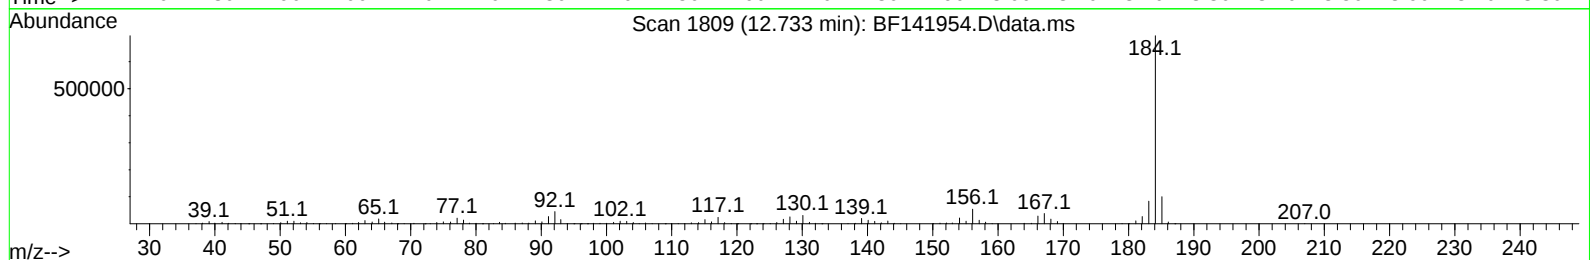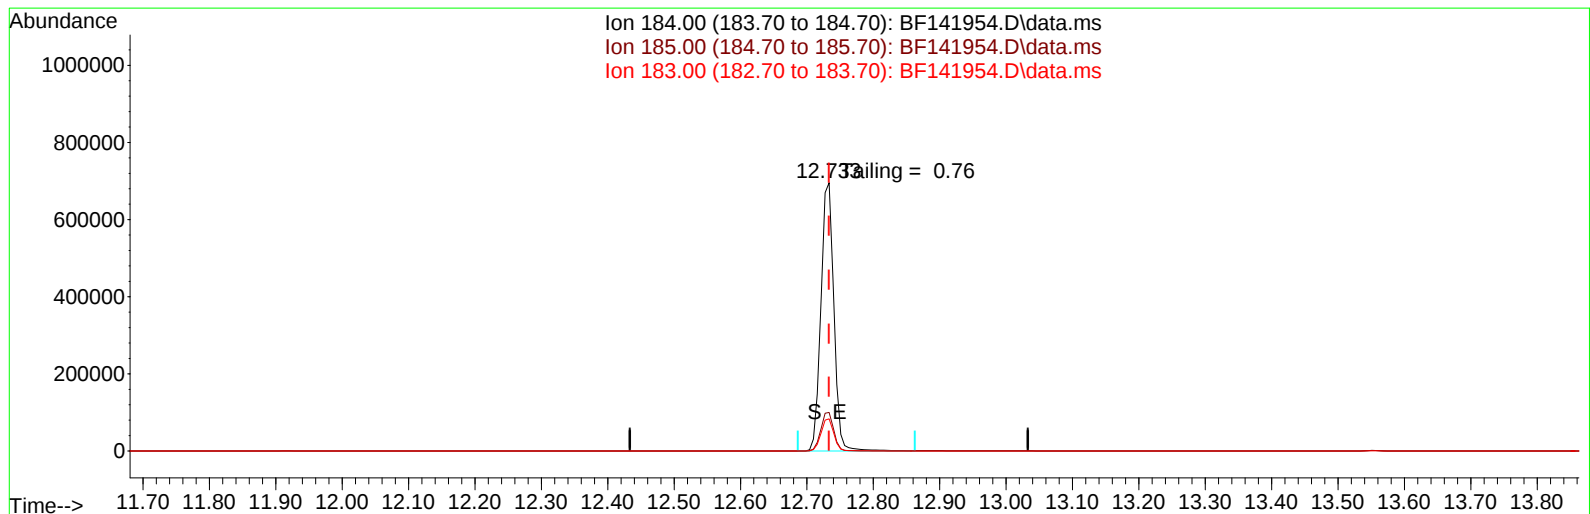

TIC: BF141954.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 228340.27 ng

response 946176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	12.10	11.99
0.00	0.00	0.00