
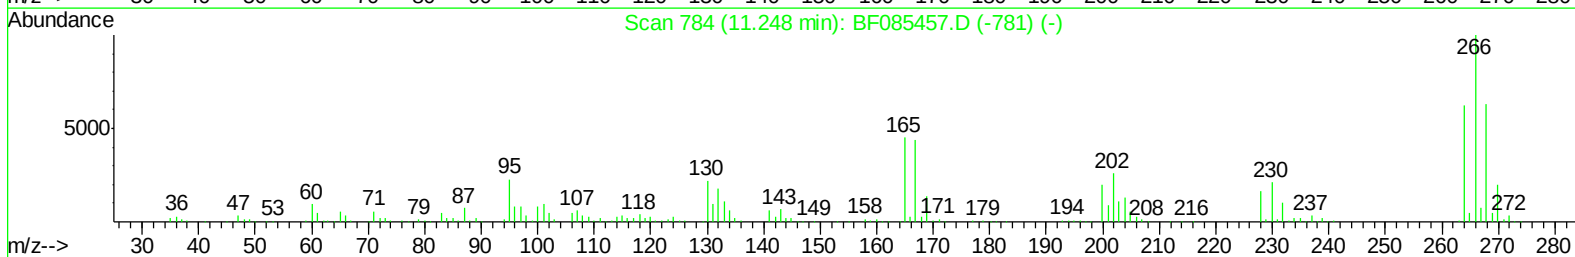
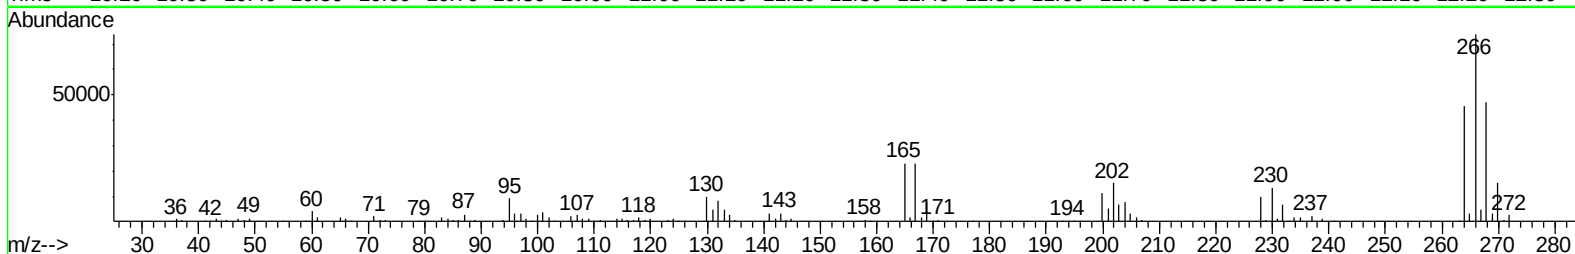


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031516\
Data File : BF085452.D
Acq On : 15 Mar 2016 13:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 16 05:29:15 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

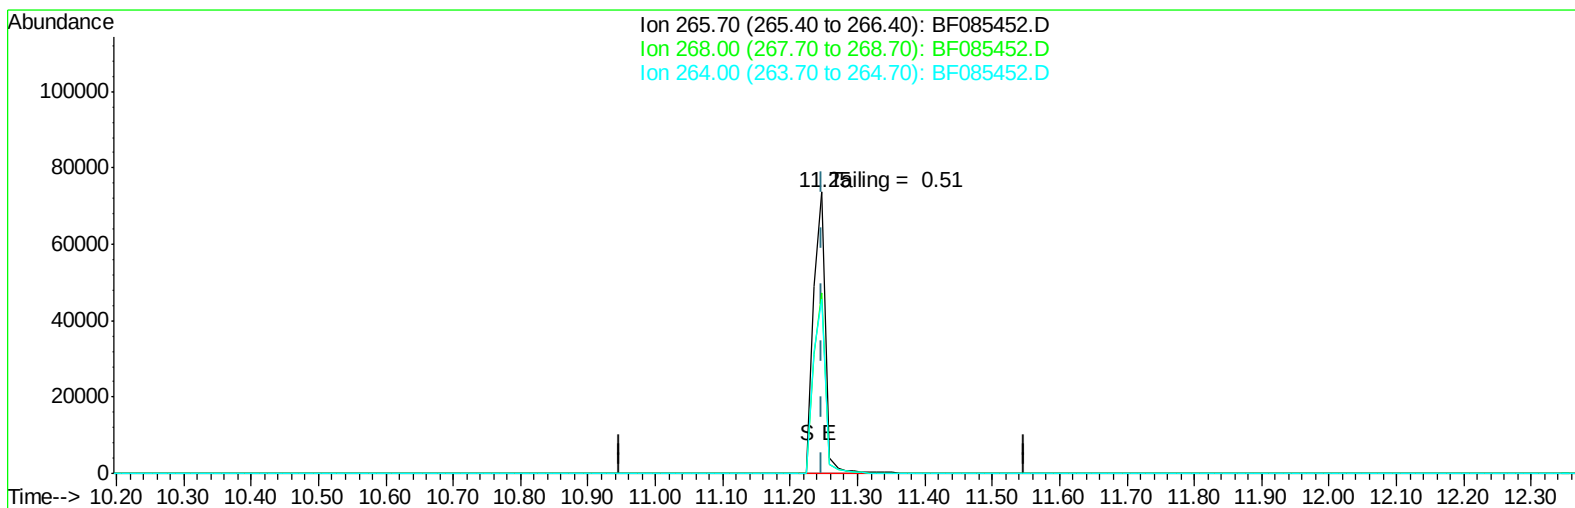

TIC: BF085452.D

(69) Pentachlorophenol (C)

11.248min (-0.000) 0.00ng




response 90081

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	63.97
264.00	64.30	61.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031516\
Data File : BF085452.D
Acq On : 15 Mar 2016 13:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 16 05:29:15 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

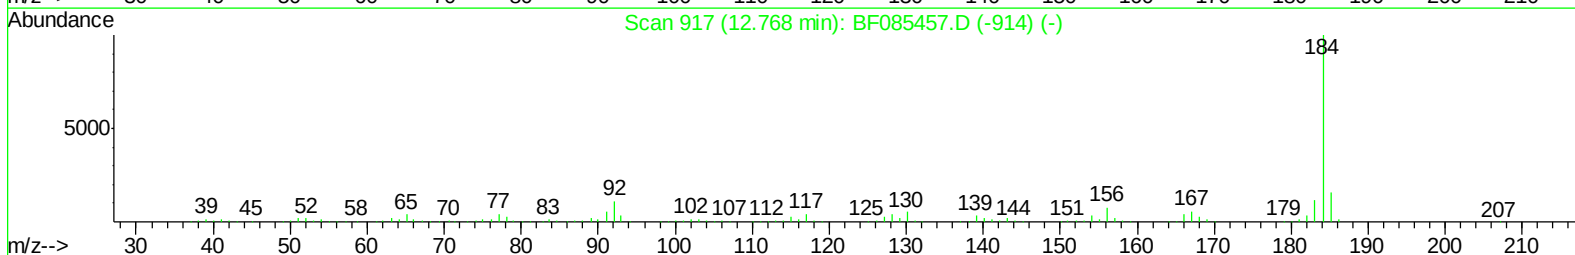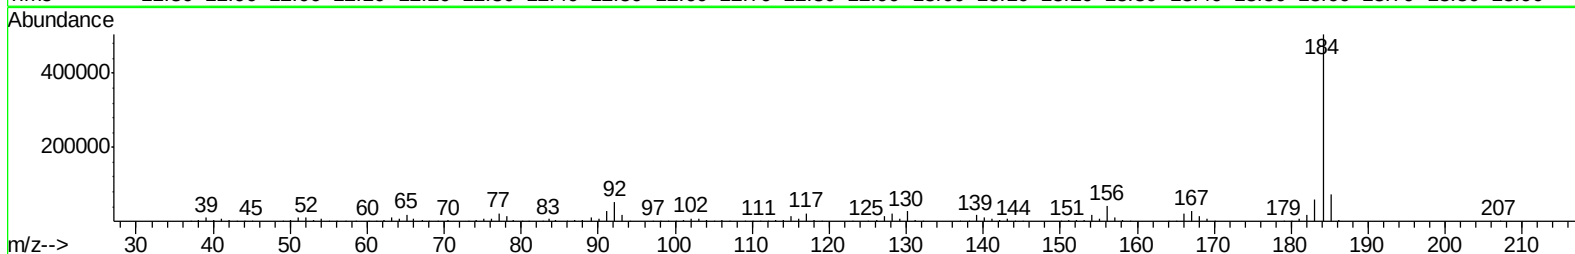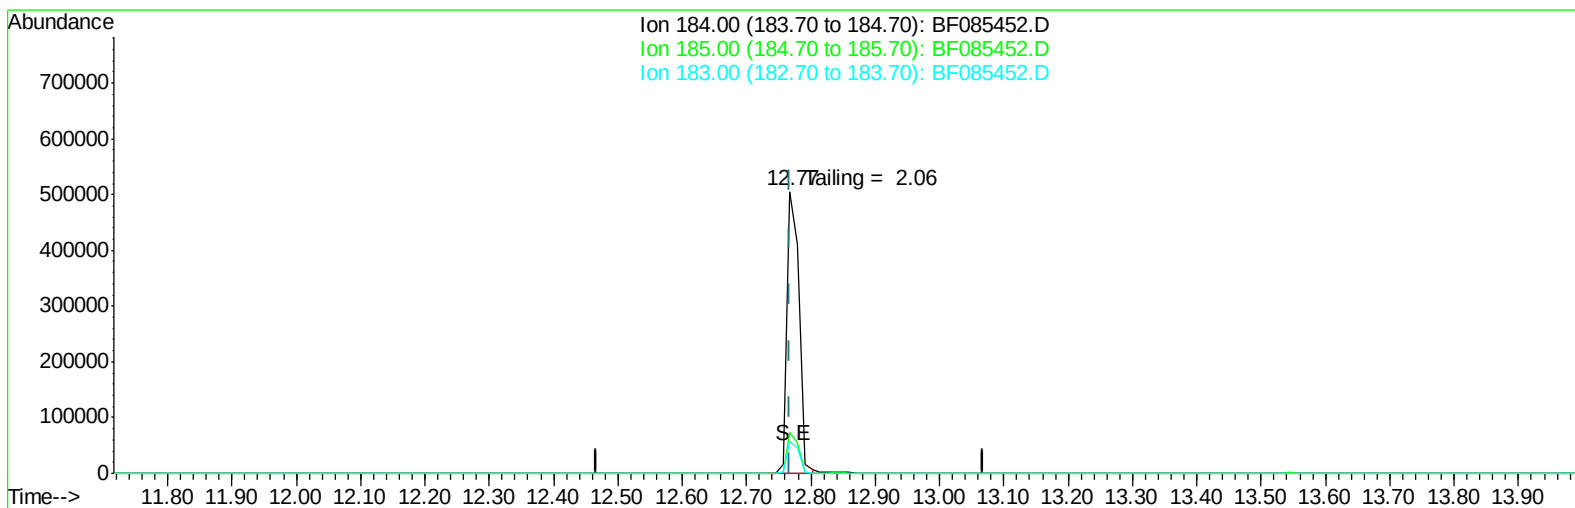

TIC: BF085452.D

(76) Benzidine

12.768min (-0.000) 88289.90ng




response 666402

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.55
183.00	11.80	11.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031516\
Data File : BF085452.D
Acq On : 15 Mar 2016 13:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 16 05:33:24 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

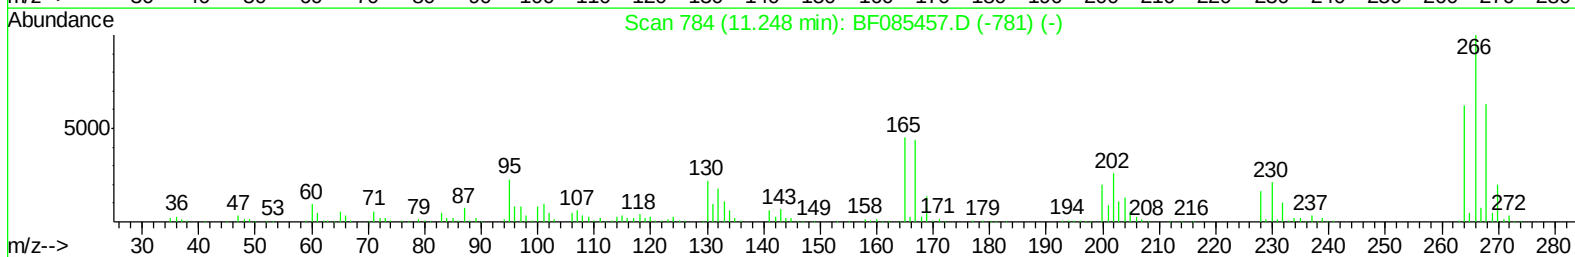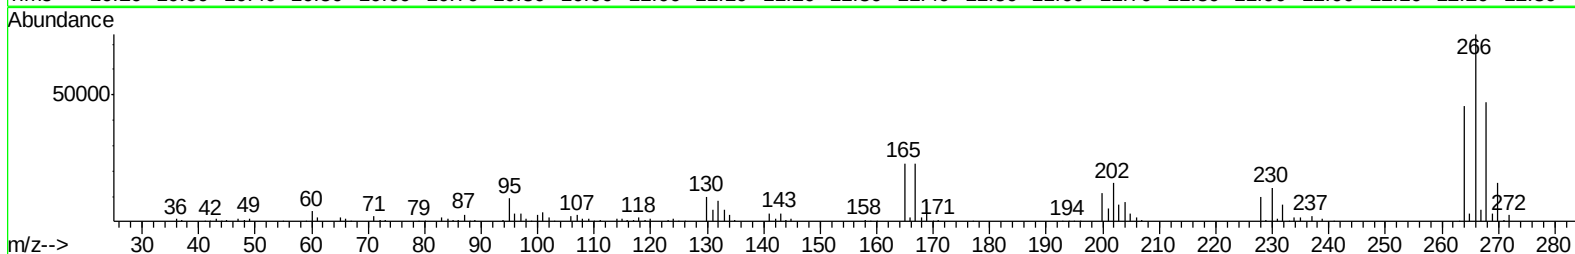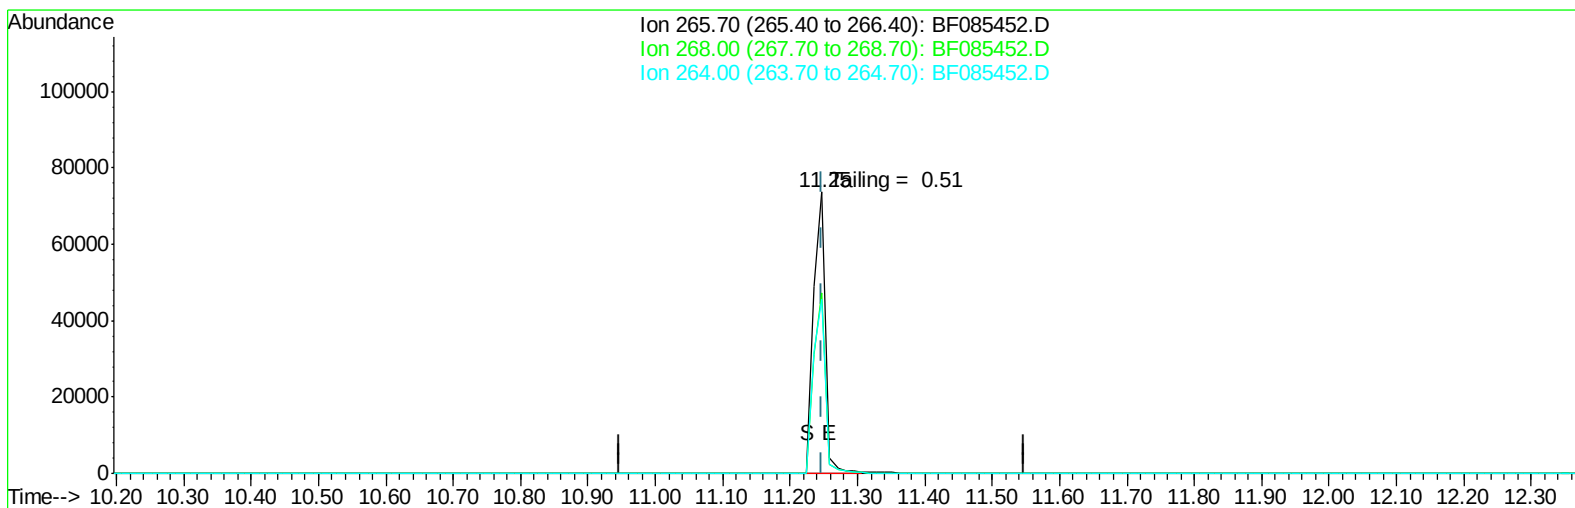

TIC: BF085452.D

(69) Pentachlorophenol (C)

11.248min (-0.000) 0.00ng




response 90081

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	63.97
264.00	64.30	61.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031516\
Data File : BF085452.D
Acq On : 15 Mar 2016 13:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 16 05:33:24 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

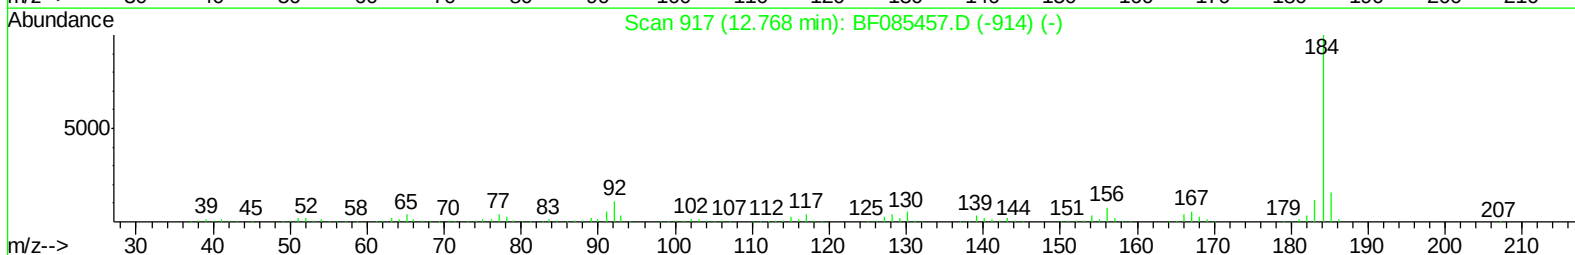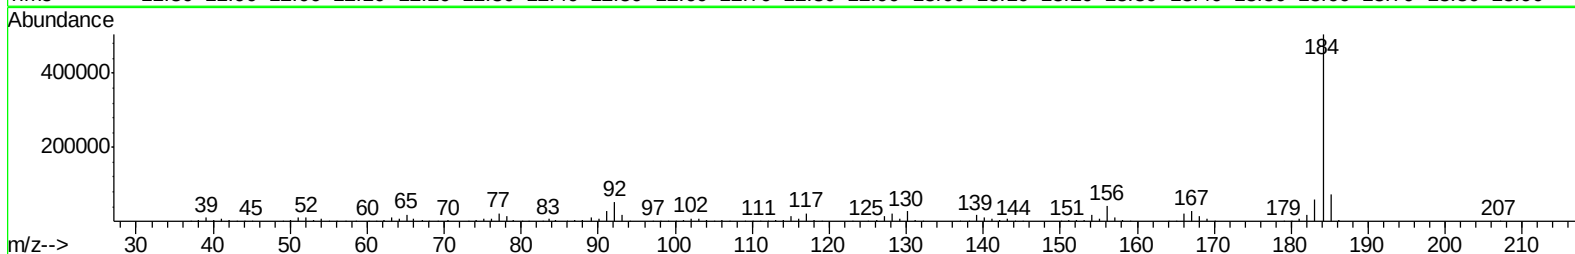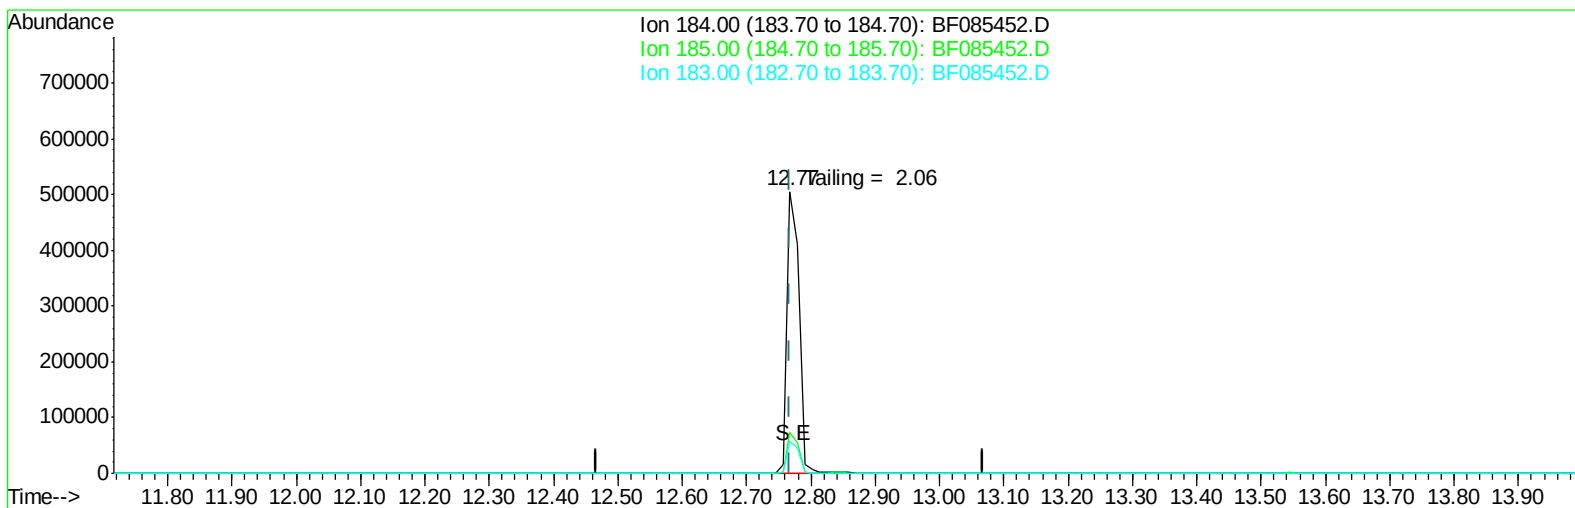

TIC: BF085452.D

(76) Benzidine

12.768min (-0.000) 88289.90ng

response 666402

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.55
183.00	11.80	11.56
0.00	0.00	0.00