


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031516\
Data File : BF085452.D
Acq On : 15 Mar 2016 13:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 15 18:57:05 2016

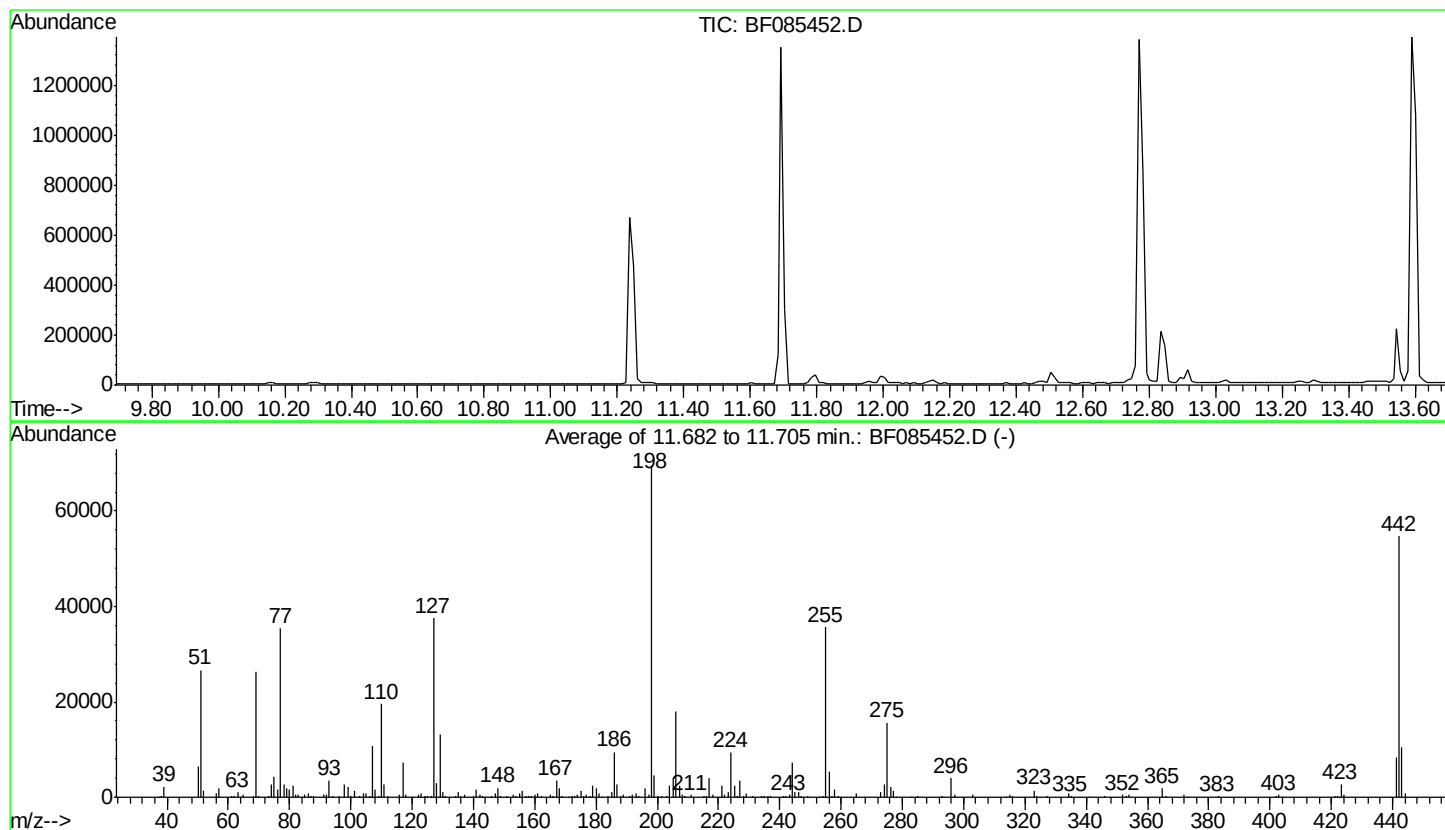

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	26673	PASS
68	69	0.00	2	1.4	366	PASS
69	198	0.00	100	37.8	26303	PASS
70	69	0.00	2	0.6	161	PASS
127	198	10	80	53.9	37462	PASS
197	198	0.00	2	0.7	479	PASS
198	198	100	100	100.0	69522	PASS
199	198	5	9	6.5	4492	PASS
275	198	10	60	22.5	15656	PASS
365	198	1	100	2.7	1862	PASS
441	442	0.01	24	15.0	8212	PASS
442	198	50	100	78.6	54653	PASS
443	442	15	24	19.0	10374	PASS