
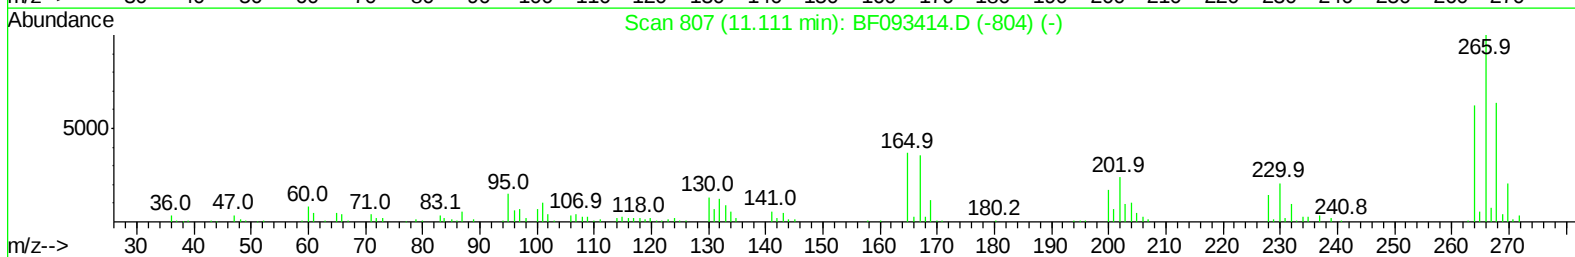
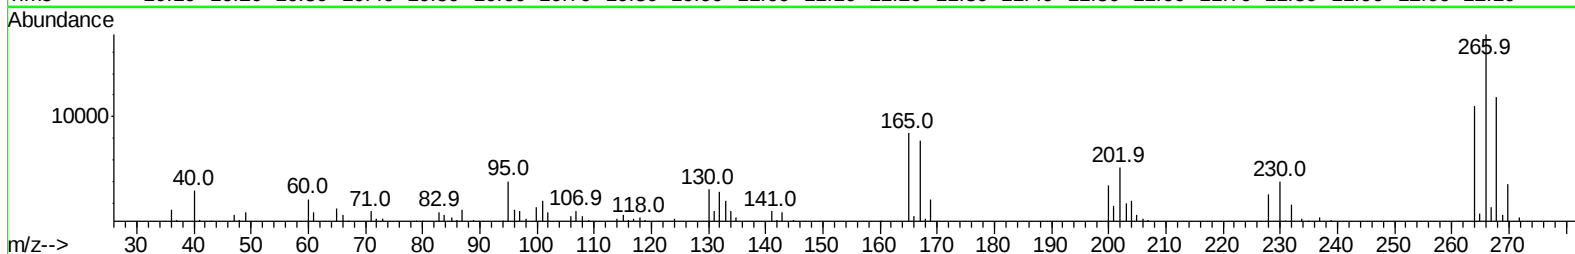


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031517\
Data File : BF093690.D
Acq On : 16 Mar 2017 3:45
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 07:30:05 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

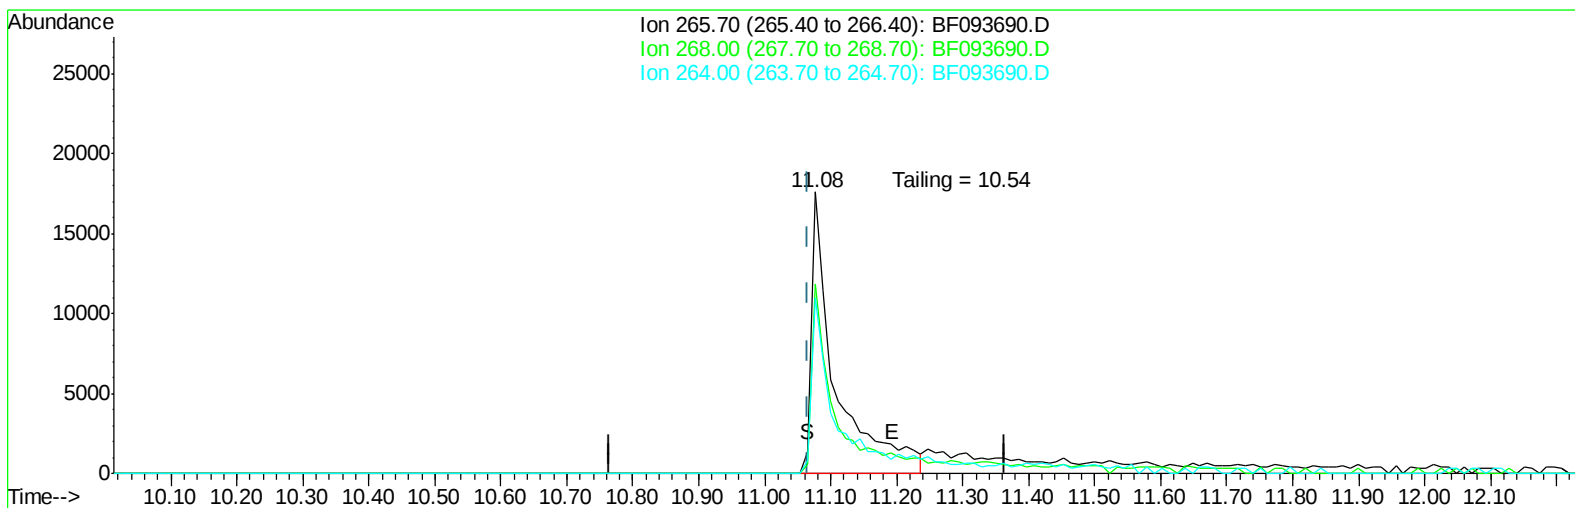

TIC: BF093690.D

(69) Pentachlorophenol (C)




11.076min (+0.011) 0.00ng

response 44453

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.25
264.00	62.90	62.44
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031517\
Data File : BF093690.D
Acq On : 16 Mar 2017 3:45
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 07:30:05 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 13 15:05:08 2017
Response via : Initial Calibration

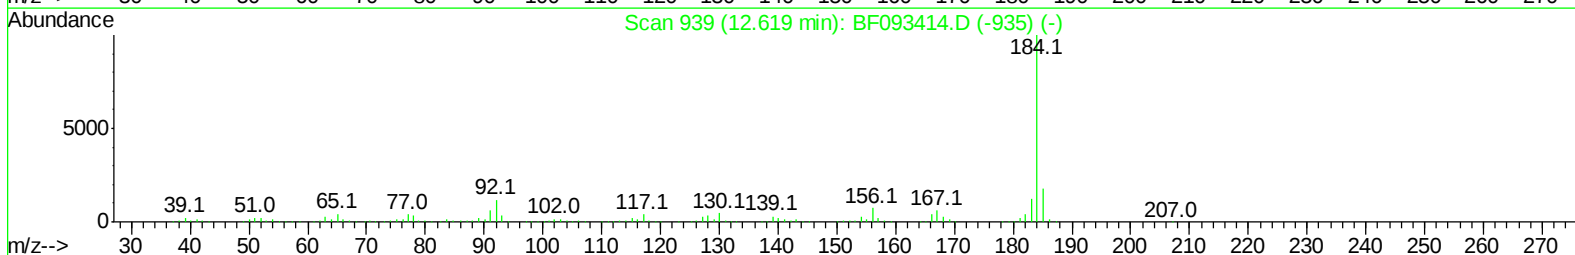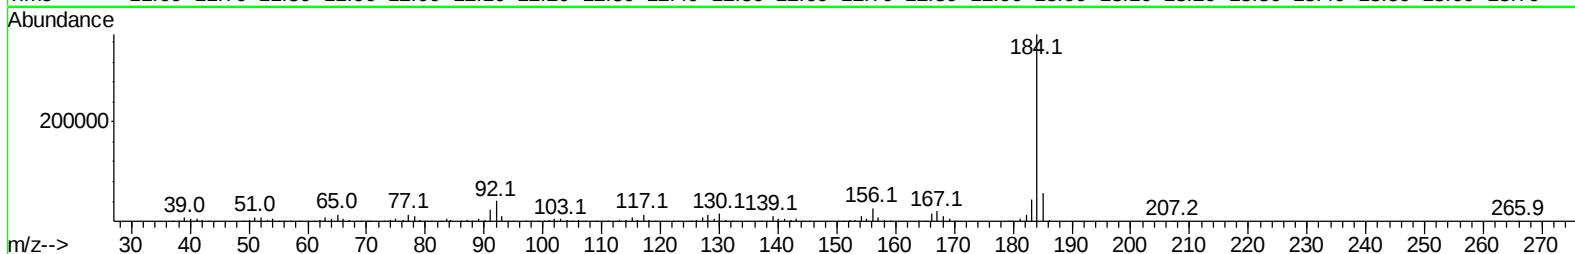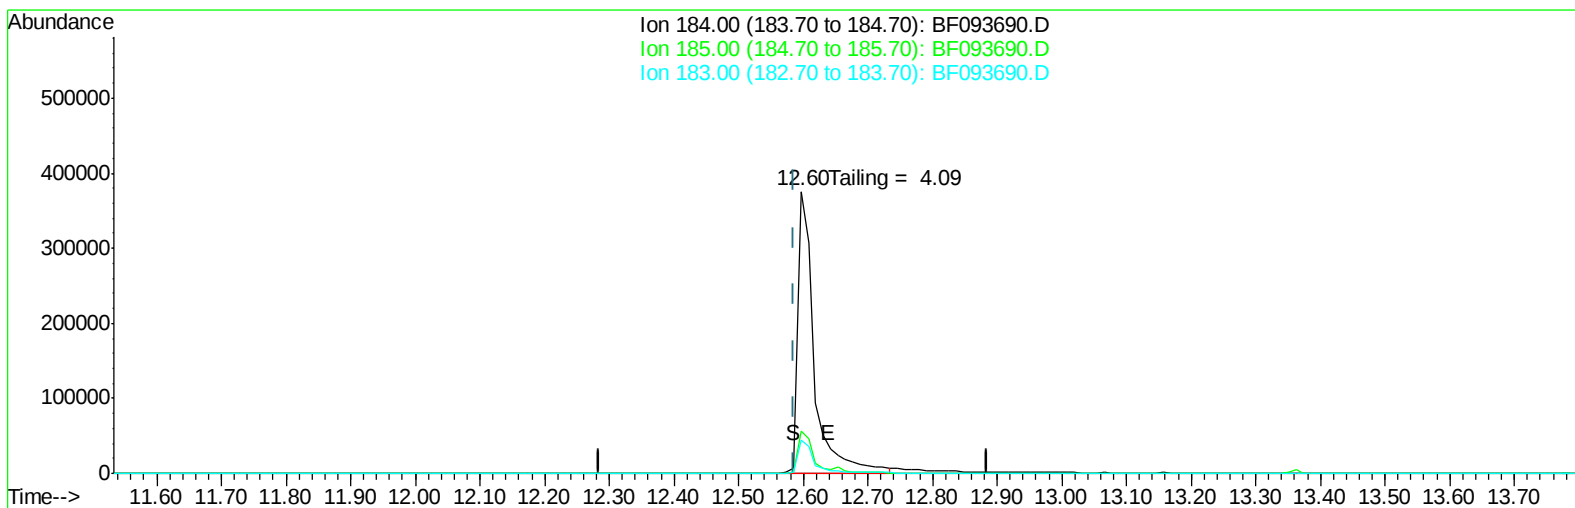

TIC: BF093690.D

(76) Benzidine

12.597min (+0.011) 0.00ng

response 687377

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.15
183.00	11.50	12.06
0.00	0.00	0.00