

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031517\
 Data File : BF093666.D
 Acq On : 15 Mar 2017 14:30
 Operator : SJ/MA
 Sample : PB97589BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB97589BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.881	260	262	276	rBV	214019	607385	11.13%	1.401%
2	5.304	297	299	325	rBV	3729440	5458673	100.00%	12.589%
3	6.367	390	392	400	rBV	4015257	5018884	91.94%	11.575%
4	6.481	400	402	405	rVB	4481231	4777737	87.53%	11.018%
5	6.710	420	422	433	rVB	929784	1057984	19.38%	2.440%
6	6.859	433	435	447	rBV	3633040	3728438	68.30%	8.599%
7	7.282	470	472	490	rBV	2639945	3364193	61.63%	7.759%
8	8.002	532	535	548	rBV	1310899	1436495	26.32%	3.313%
9	9.076	627	629	632	rBV	3990839	4959510	90.86%	11.438%
10	9.762	687	689	691	rBV	1209623	1541943	28.25%	3.556%
11	10.550	756	758	775	rBV	2140673	2758476	50.53%	6.362%
12	11.248	817	819	830	rBV	1582625	1578199	28.91%	3.640%
13	12.836	955	958	960	rBV	4277339	4693971	85.99%	10.825%
14	13.888	1048	1050	1061	rBV	955133	1231055	22.55%	2.839%
15	15.294	1170	1173	1184	rBV	510813	874297	16.02%	2.016%
16	15.660	1202	1205	1212	rVB	44665	73727	1.35%	0.170%
17	16.105	1241	1244	1249	rBV	43256	73339	1.34%	0.169%
18	16.620	1285	1289	1295	rBV	27584	58760	1.08%	0.136%
19	17.225	1337	1342	1349	rBV4	22855	68100	1.25%	0.157%


Sum of corrected areas: 43361166

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031517\
Data File : BF093666.D
Acq On : 15 Mar 2017 14:30
Operator : SJ/MA
Sample : PB97589BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB97589BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

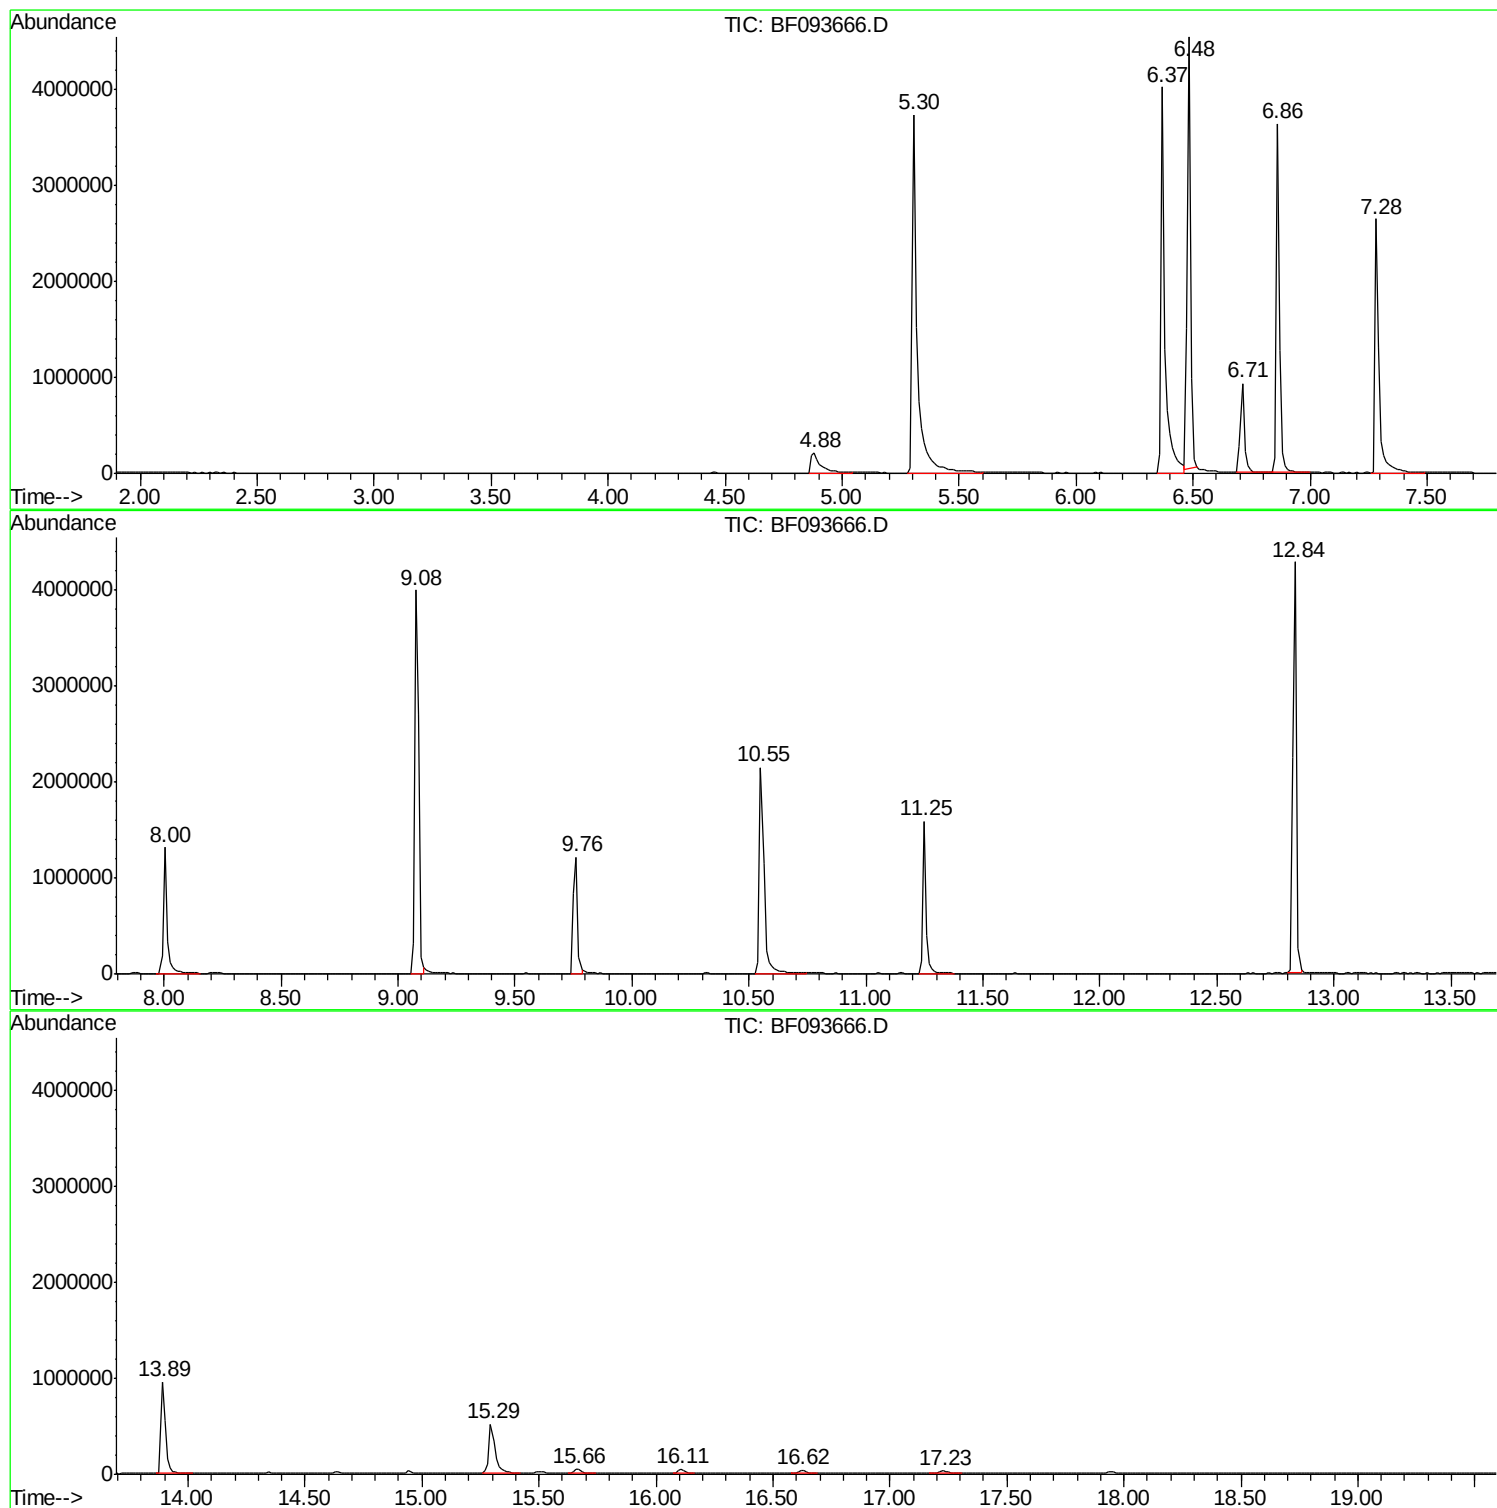

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031517\
Data File : BF093666.D
Acq On : 15 Mar 2017 14:30
Operator : SJ/MA
Sample : PB97589BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB97589BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.88	11.48 ng	607385	1,4-Dichlorobenzene-d4	6.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		Propane, 2-methyl-2-(1-methylethoxy)-	116	C7H16O	017348-59-3	42
3		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
4		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
5		Acetic acid, cyano-, 1,1-dimethyl-	141	C7H11NO2	001116-98-9	23

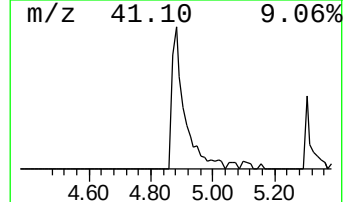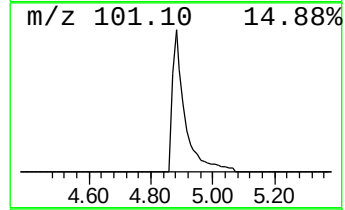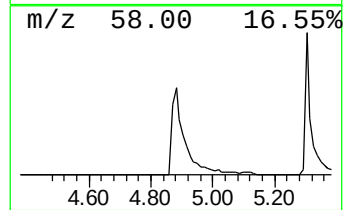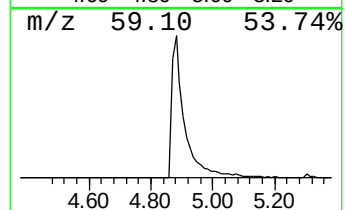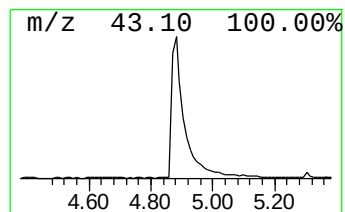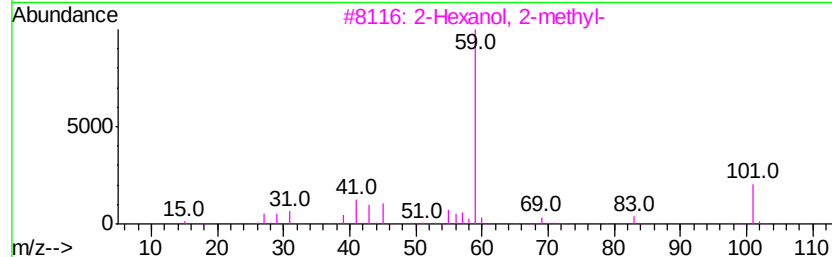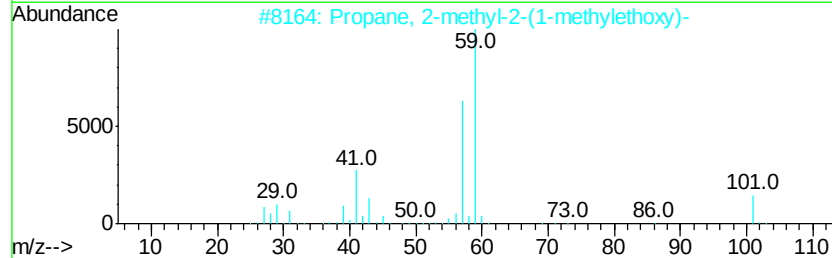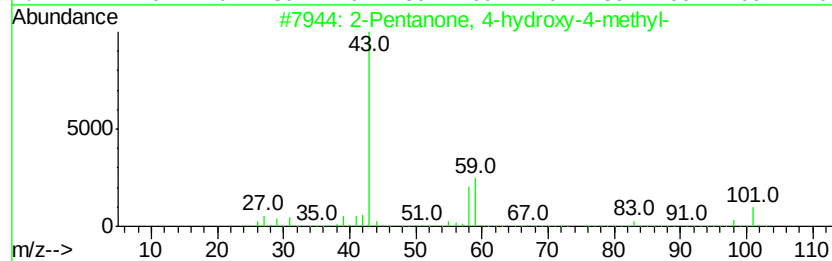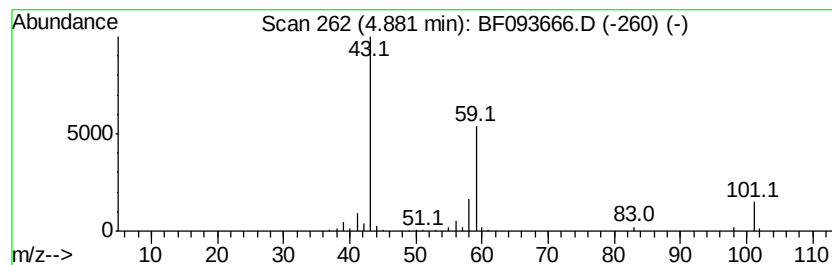

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031517\
Data File : BF093666.D
Acq On : 15 Mar 2017 14:30
Operator : SJ/MA
Sample : PB97589BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB97589BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	90.32 ng	4777740	1,4-Dichlorobenzene-d4	6.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

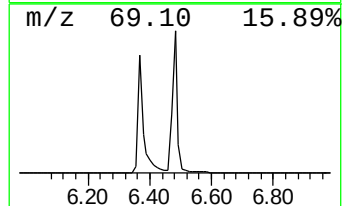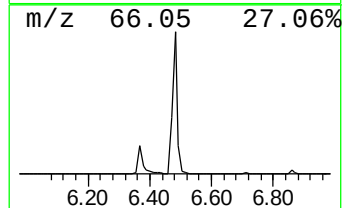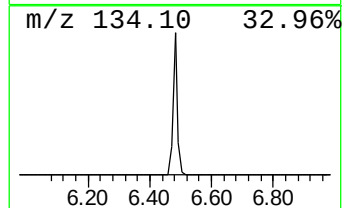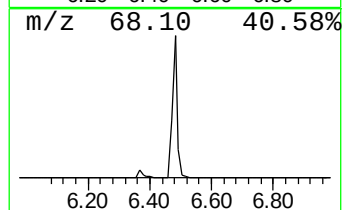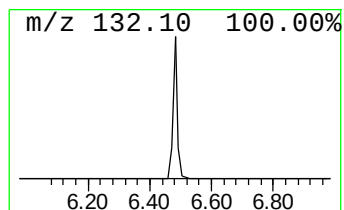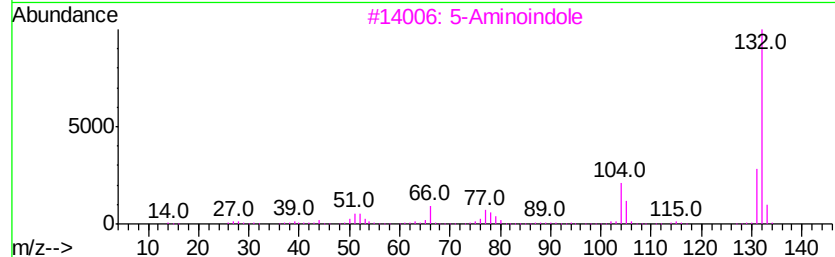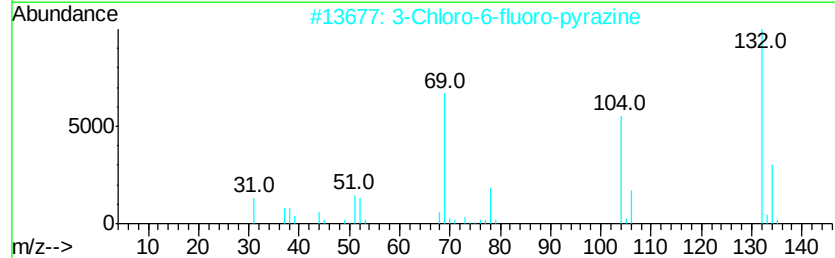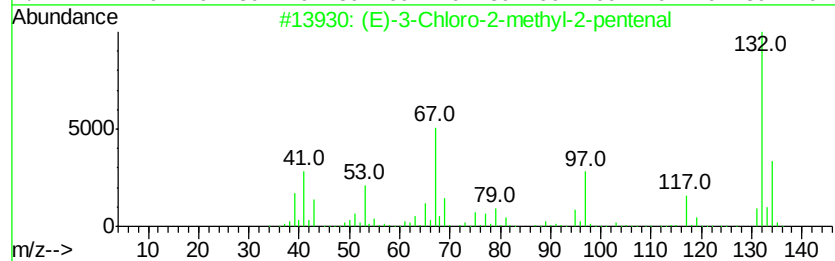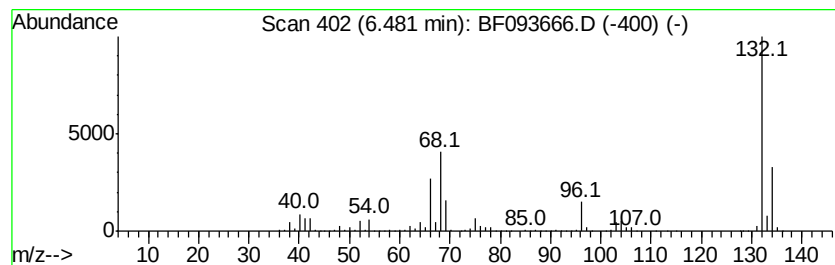

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031517\
Data File : BF093666.D
Acq On : 15 Mar 2017 14:30
Operator : SJ/MA
Sample : PB97589BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB97589BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.88	11.5	ng	607385	1	6.71	1057980	20.0
unknown6.48	6.48	90.3	ng	4777740	1	6.71	1057980	20.0