


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031517\
 Data File : BF093664.D
 Acq On : 15 Mar 2017 13:35
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

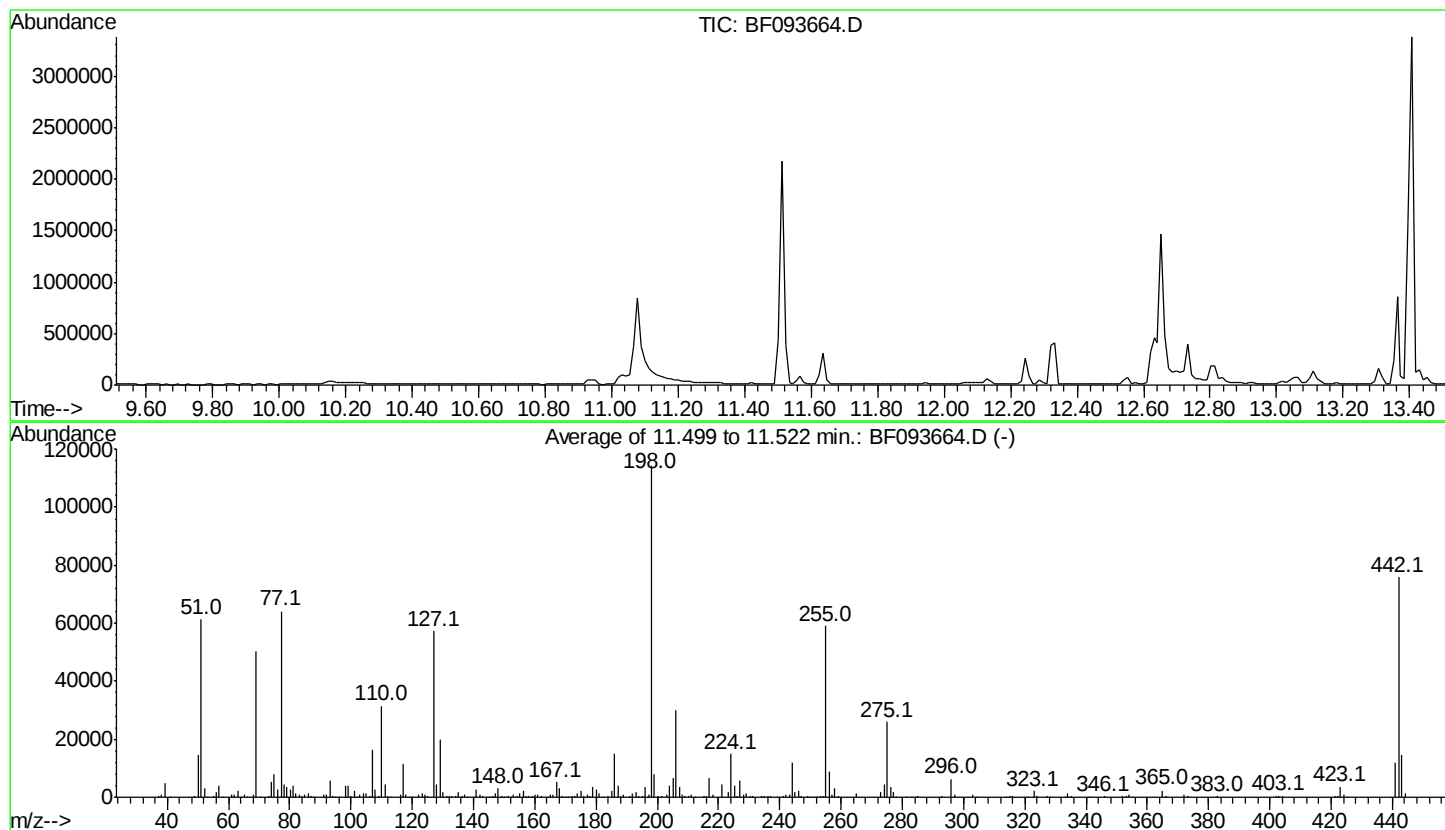

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	61281	PASS
68	69	0.00	2	1.9	941	PASS
69	198	0.00	100	44.0	50324	PASS
70	69	0.00	2	0.4	186	PASS
127	198	10	80	50.0	57214	PASS
197	198	0.00	2	0.9	1025	PASS
198	198	100	100	100.0	114346	PASS
199	198	5	9	6.9	7868	PASS
275	198	10	60	22.7	26005	PASS
365	198	1	100	2.1	2428	PASS
441	442	0.01	24	15.6	11828	PASS
442	198	50	100	66.3	75764	PASS
443	442	15	24	19.4	14701	PASS