


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031517\
 Data File : BF093690.D
 Acq On : 16 Mar 2017 3:45
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

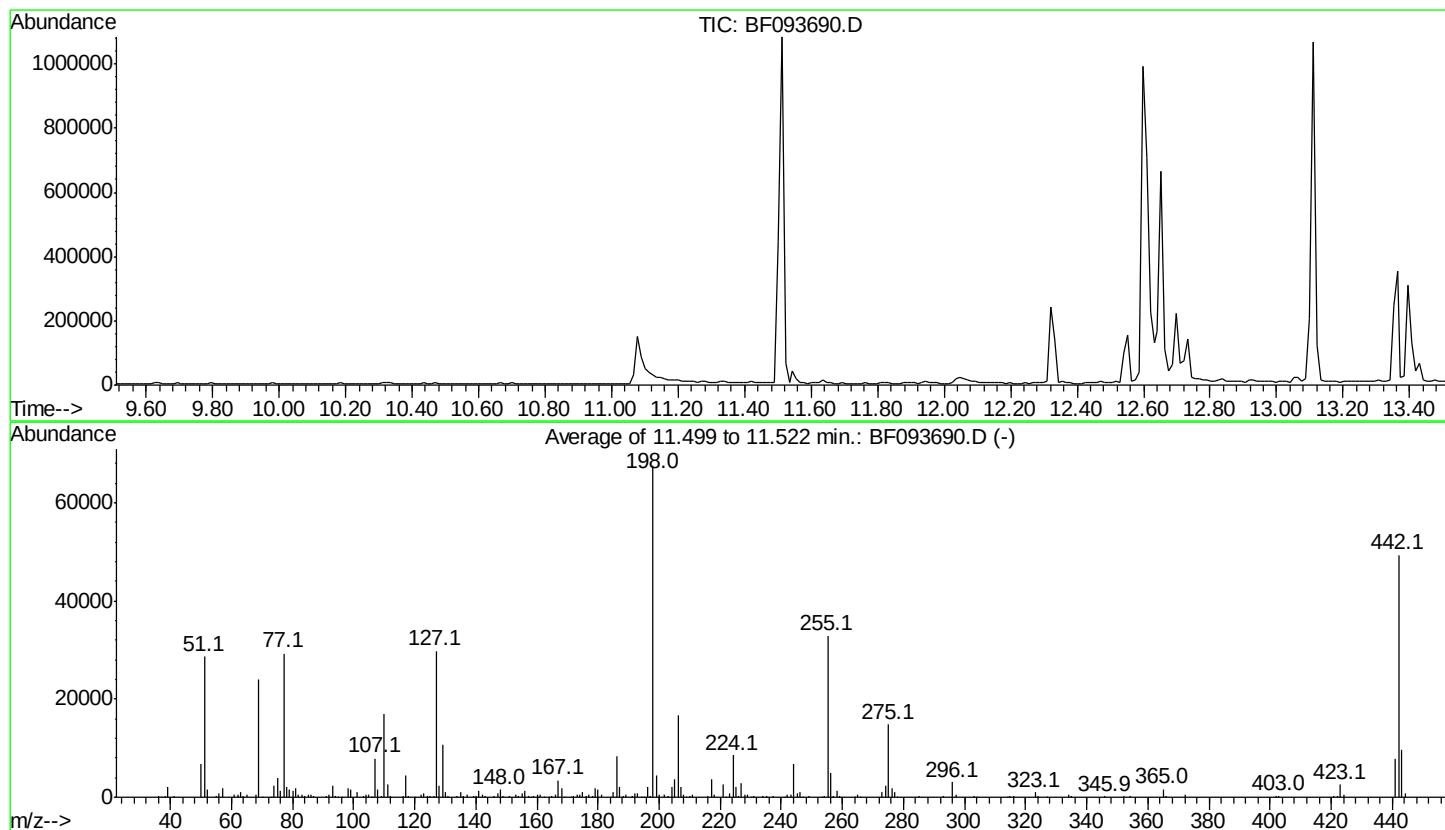

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	28650	PASS
68	69	0.00	2	1.9	447	PASS
69	198	0.00	100	35.6	24081	PASS
70	69	0.00	2	0.4	103	PASS
127	198	10	80	44.2	29846	PASS
197	198	0.00	2	0.3	206	PASS
198	198	100	100	100.0	67566	PASS
199	198	5	9	6.6	4485	PASS
275	198	10	60	21.8	14754	PASS
365	198	1	100	2.4	1608	PASS
441	442	0.01	24	15.7	7752	PASS
442	198	50	100	73.1	49377	PASS
443	442	15	24	19.8	9789	PASS