



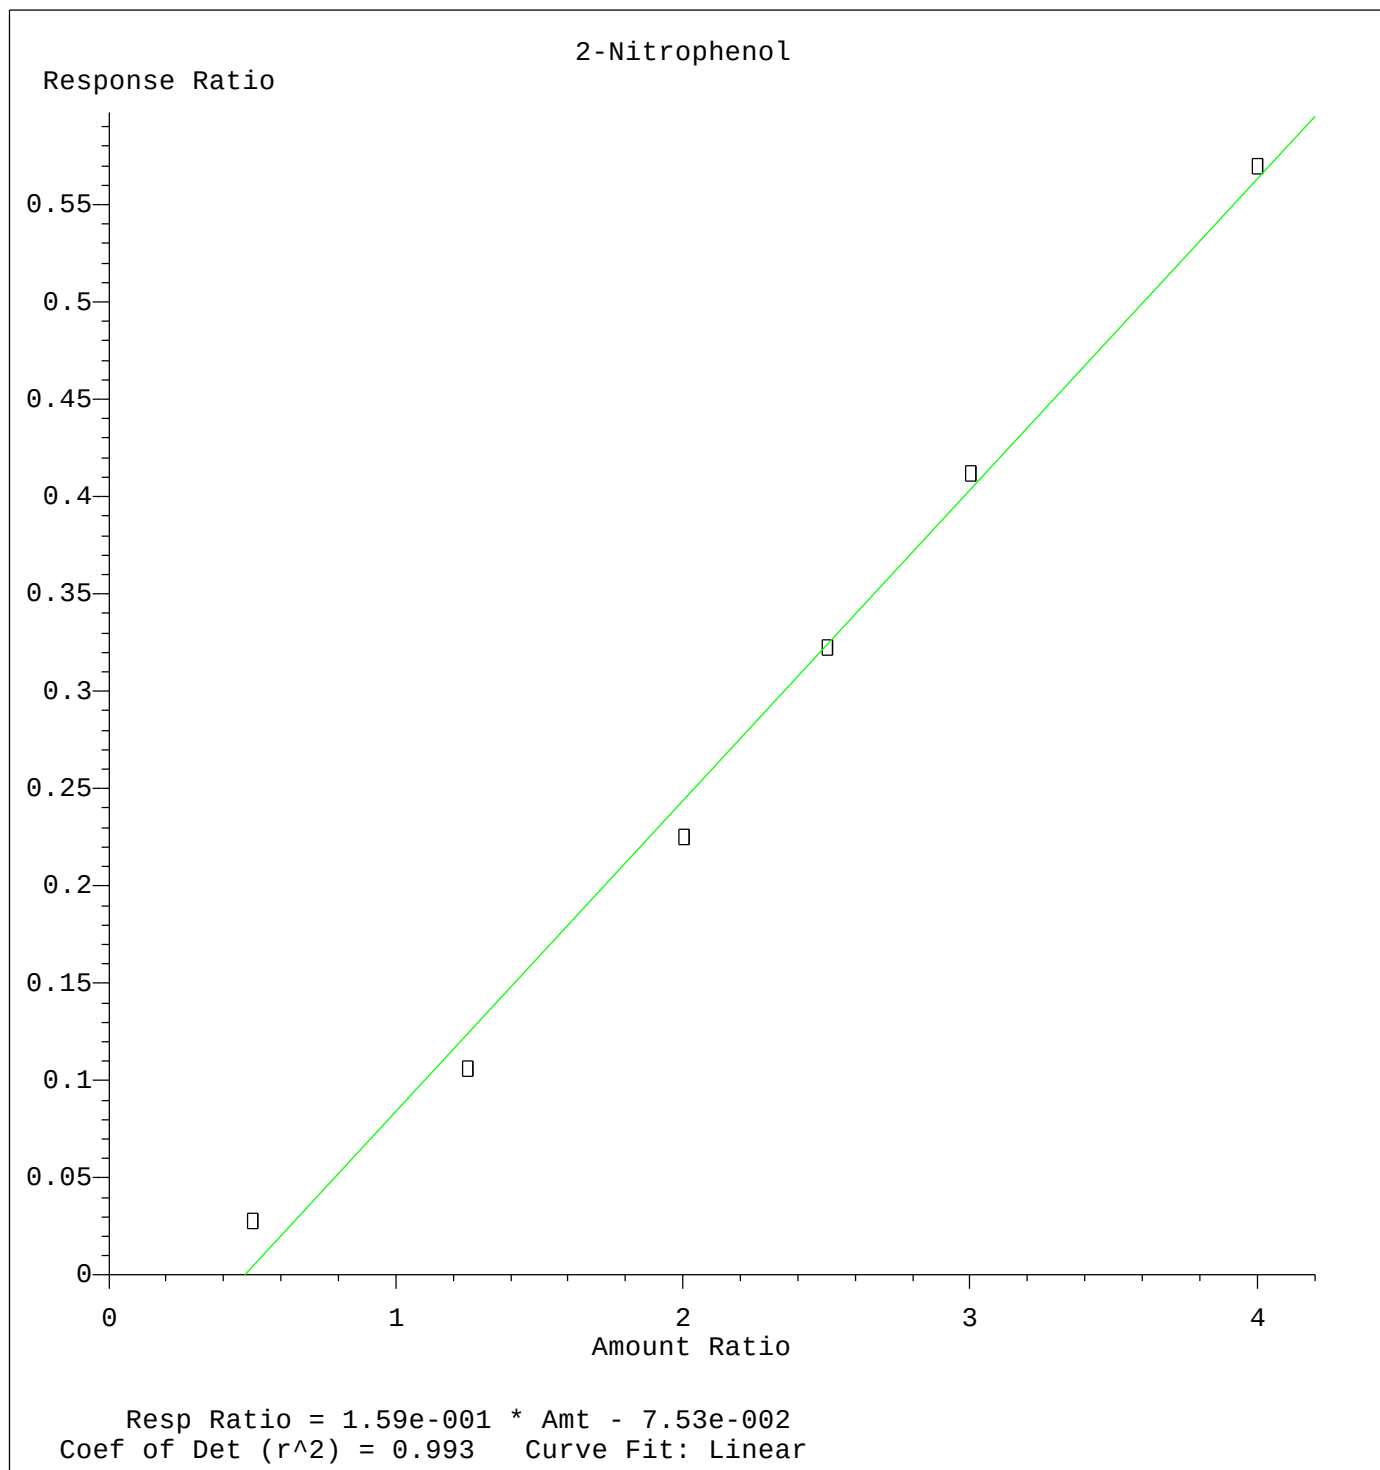


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018

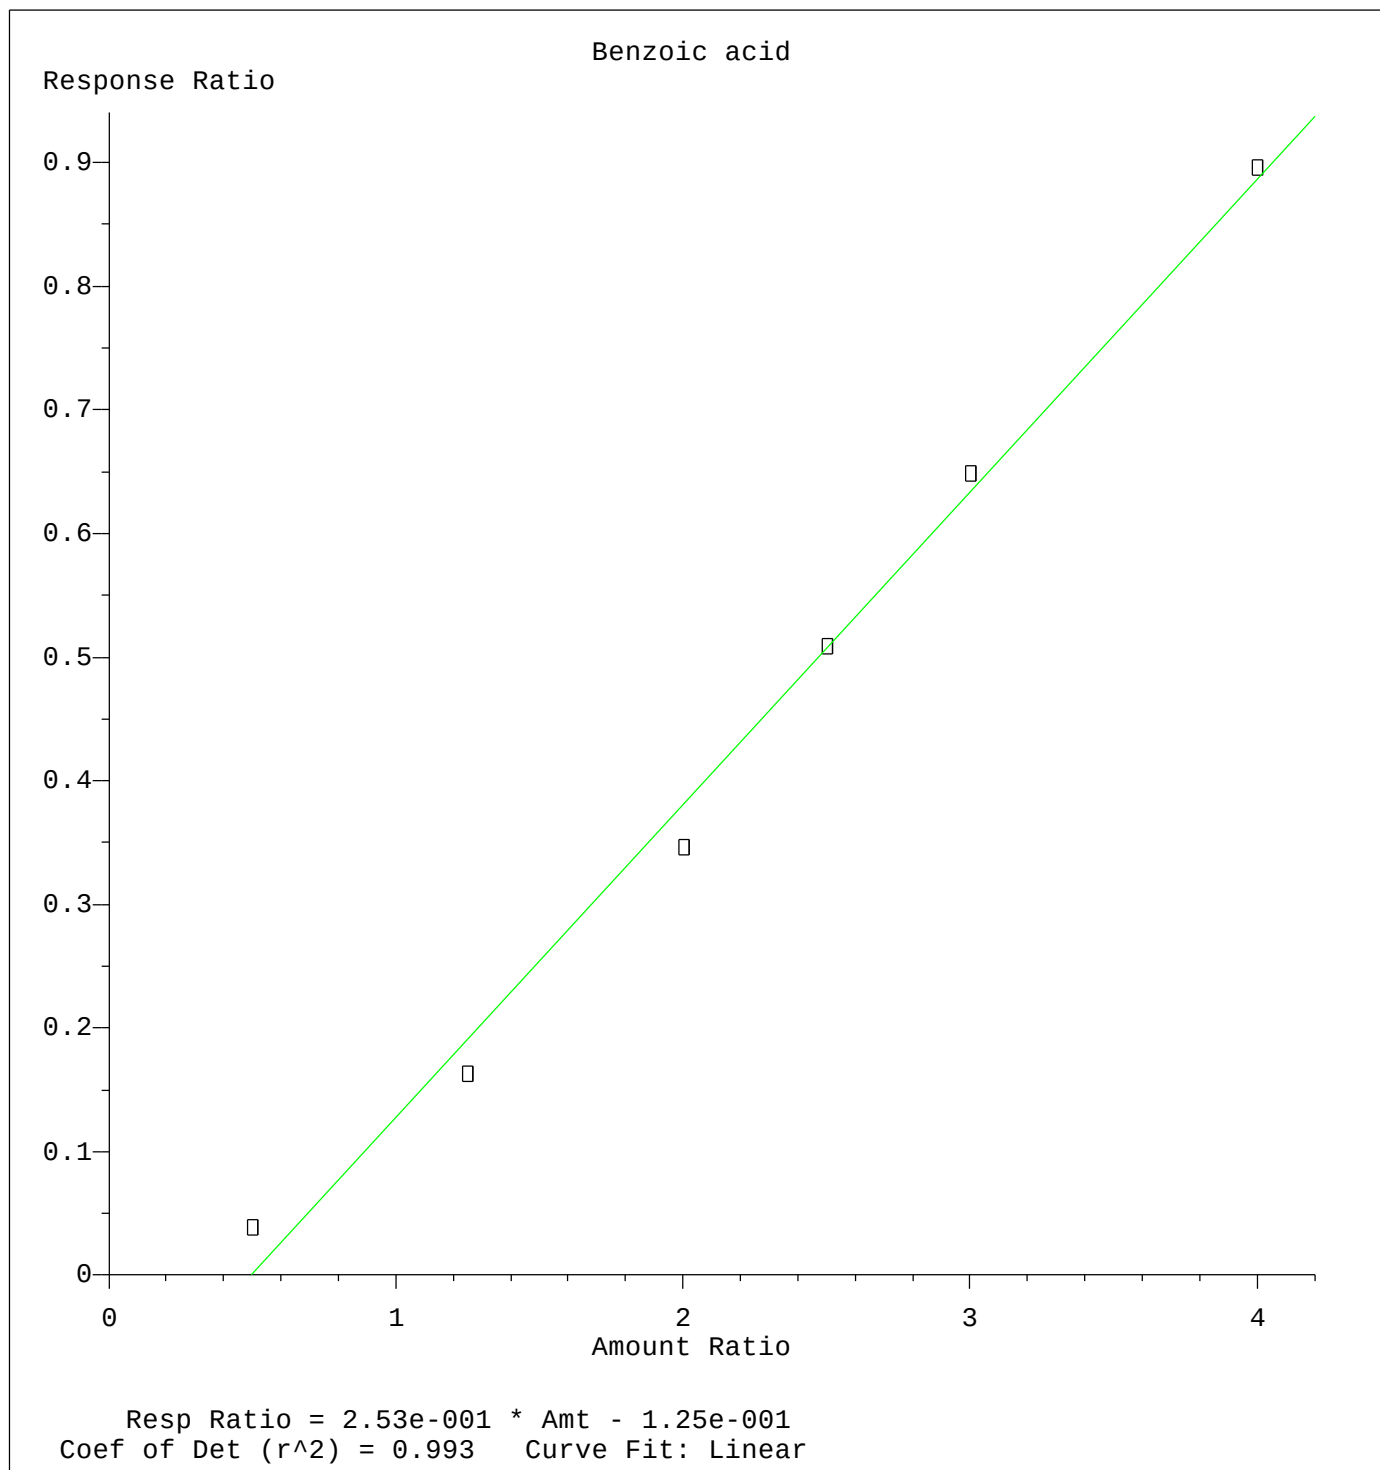

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018

2-Nitroaniline

Response Ratio

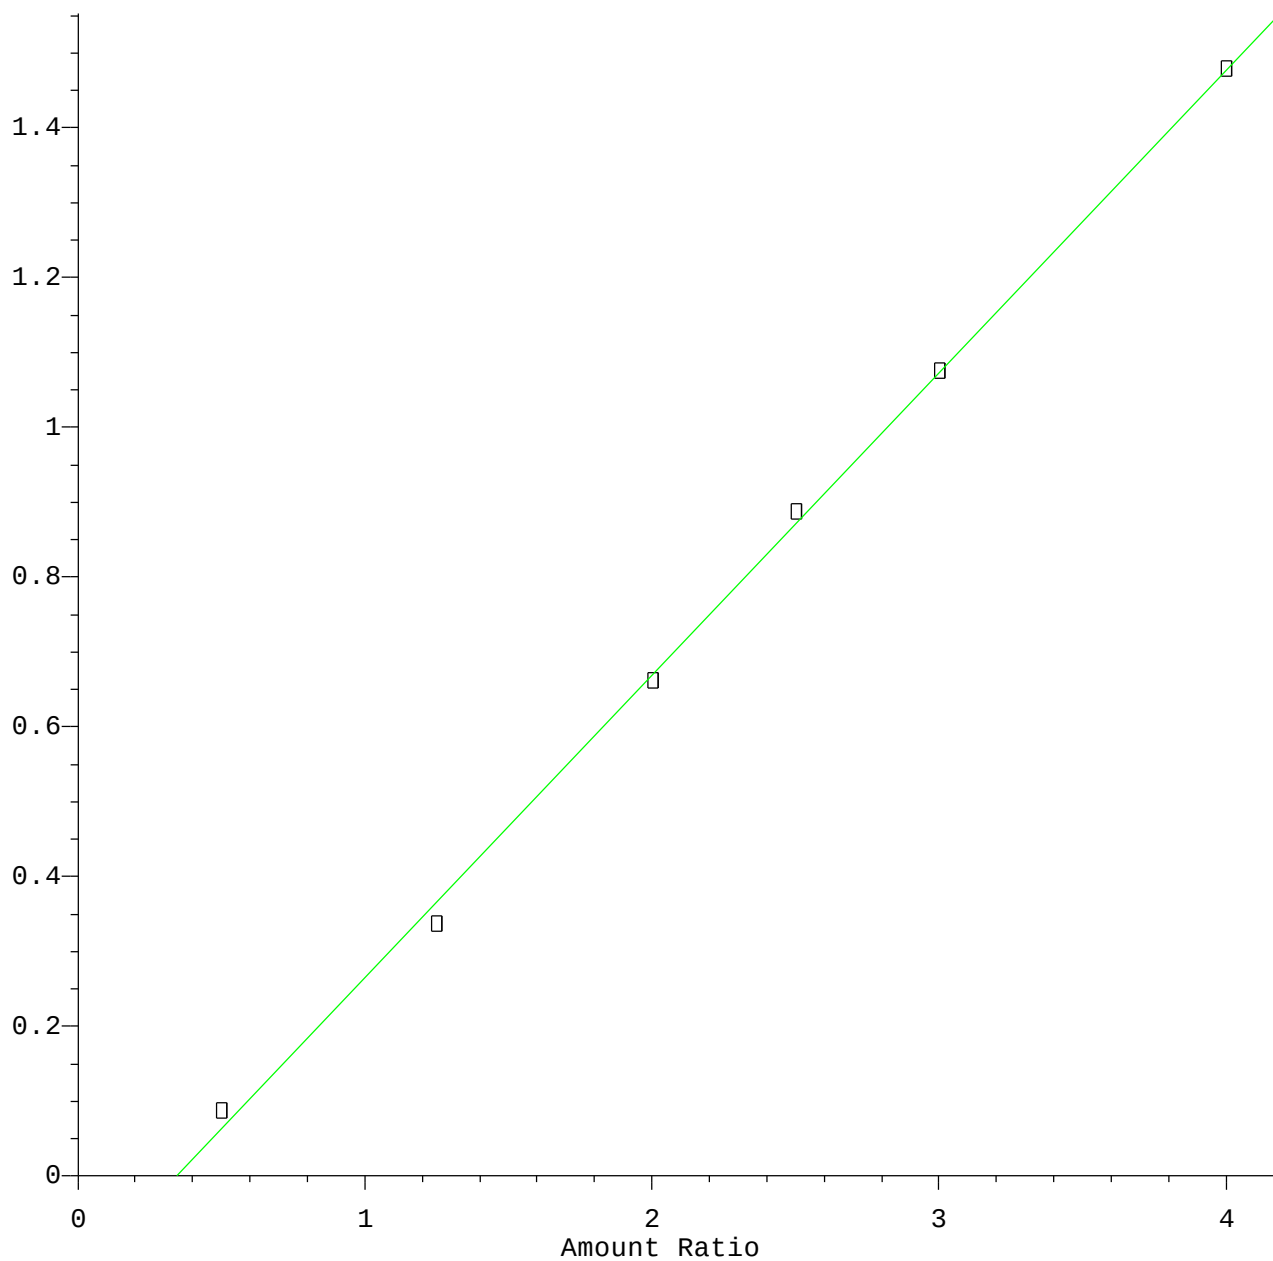


Resp Ratio = 4.04e-001 * Amt - 1.38e-001
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018

2,6-Dinitrotoluene

Response Ratio

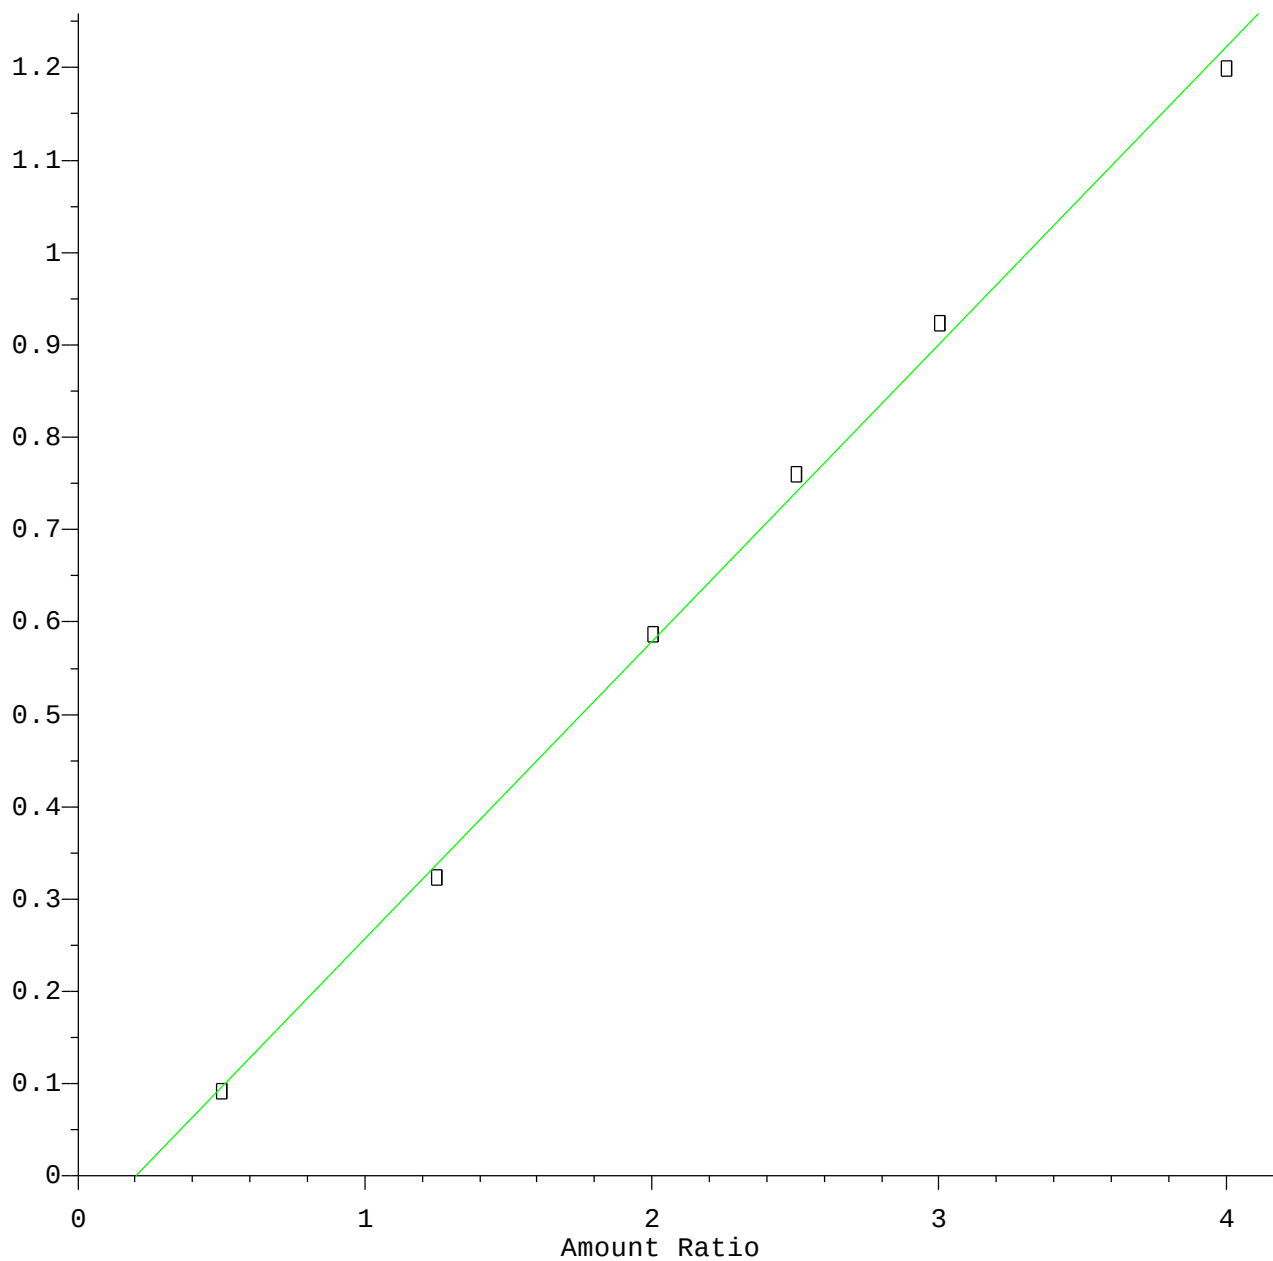


Resp Ratio = $3.22 \times 10^{-1} \times \text{Amt} - 6.41 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018


3-Nitroaniline

Response Ratio

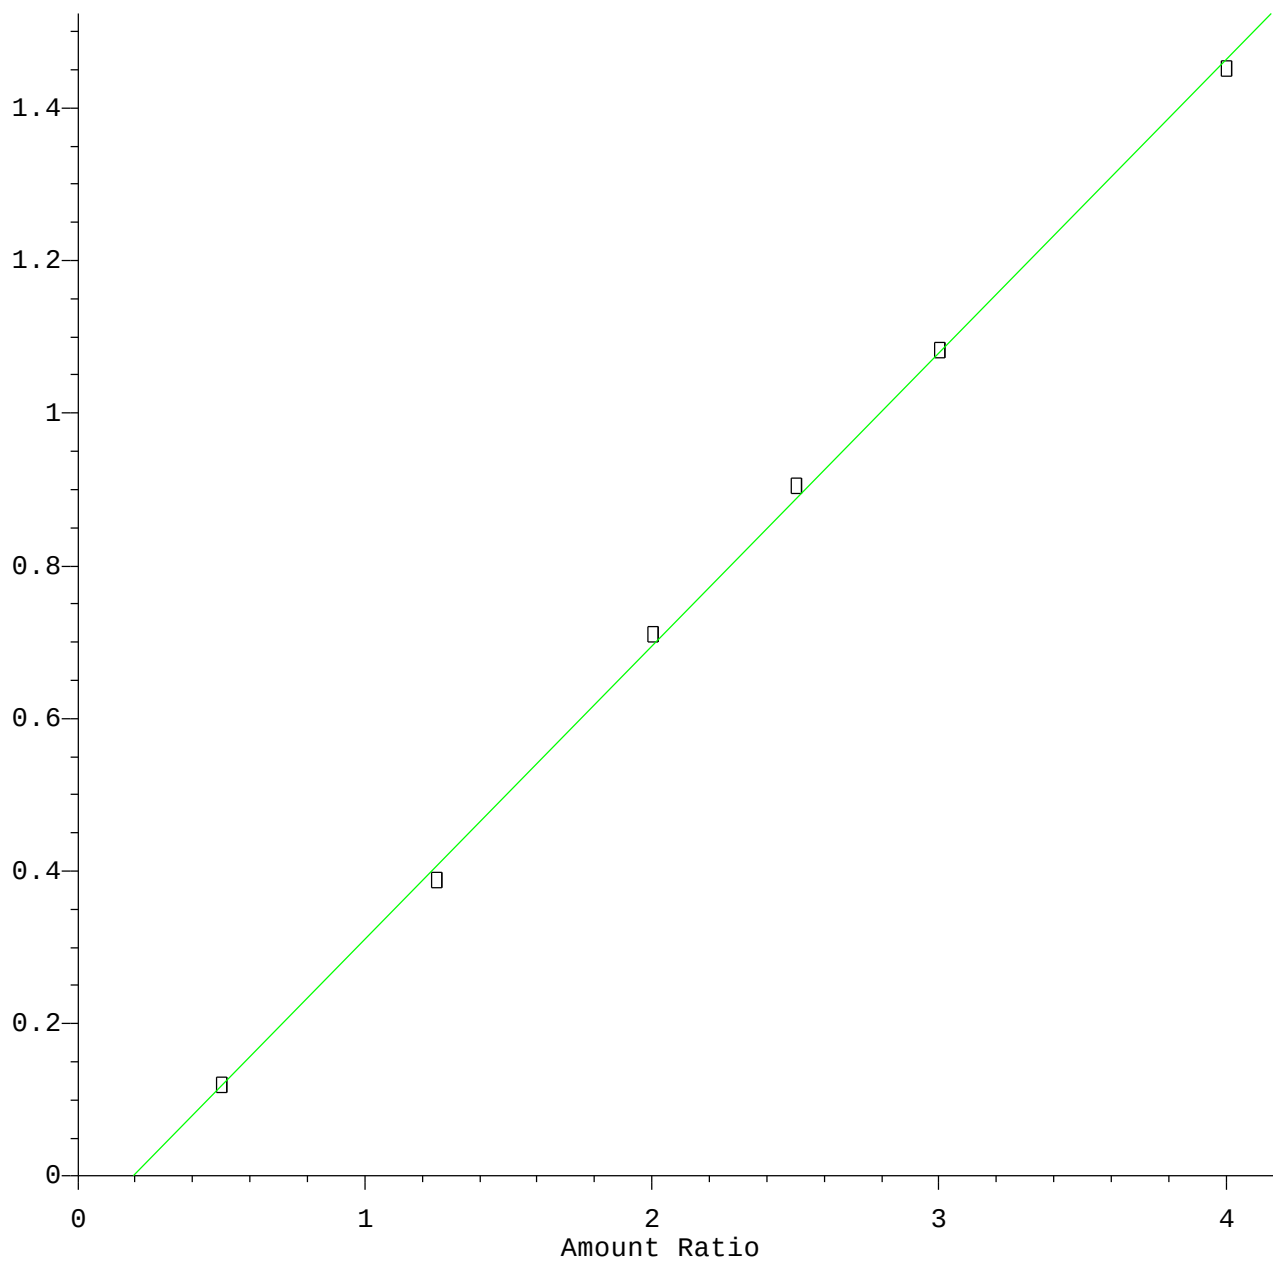


Resp Ratio = $3.84 \times 10^{-1} \times \text{Amt} - 7.33 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018

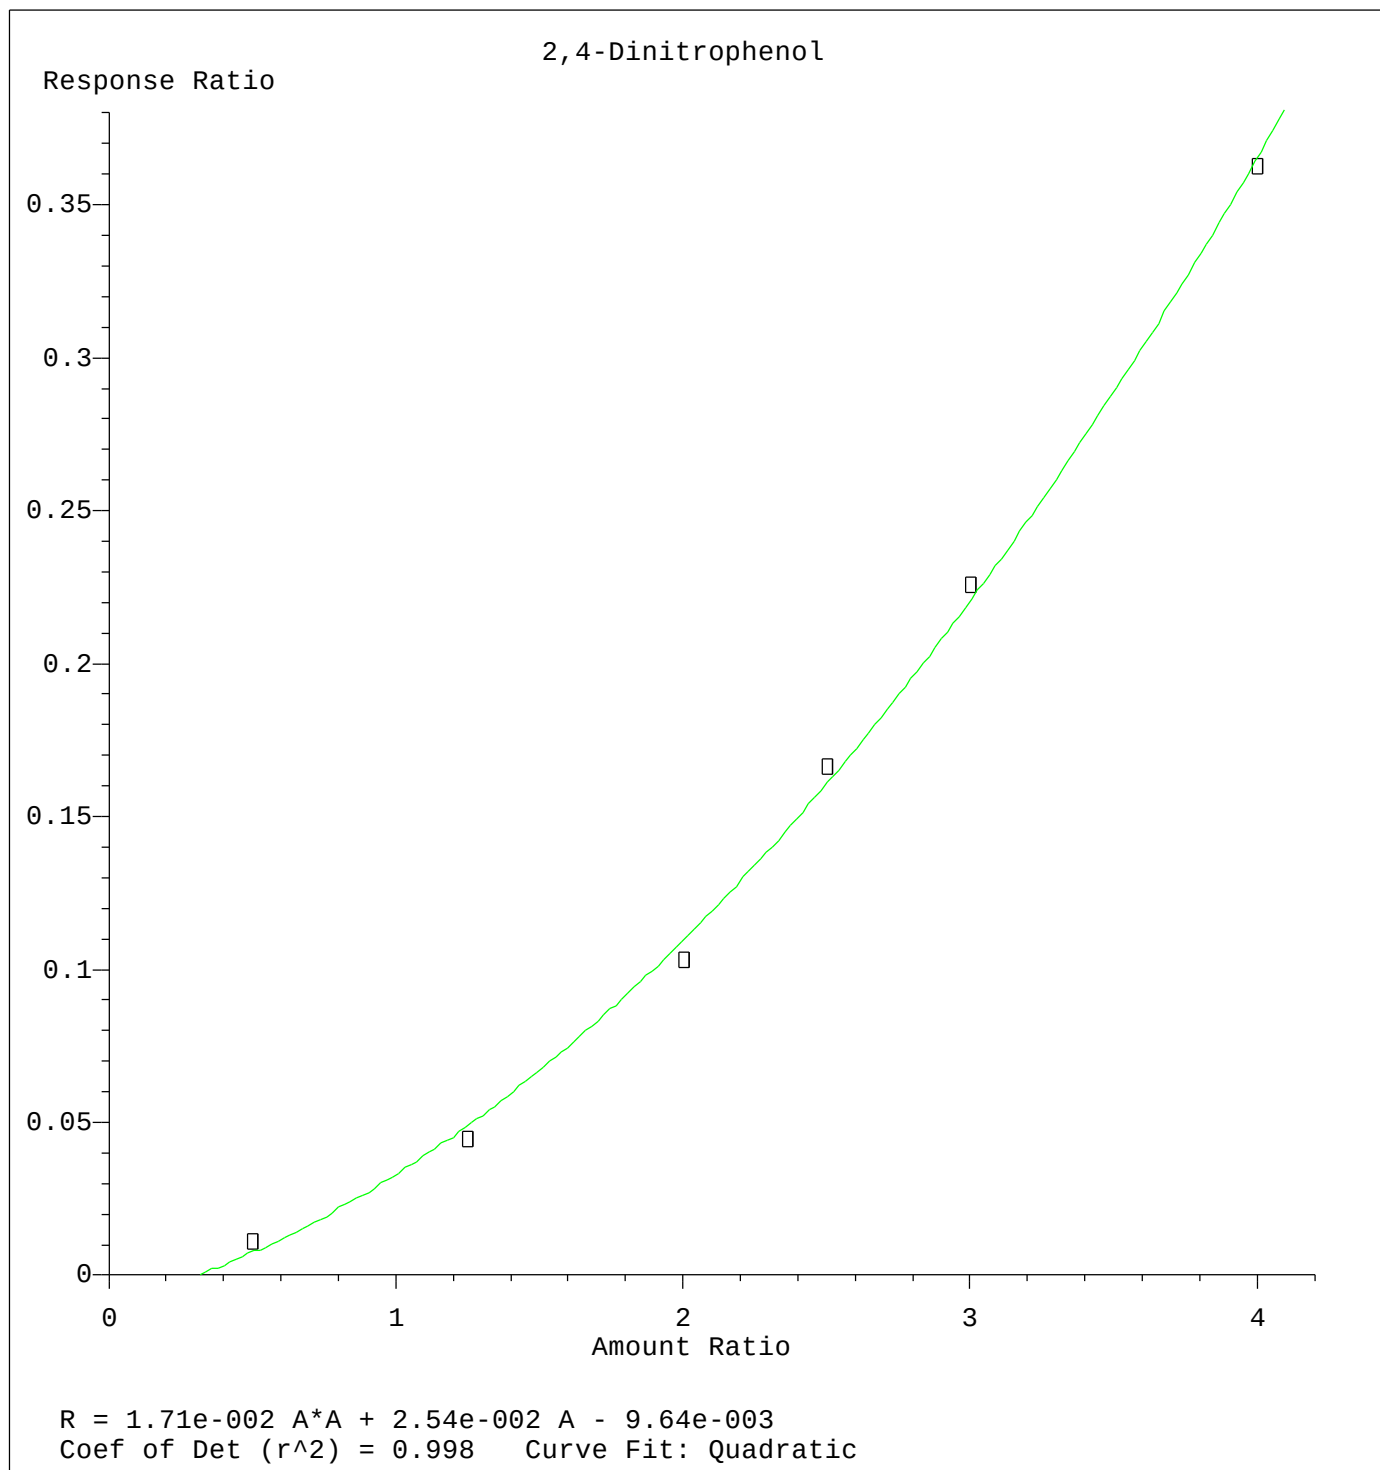


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018

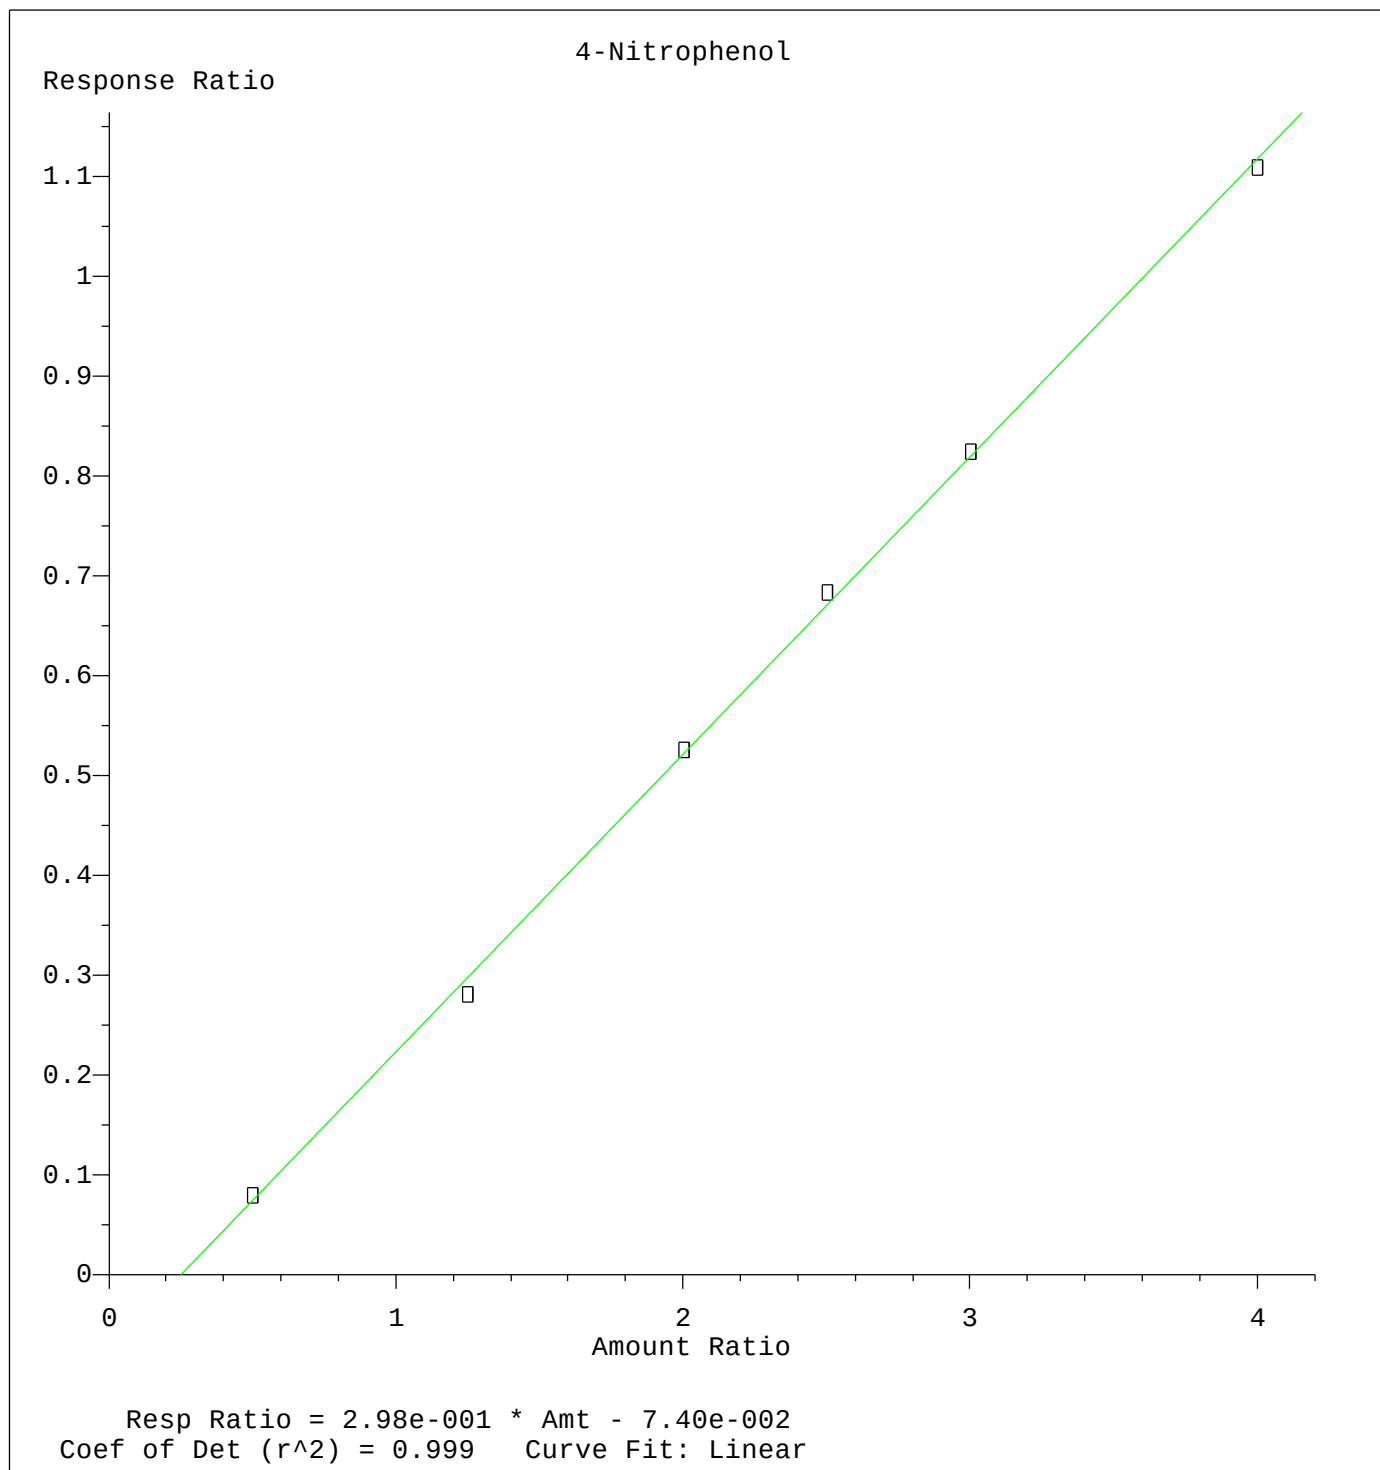

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018


2,4-Dinitrotoluene

Response Ratio

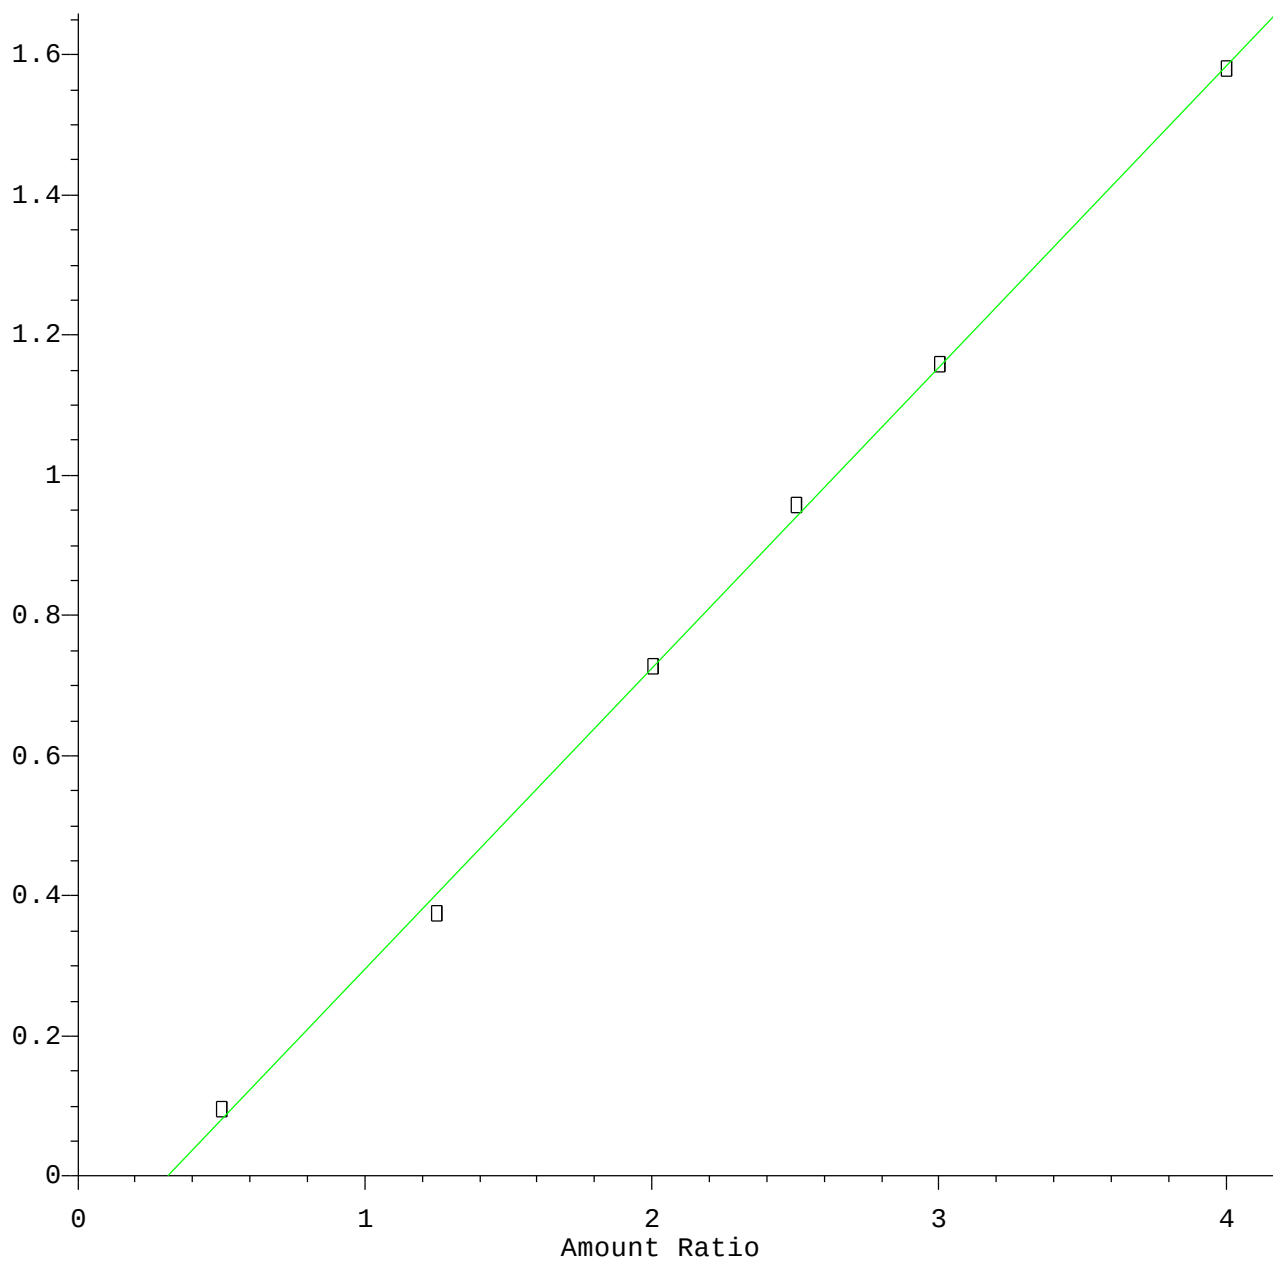


Resp Ratio = $4.30 \times 10^{-1} \times \text{Amt} - 1.33 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018

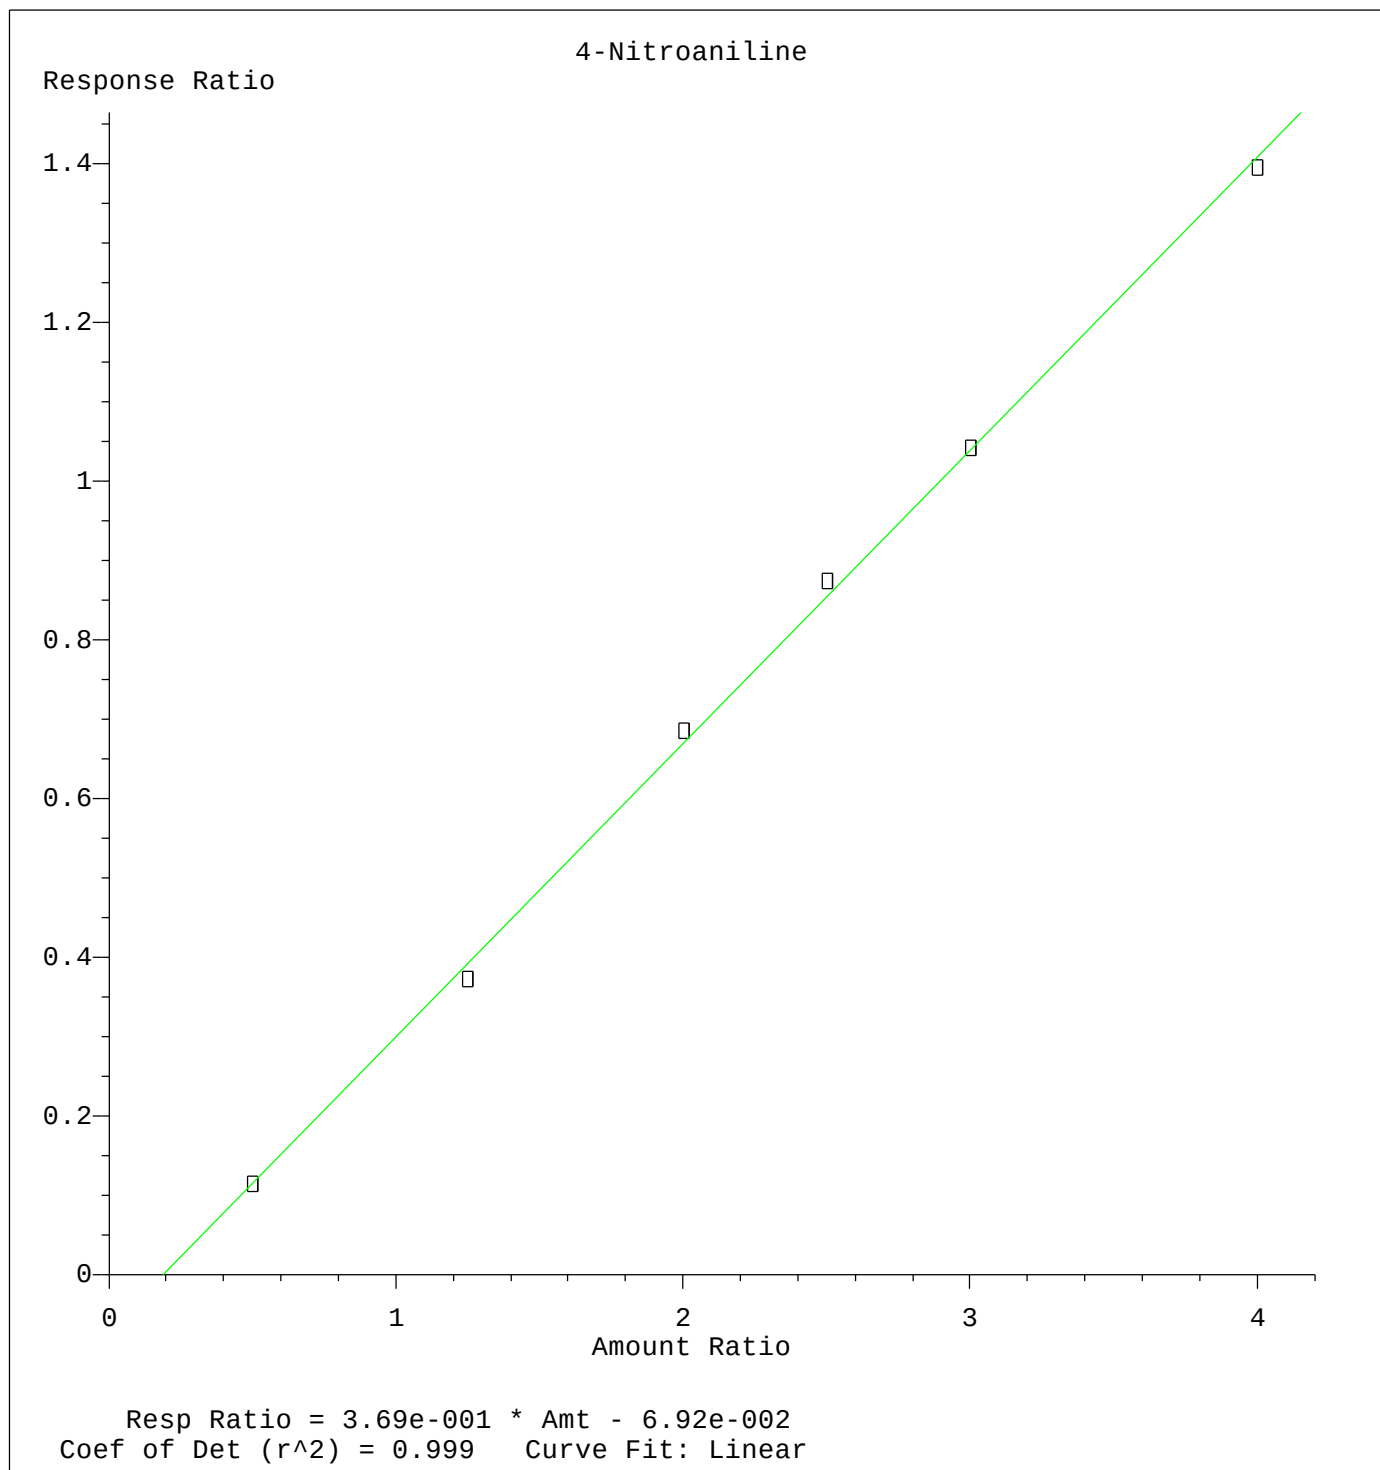

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018

4,6-Dinitro-2-methylphenol

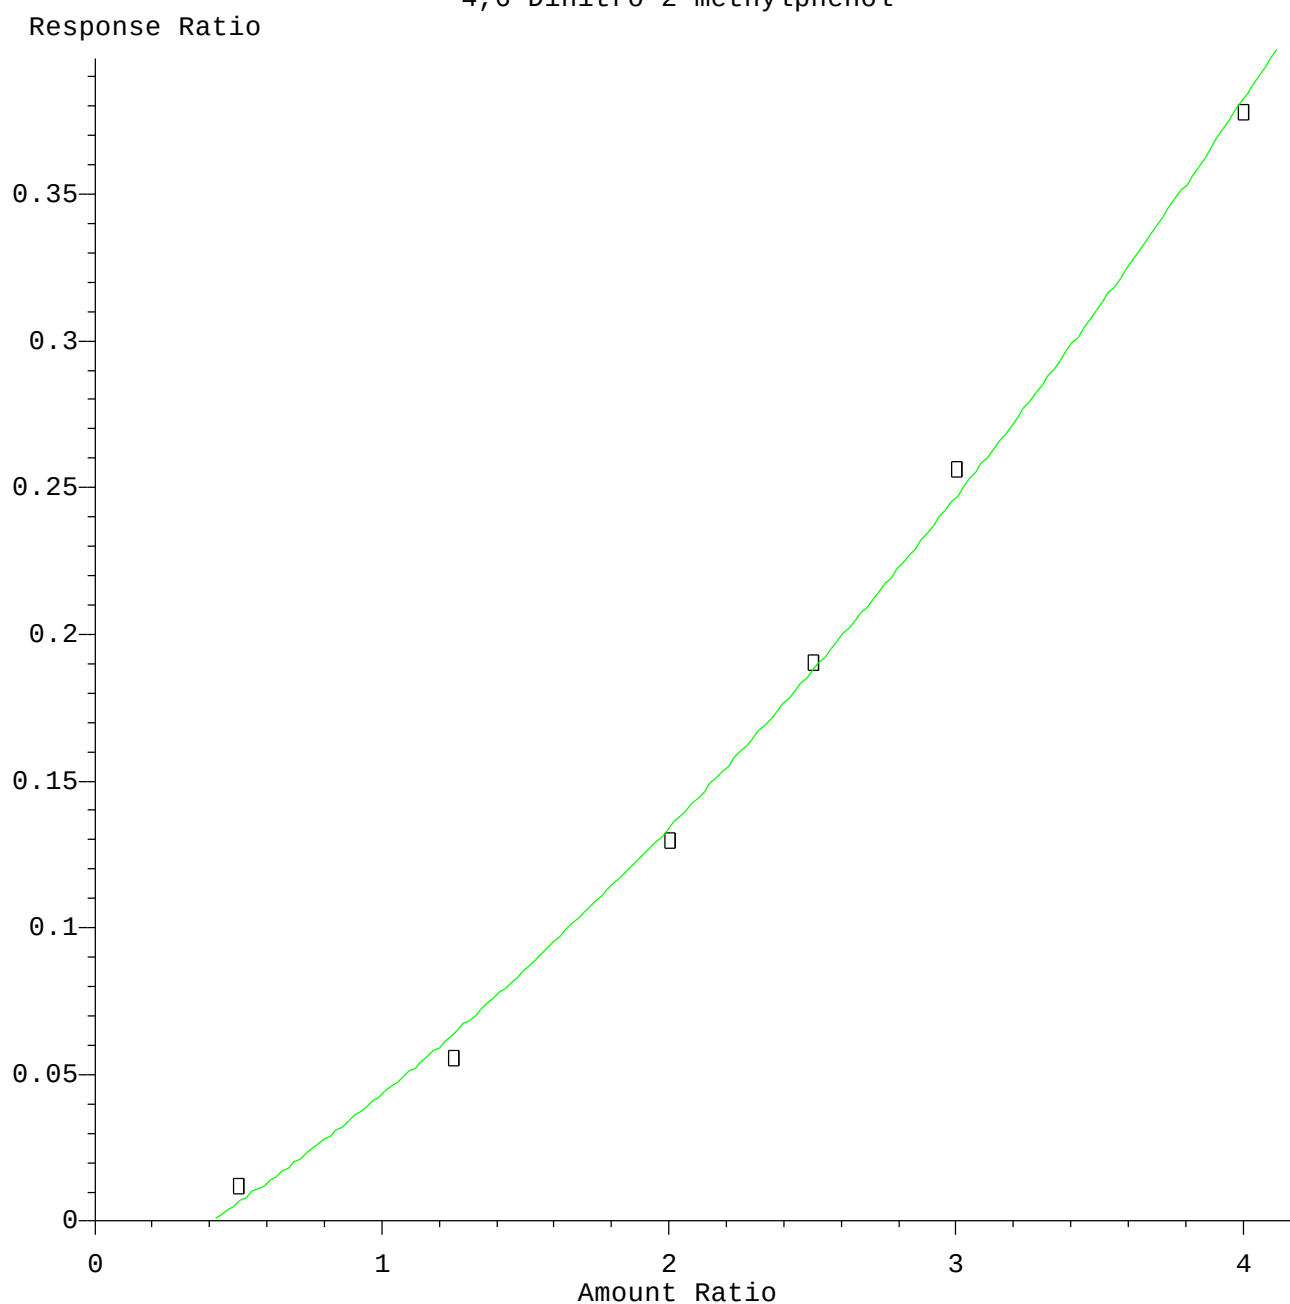

$R = 1.12e-002 A^2 + 5.72e-002 A - 2.50e-002$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Calibration Table Last Updated: Thu Mar 15 18:31:53 2018