


Data Path : Z:\HPCHEM1\BNA F\Data\BF031518\
 Data File : BF103666.D
 Acq On : 15 Mar 2018 13:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 15 18:31:53 2018

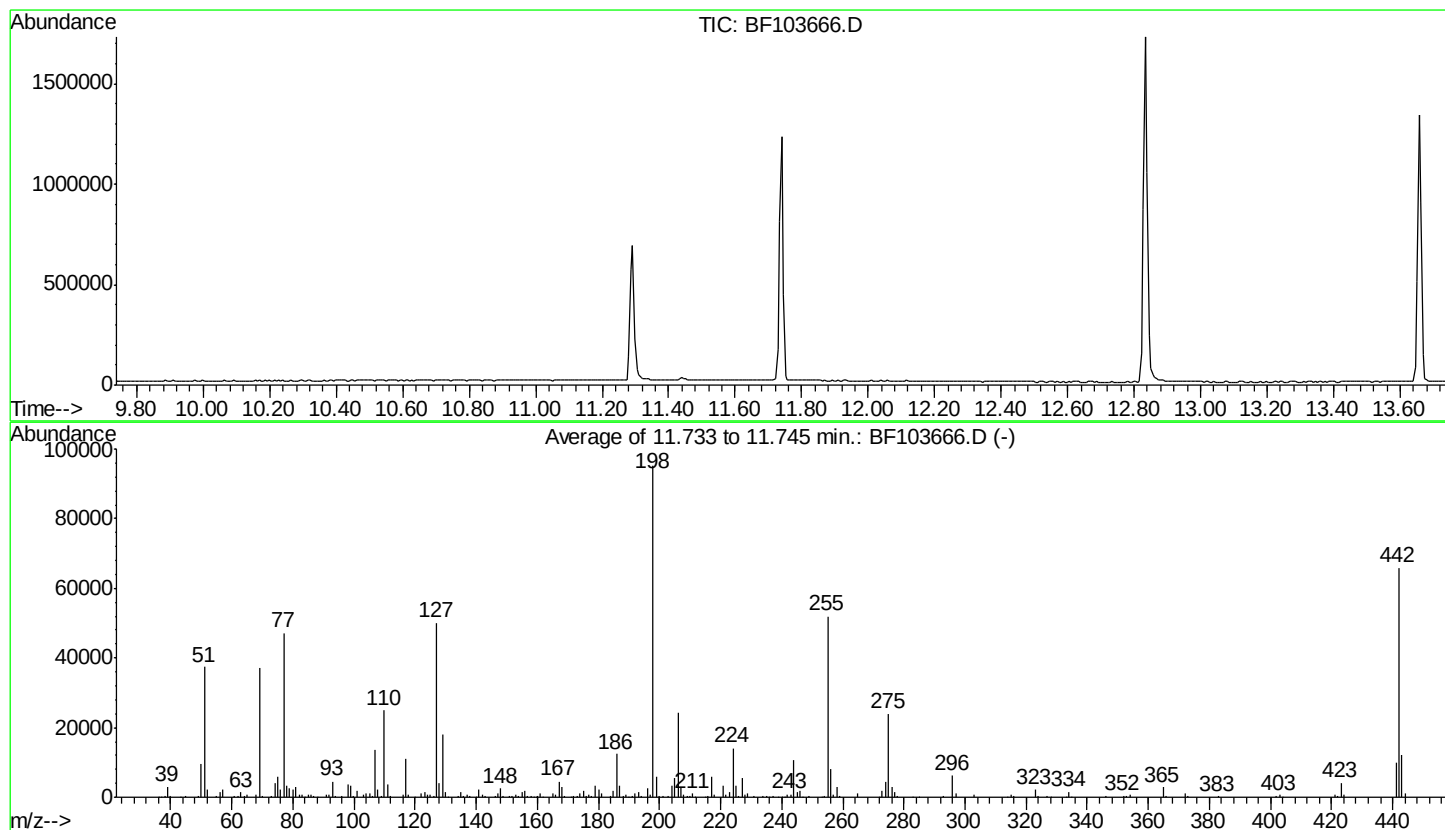

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	37375	PASS
68	69	0.00	2	1.7	618	PASS
69	198	0.00	100	39.0	37174	PASS
70	69	0.00	2	0.7	263	PASS
127	198	10	80	52.6	50144	PASS
197	198	0.00	2	0.8	774	PASS
198	198	100	100	100.0	95253	PASS
199	198	5	9	6.4	6051	PASS
275	198	10	60	25.3	24082	PASS
365	198	1	100	3.0	2850	PASS
441	443	0.01	100	83.5	10043	PASS
442	198	50	100	69.3	65992	PASS
443	442	15	24	18.2	12025	PASS