
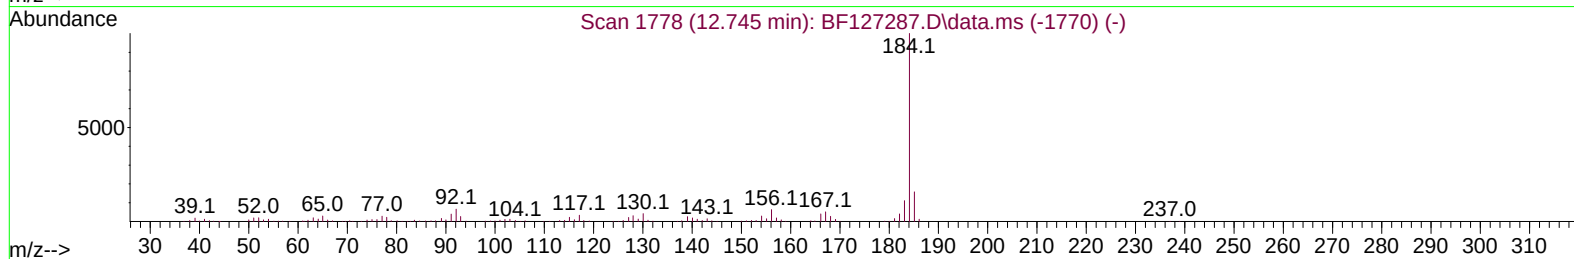
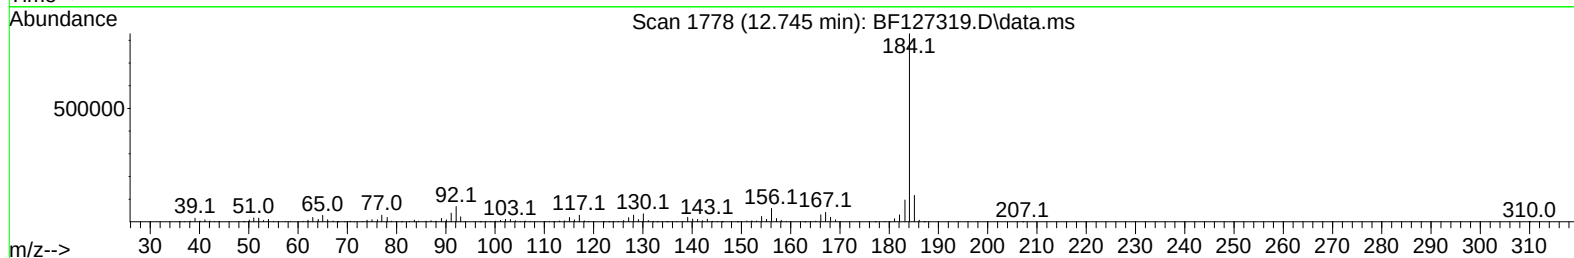


Quant Time: Mar 15 14:18:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

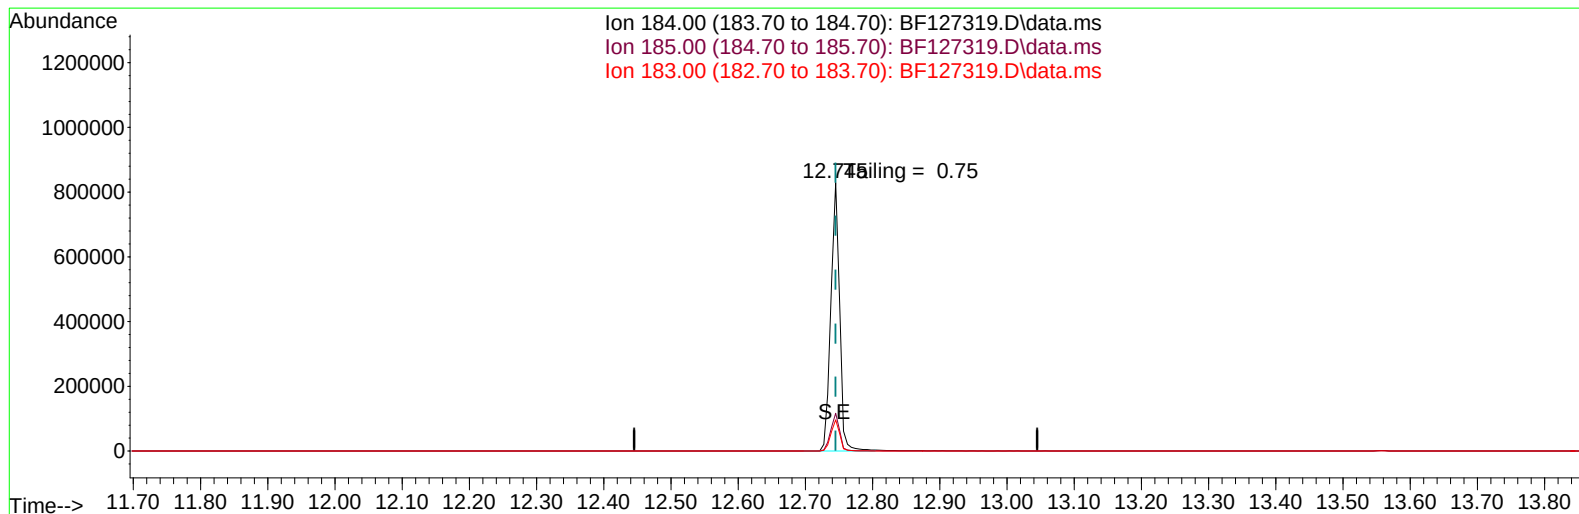

TIC: BF127319.D\data.ms

(77) Benzidine

12.745min (-0.000) 32053.87 ng

response **757254**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.08
183.00	10.20	11.62
0.00	0.00	0.00