
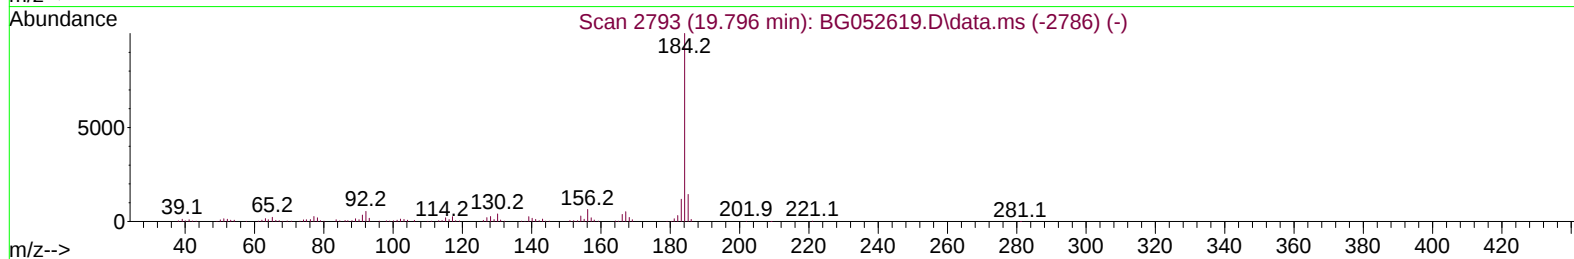
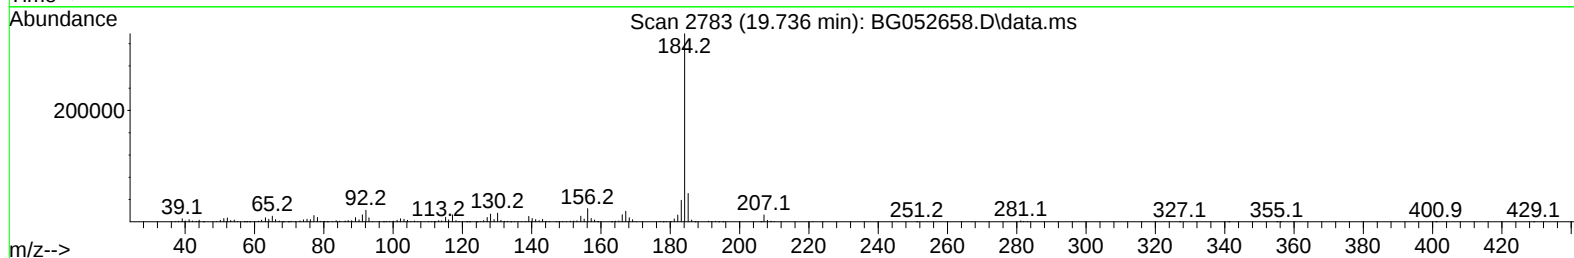


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
 Data File : BG052658.D
 Acq On : 15 Mar 2022 9:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 11:46:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 11:46:28 2022
 Response via : Initial Calibration

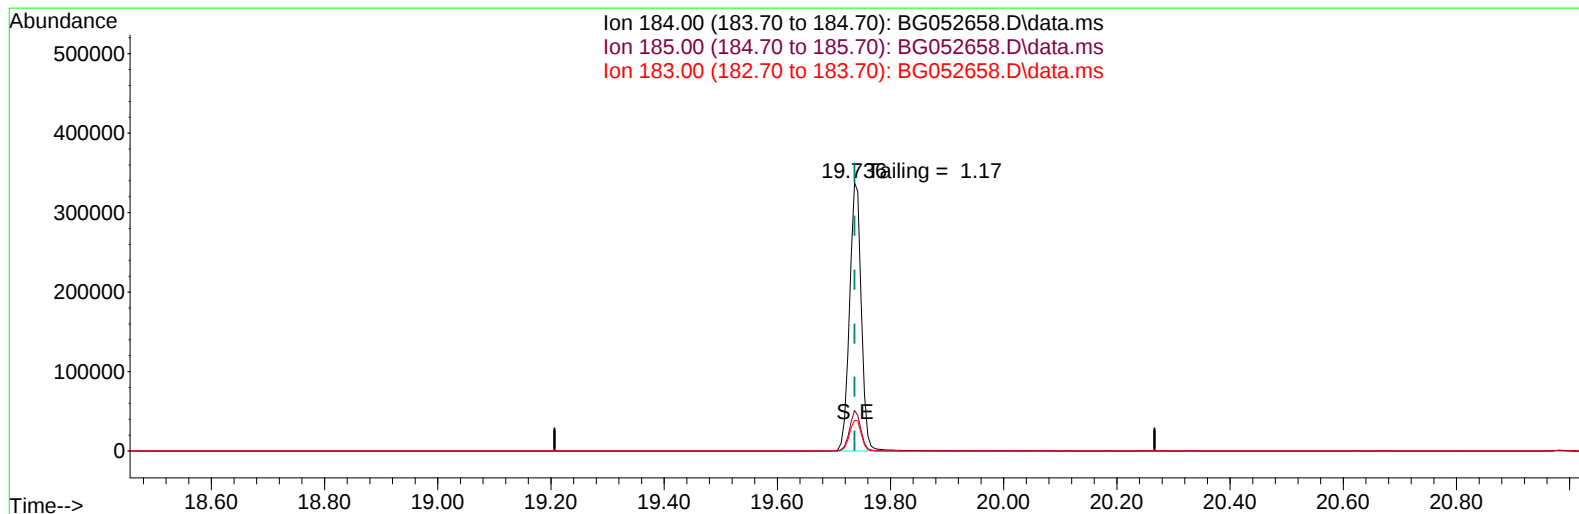

TIC: BG052658.D\data.ms

(77) Benzidine**19.736min (0.000) 426525.49 ng****response 486644**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.11
183.00	11.80	11.46
0.00	0.00	0.00