
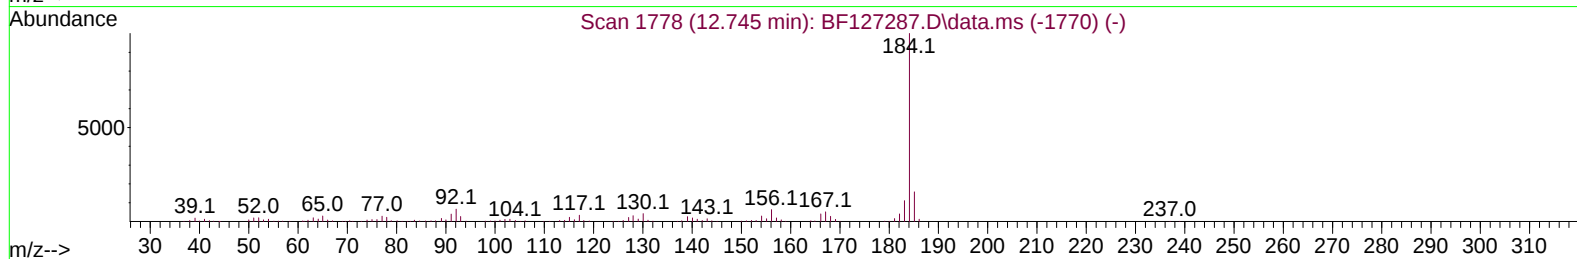
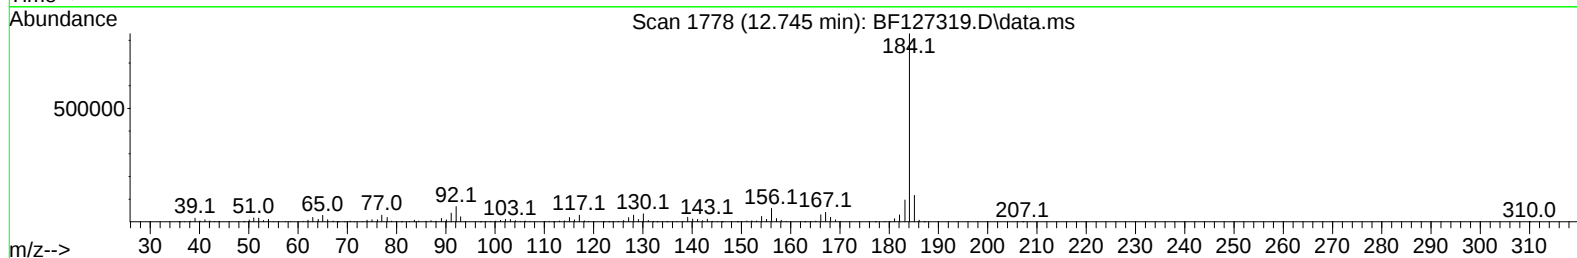


Quant Time: Mar 15 14:18:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

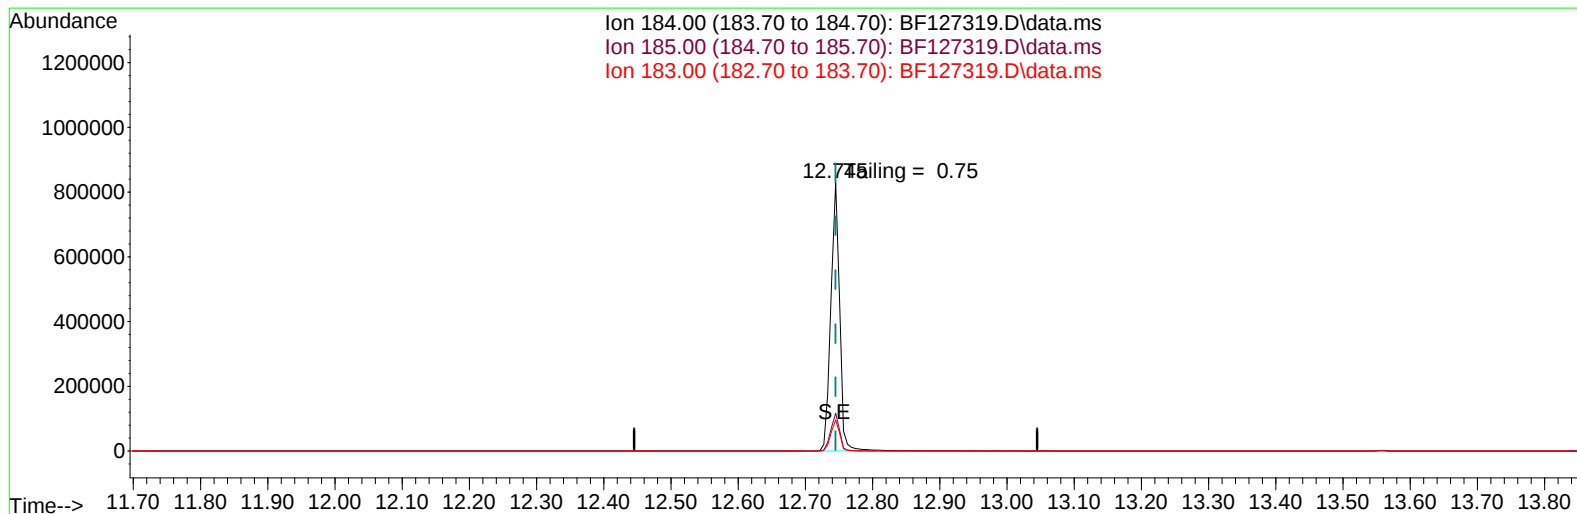

TIC: BF127319.D\data.ms

(77) Benzidine




12.745min (-0.000) 32053.87 ng

response 757254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.08
183.00	10.20	11.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127319.D
Acq On : 15 Mar 2022 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 14:18:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

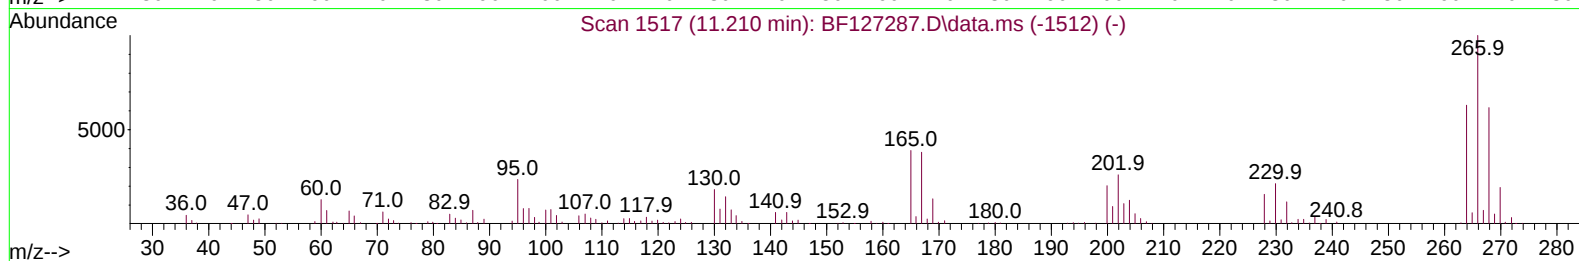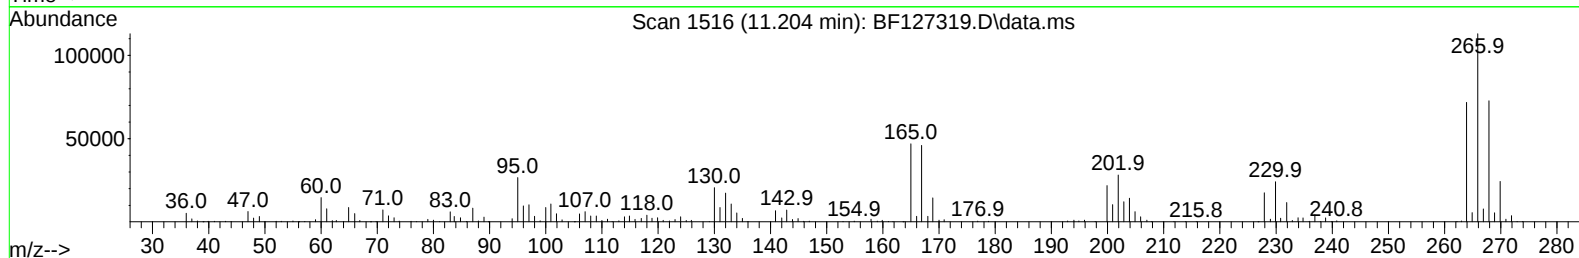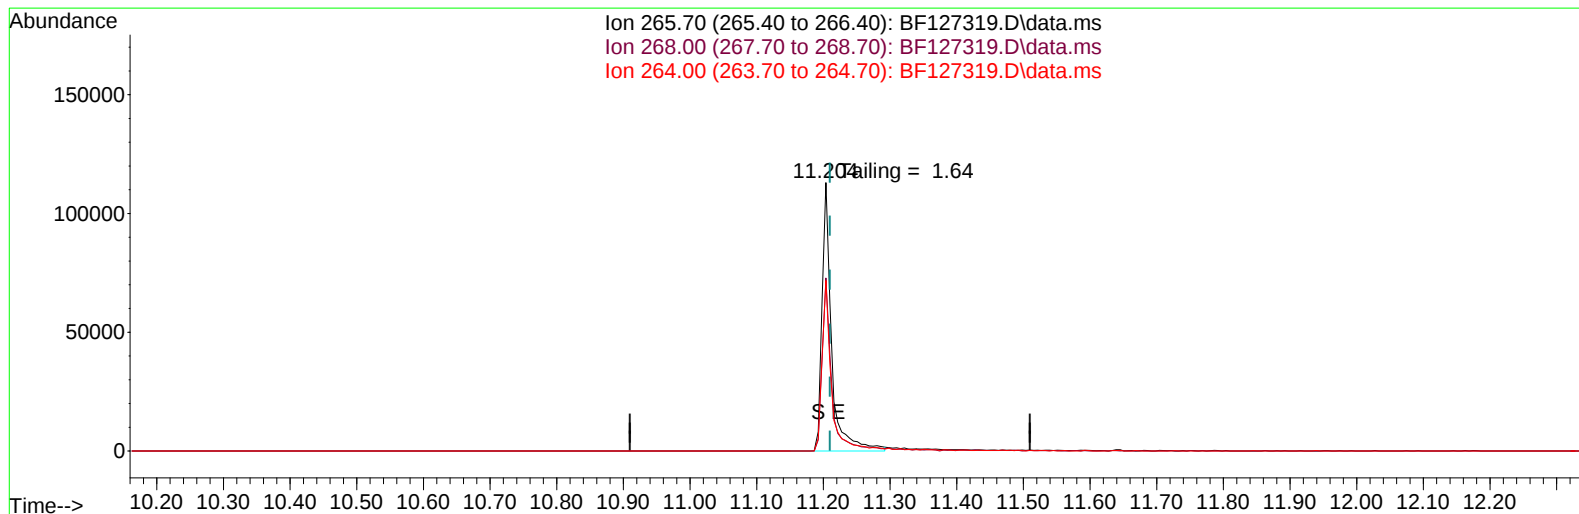

TIC: BF127319.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 394197.19 ng

response 117092

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.43
264.00	63.00	63.50
0.00	0.00	0.00