

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
 Data File : BF127330.D
 Acq On : 15 Mar 2022 18:04
 Operator : CG\JU
 Sample : PB143311BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143311BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	542	547	551	rBV	3217235	3773882	82.27%	13.509%
2	6.504	711	717	720	rBV	3104390	3899631	85.02%	13.959%
3	6.863	775	778	782	rBV	827987	749175	16.33%	2.682%
4	7.439	869	876	878	rBV	2160027	2748206	59.91%	9.838%
5	8.151	991	997	1000	rBV	984257	983899	21.45%	3.522%
6	9.227	1173	1180	1183	rBV	4410301	4545467	99.10%	16.271%
7	9.904	1290	1295	1299	rBV	1242700	1137410	24.80%	4.072%
8	10.704	1424	1431	1434	rBV	2828208	2700636	58.88%	9.667%
9	11.398	1545	1549	1552	rBV	1457368	1138014	24.81%	4.074%
10	12.992	1814	1820	1823	rBV	4515101	4586921	100.00%	16.420%
11	14.045	1995	1999	2008	rBV	1041625	934514	20.37%	3.345%
12	15.527	2246	2251	2261	rBV	583327	737796	16.08%	2.641%




Sum of corrected areas: 27935551

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127330.D
Acq On : 15 Mar 2022 18:04
Operator : CG\JU
Sample : PB143311BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

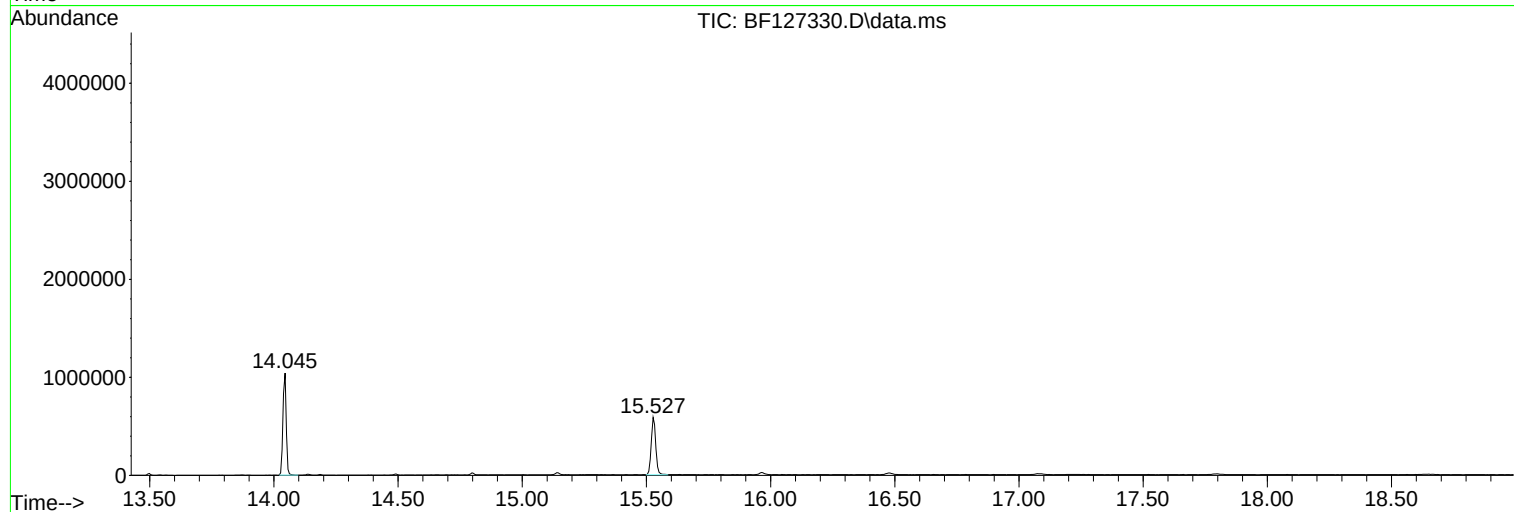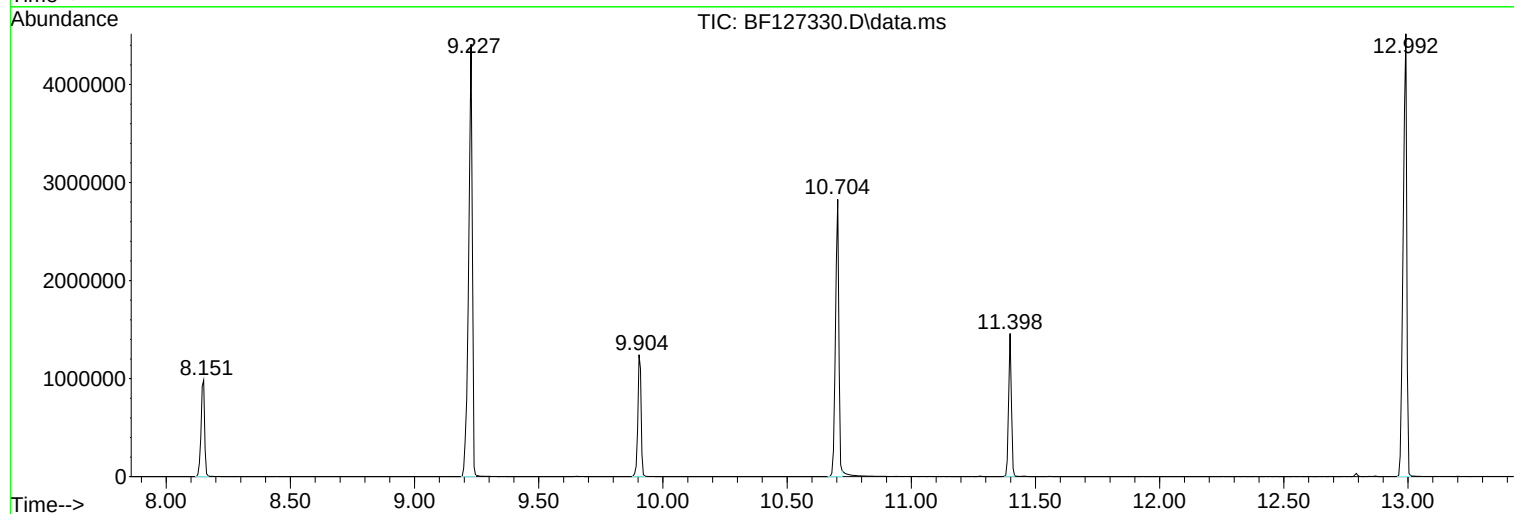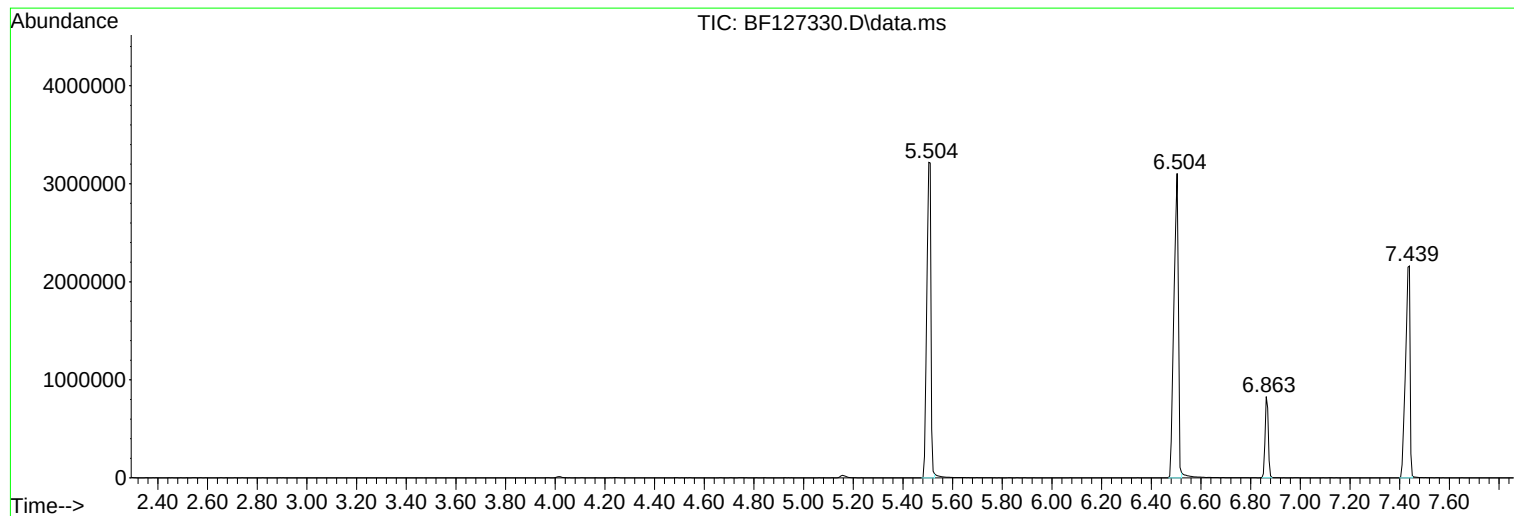

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127330.D
Acq On : 15 Mar 2022 18:04
Operator : CG\JU
Sample : PB143311BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127330.D
Acq On : 15 Mar 2022 18:04
Operator : CG\JU
Sample : PB143311BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------