

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
 Data File : BF127334.D
 Acq On : 15 Mar 2022 20:12
 Operator : CG\JU
 Sample : N1948-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	474	478	486	rBV	152997	194965	6.99%	1.133%
2	5.493	541	545	565	rBV	2275478	2105980	75.49%	12.237%
3	6.498	711	716	733	rBV	2275900	2276613	81.60%	13.229%
4	6.863	775	778	782	rBV	709382	586856	21.04%	3.410%
5	7.434	870	875	878	rBV	1505825	1509126	54.09%	8.769%
6	8.145	992	996	1000	rBV	817157	783646	28.09%	4.554%
7	9.222	1174	1179	1183	rBV	2611412	2618407	93.86%	15.215%
8	9.904	1291	1295	1299	rBV	1124918	942236	33.77%	5.475%
9	10.698	1426	1430	1438	rBV	1161941	1049519	37.62%	6.098%
10	11.398	1545	1549	1552	rBV	1257979	1021083	36.60%	5.933%
11	12.986	1814	1819	1822	rBV	3151200	2789810	100.00%	16.211%
12	14.045	1995	1999	2004	rVB	703260	647263	23.20%	3.761%
13	14.139	2011	2015	2019	rVB	38830	42468	1.52%	0.247%
14	14.874	2137	2140	2144	rVB	32597	35483	1.27%	0.206%
15	15.527	2246	2251	2261	rVB	487335	606255	21.73%	3.523%




Sum of corrected areas: 17209710

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127334.D
Acq On : 15 Mar 2022 20:12
Operator : CG\JU
Sample : N1948-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

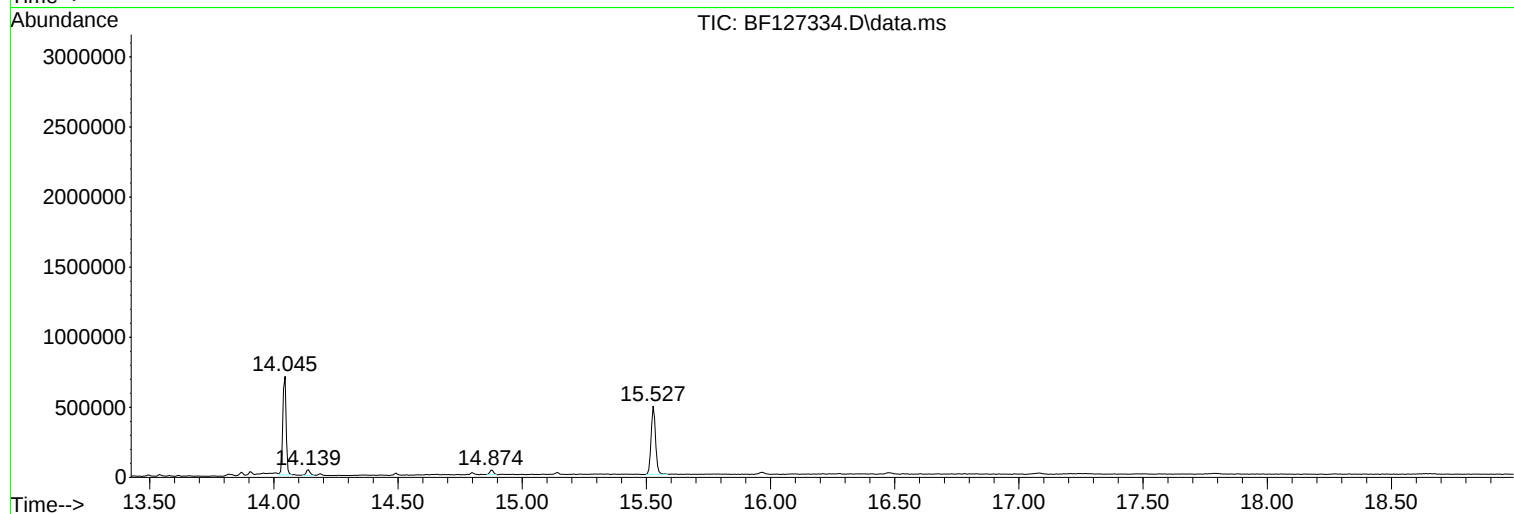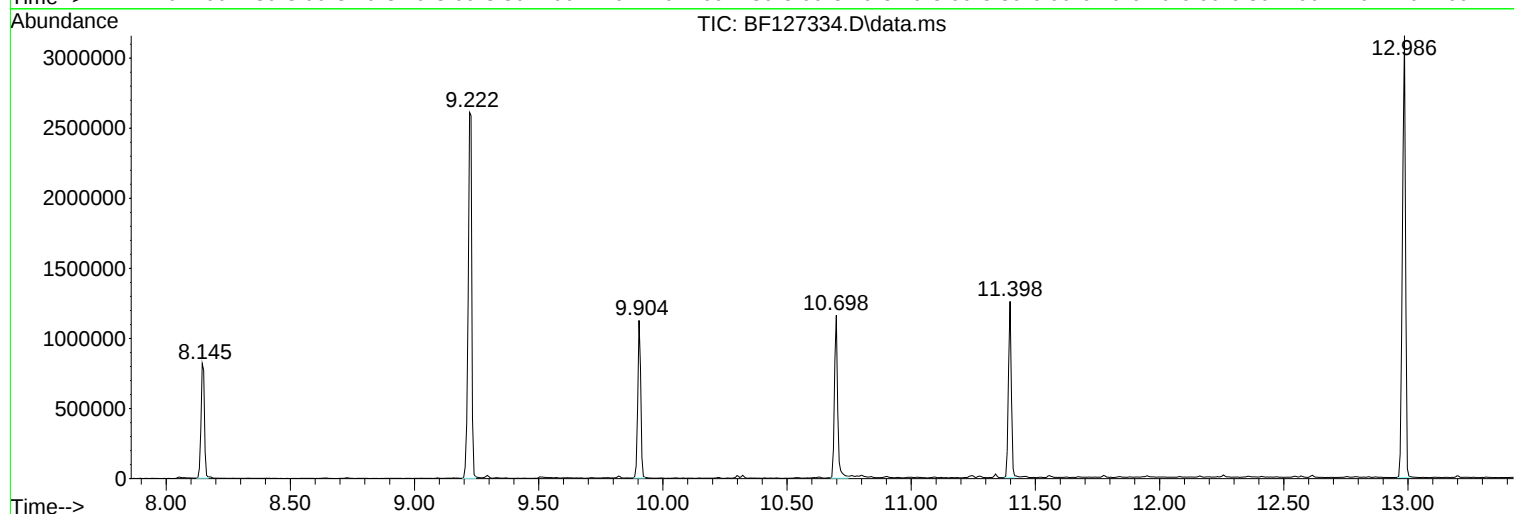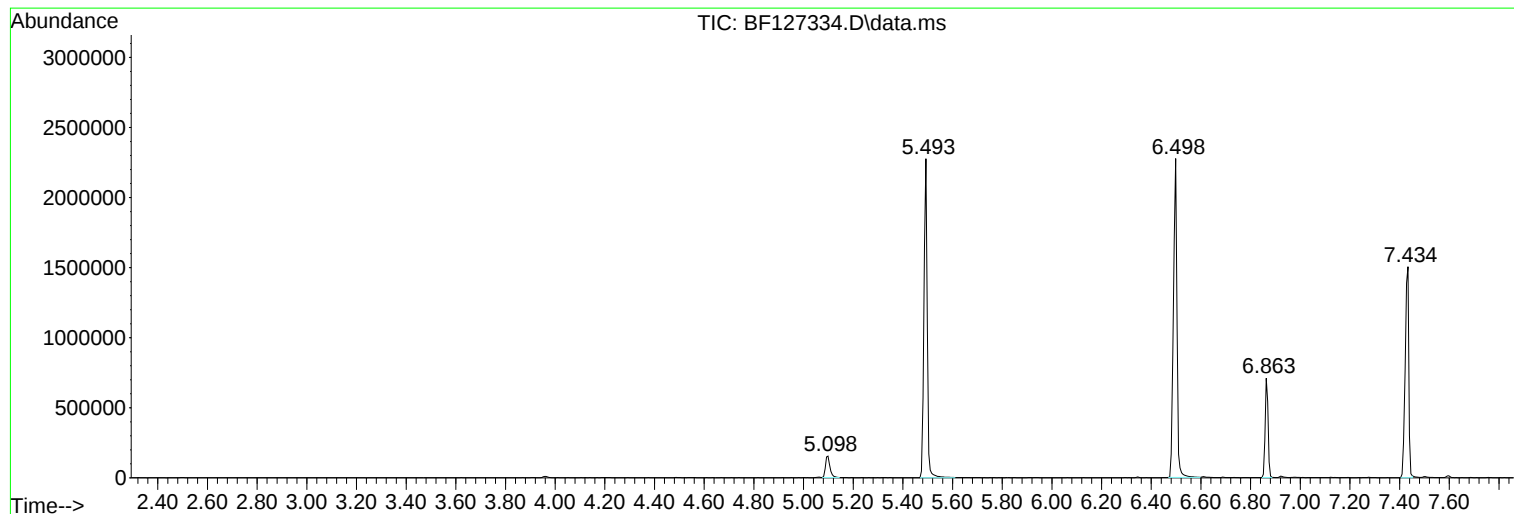

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127334.D
Acq On : 15 Mar 2022 20:12
Operator : CG\JU
Sample : N1948-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.098	6.64 ng	194965	1,4-Dichlorobenzene-d4	6.863

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36		
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32		
5	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28		

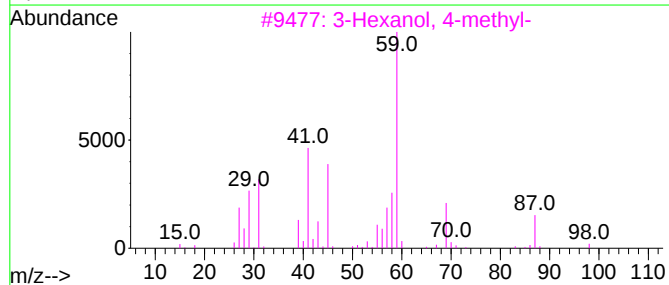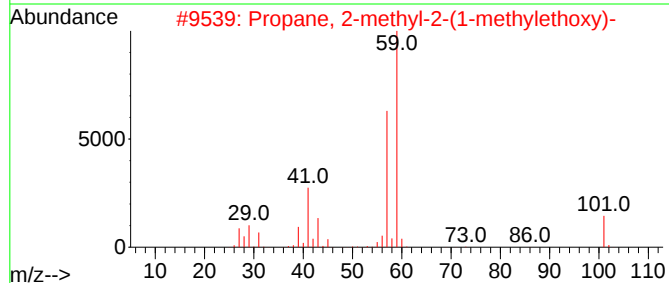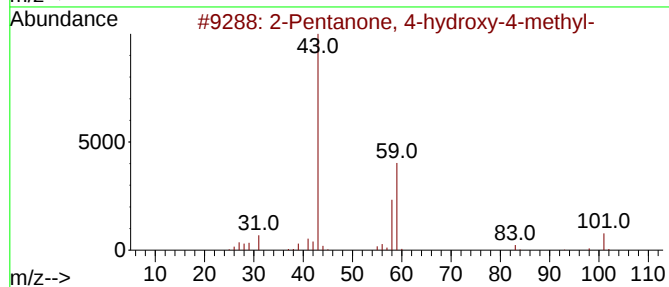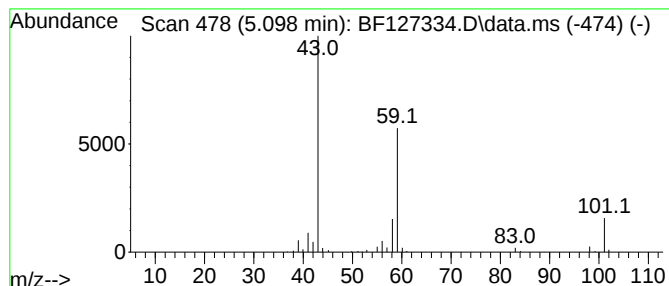

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127334.D
Acq On : 15 Mar 2022 20:12
Operator : CG\JU
Sample : N1948-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.098	6.6	ng	194965	1	6.863	586856	20.0