

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
 Data File : BF127339.D
 Acq On : 15 Mar 2022 22:37
 Operator : CG\JU
 Sample : N1922-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 7PH-2-8.5-9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	476	479	491	rVB	28106	37325	1.42%	0.219%
2	5.493	541	545	556	rBV	2307053	2116740	80.65%	12.443%
3	6.498	711	716	719	rBV	2240799	2177974	82.98%	12.803%
4	6.863	775	778	782	rBV	672387	554486	21.13%	3.259%
5	7.434	870	875	878	rBV	1461481	1466943	55.89%	8.623%
6	8.051	976	980	988	rBV	40456	65336	2.49%	0.384%
7	8.145	992	996	1000	rBV	794733	725263	27.63%	4.263%
8	9.222	1174	1179	1183	rBV	2743917	2558152	97.47%	15.038%
9	9.904	1291	1295	1299	rBV	1066810	879213	33.50%	5.168%
10	10.698	1426	1430	1439	rBV	1543337	1367392	52.10%	8.038%
11	11.398	1545	1549	1552	rBV	1169481	946814	36.07%	5.566%
12	11.774	1610	1613	1616	rVB	45891	37898	1.44%	0.223%
13	12.486	1727	1734	1736	rBV	76987	69140	2.63%	0.406%
14	12.986	1814	1819	1822	rBV	2968972	2624667	100.00%	15.429%
15	13.510	1904	1908	1911	rBV	169466	133101	5.07%	0.782%
16	13.904	1972	1975	1979	rBV	28717	29382	1.12%	0.173%
17	14.045	1995	1999	2007	rVB	634040	616041	23.47%	3.621%
18	14.874	2137	2140	2144	rVB	40429	40712	1.55%	0.239%
19	15.527	2246	2251	2257	rBV	463861	565049	21.53%	3.322%




Sum of corrected areas: 17011628

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127339.D
Acq On : 15 Mar 2022 22:37
Operator : CG\JU
Sample : N1922-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
7PH-2-8.5-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

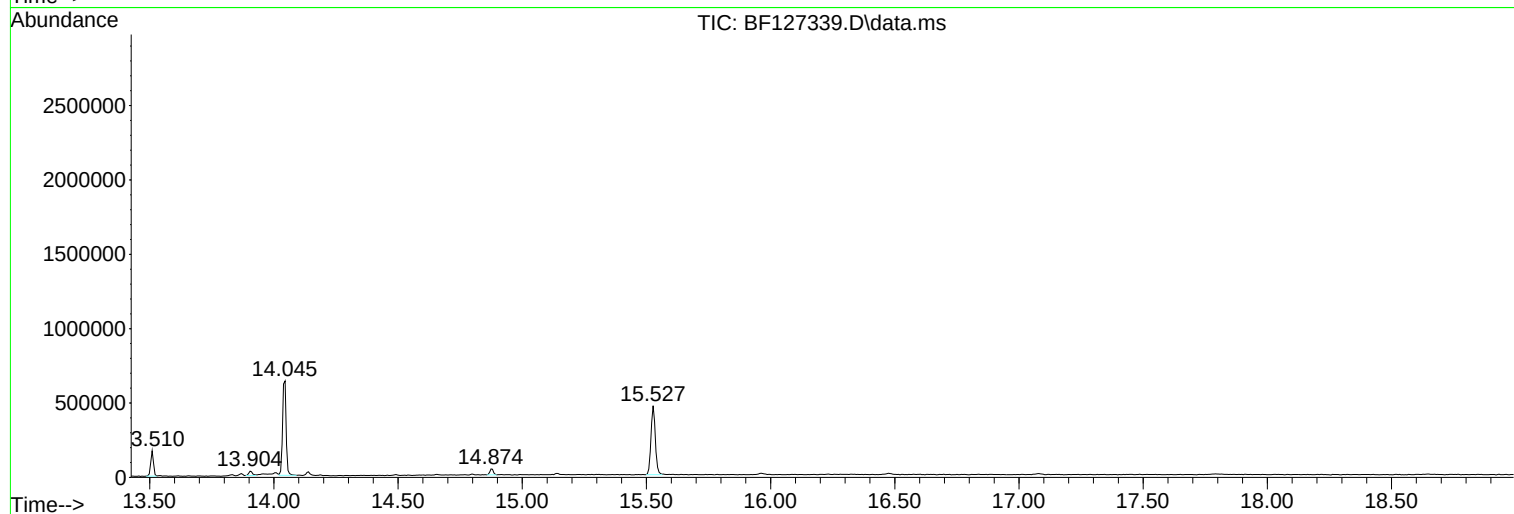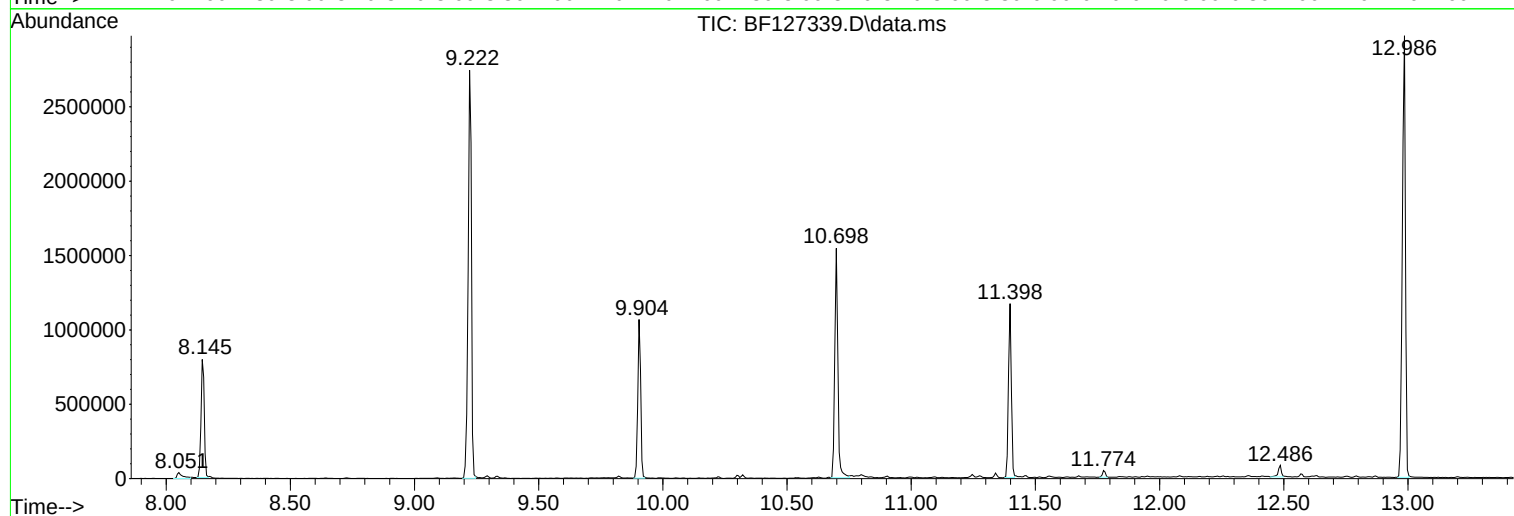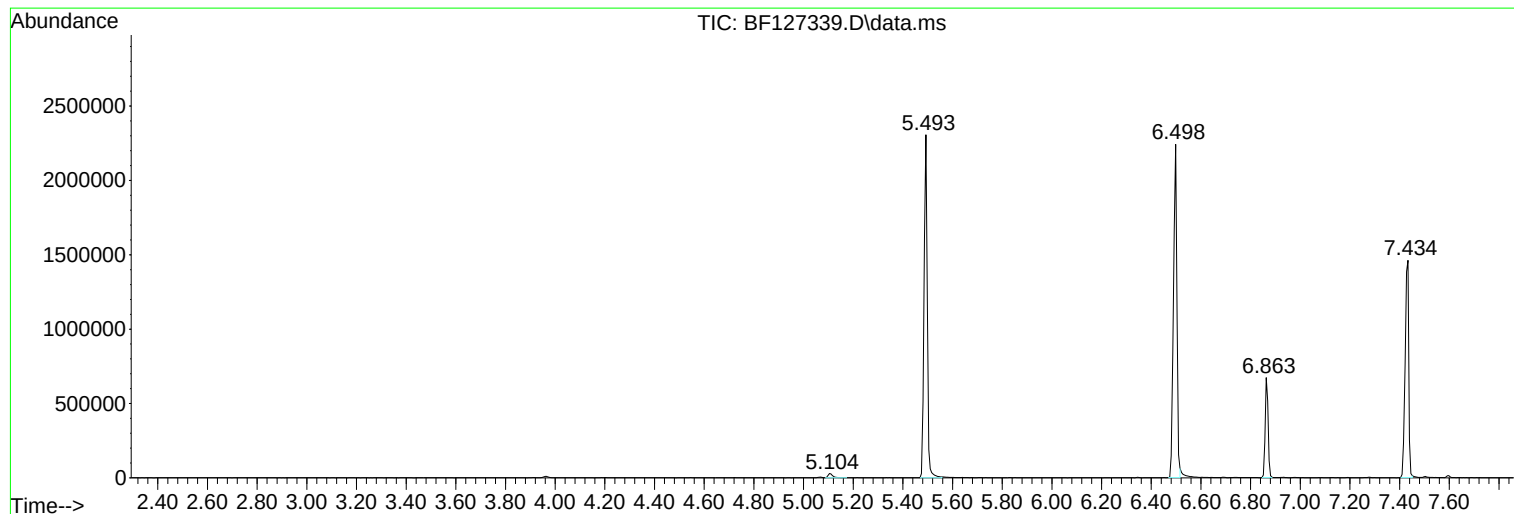

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127339.D
Acq On : 15 Mar 2022 22:37
Operator : CG\JU
Sample : N1922-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
7PH-2-8.5-9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.510	4.32 ng	133101	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	72
3			Hexanedioic acid, mono(2-ethylhe...	258	C14H26O4	004337-65-9	64
4			Diisooctyl adipate	370	C22H42O4	001330-86-5	52
5			Adipic acid, cis-hex-3-enyl isob...	284	C16H28O4	1000353-97-1	47

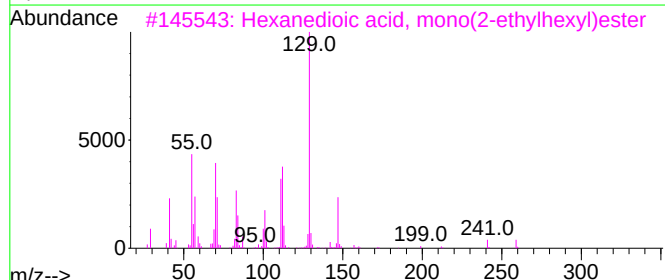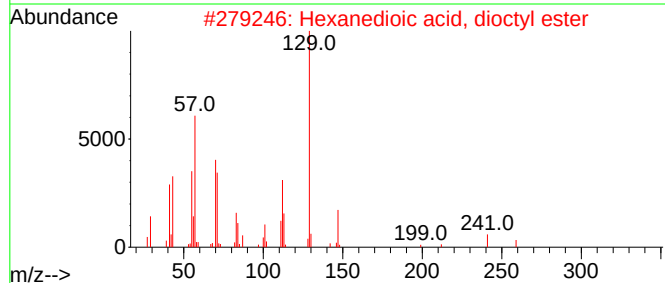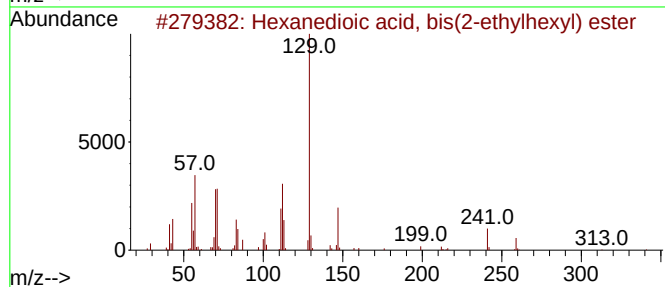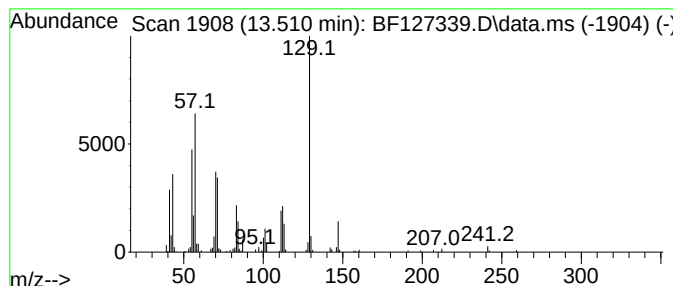

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127339.D
Acq On : 15 Mar 2022 22:37
Operator : CG\JU
Sample : N1922-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
7PH-2-8.5-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	13.510	4.3	ng	133101	5	14.045	616041	20.0