

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
 Data File : BF127340.D
 Acq On : 15 Mar 2022 23:06
 Operator : CG\JU
 Sample : N1948-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	474	477	491	rVB	84795	106334	4.81%	0.717%
2	5.493	541	545	561	rBV	1982727	1847999	83.67%	12.458%
3	6.498	712	716	732	rBV	2083857	1945951	88.11%	13.118%
4	6.863	775	778	782	rBV	608790	543716	24.62%	3.665%
5	7.428	870	874	878	rBV	1285896	1274963	57.73%	8.595%
6	8.051	977	980	993	rBV	35786	68779	3.11%	0.464%
7	8.145	993	996	1000	rBV	783927	711263	32.20%	4.795%
8	9.222	1175	1179	1183	rBV	2436242	2208552	100.00%	14.888%
9	9.333	1195	1198	1202	rBV	71605	63569	2.88%	0.429%
10	9.904	1292	1295	1299	rBV	996565	836732	37.89%	5.641%
11	10.698	1426	1430	1438	rBV	1369838	1183404	53.58%	7.978%
12	11.398	1545	1549	1552	rBV	1016814	832347	37.69%	5.611%
13	11.774	1610	1613	1618	rVB	45164	39313	1.78%	0.265%
14	12.569	1745	1748	1753	rVB2	42739	34239	1.55%	0.231%
15	12.980	1814	1818	1822	rBV	2049581	1942076	87.93%	13.092%
16	13.904	1972	1975	1980	rBV	31005	31713	1.44%	0.214%
17	14.045	1995	1999	2002	rBV	571852	528574	23.93%	3.563%
18	14.133	2011	2014	2021	rVB	21844	25739	1.17%	0.174%
19	14.874	2137	2140	2145	rVB	36286	34943	1.58%	0.236%
20	15.527	2246	2251	2259	rBV	470186	574022	25.99%	3.870%




Sum of corrected areas: 14834228

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127340.D
Acq On : 15 Mar 2022 23:06
Operator : CG\JU
Sample : N1948-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

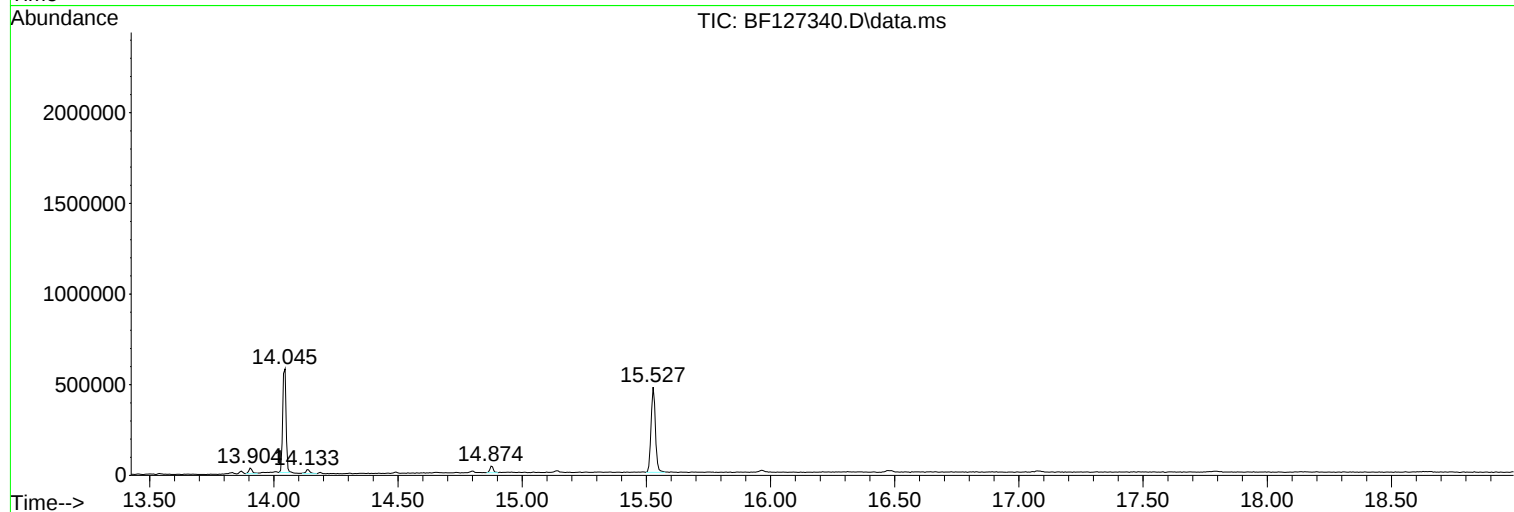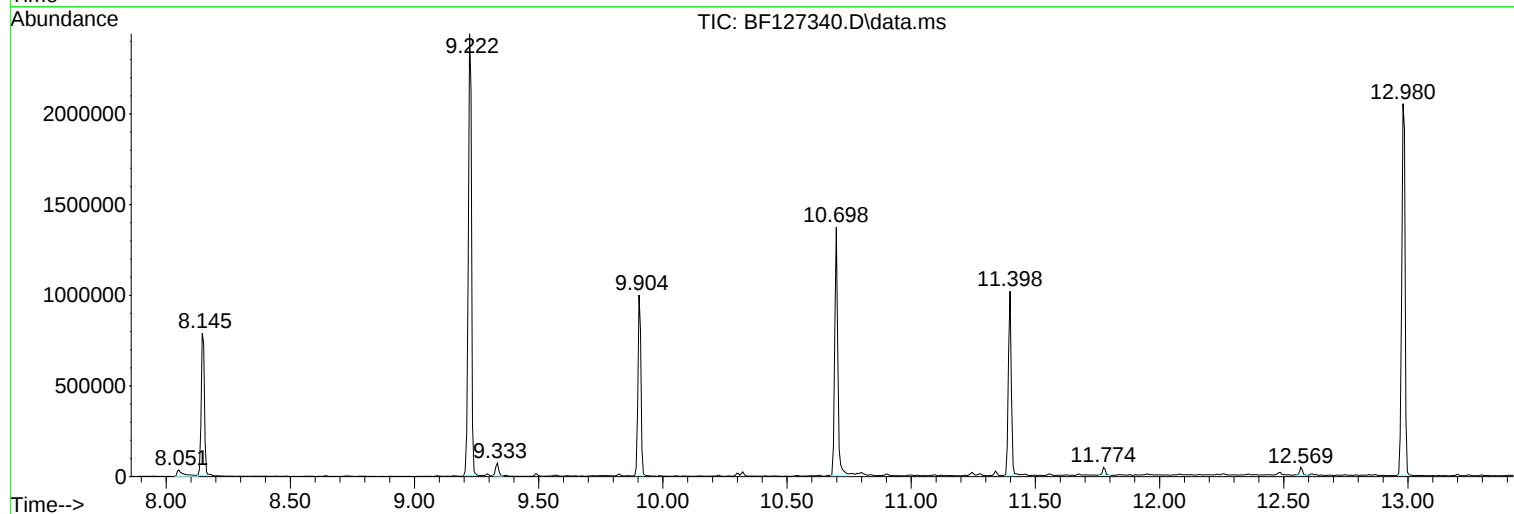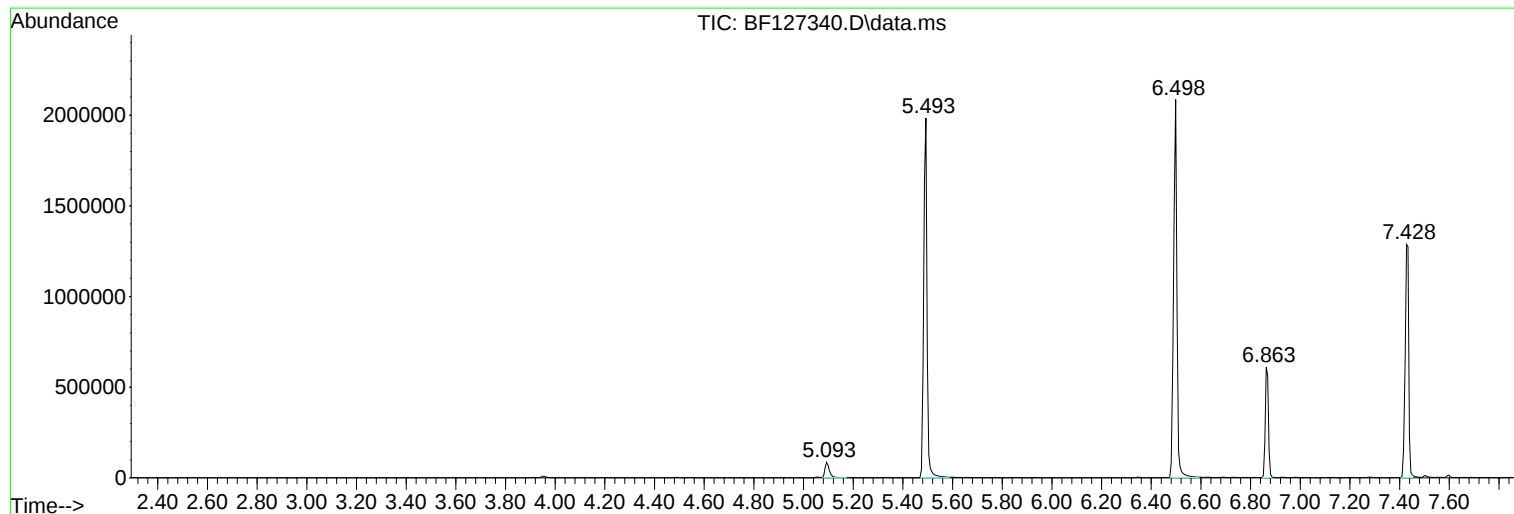

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127340.D
Acq On : 15 Mar 2022 23:06
Operator : CG\JU
Sample : N1948-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-4









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.093	3.91 ng	106334	1,4-Dichlorobenzene-d4	6.869

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59	
2	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28	
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12	
4	2-Propyn-1-ol, acetate	98	C5H6O2	000627-09-8	9	
5	Diacetamide	101	C4H7NO2	000625-77-4	9	

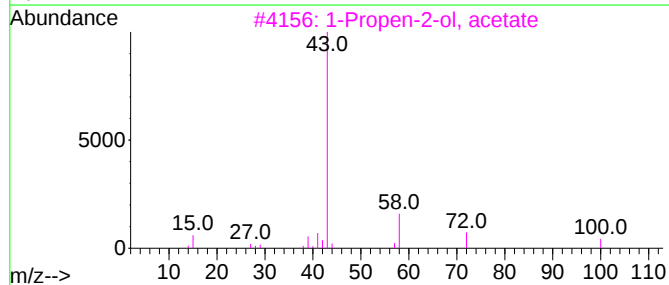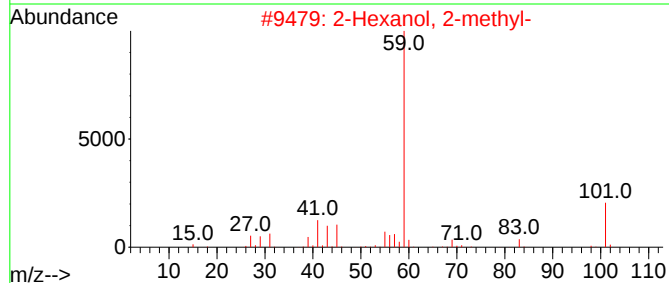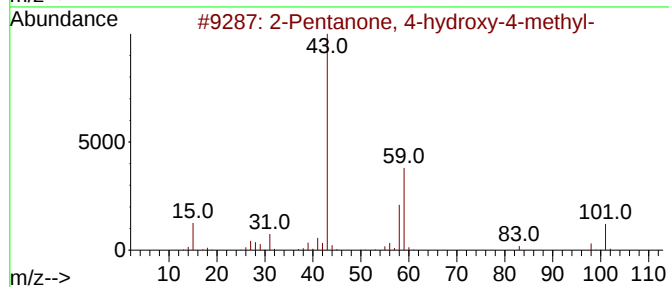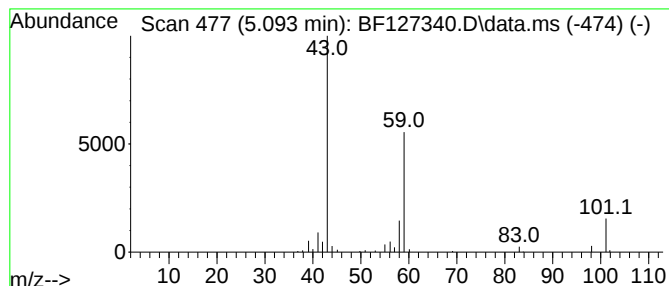

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127340.D
Acq On : 15 Mar 2022 23:06
Operator : CG\JU
Sample : N1948-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.093	3.9	ng	106334	1	6.869	543716	20.0