

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
 Data File : BF127344.D
 Acq On : 16 Mar 2022 01:01
 Operator : CG\JU
 Sample : N1914-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	477	481	489	rVB	21120	29901	1.09%	0.167%
2	5.493	541	545	565	rBV	2373074	2329823	84.99%	13.003%
3	6.498	711	716	719	rBV	2366781	2413980	88.06%	13.473%
4	6.863	775	778	782	rBV	681698	562990	20.54%	3.142%
5	7.434	870	875	878	rBV	1660672	1617870	59.02%	9.030%
6	8.051	977	980	990	rBV	34779	61620	2.25%	0.344%
7	8.145	992	996	1000	rBV	817141	754129	27.51%	4.209%
8	9.222	1174	1179	1183	rBV	2719735	2741401	100.00%	15.300%
9	9.904	1291	1295	1299	rBV	1086659	896932	32.72%	5.006%
10	10.698	1426	1430	1438	rBV	1894852	1762096	64.28%	9.834%
11	11.339	1536	1539	1542	rVB	40029	29398	1.07%	0.164%
12	11.398	1545	1549	1552	rBV	1171848	957324	34.92%	5.343%
13	11.775	1610	1613	1616	rVB	37858	29139	1.06%	0.163%
14	12.616	1752	1756	1759	rBV	49771	48013	1.75%	0.268%
15	12.845	1792	1795	1797	rVB	42735	36375	1.33%	0.203%
16	12.986	1814	1819	1822	rBV	2721695	2491437	90.88%	13.905%
17	13.904	1971	1975	1978	rBV	25937	28473	1.04%	0.159%
18	14.039	1995	1998	2002	rBV	603095	563222	20.55%	3.143%
19	15.527	2246	2251	2259	rBV	470951	563473	20.55%	3.145%




Sum of corrected areas: 17917596

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127344.D
Acq On : 16 Mar 2022 01:01
Operator : CG\JU
Sample : N1914-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

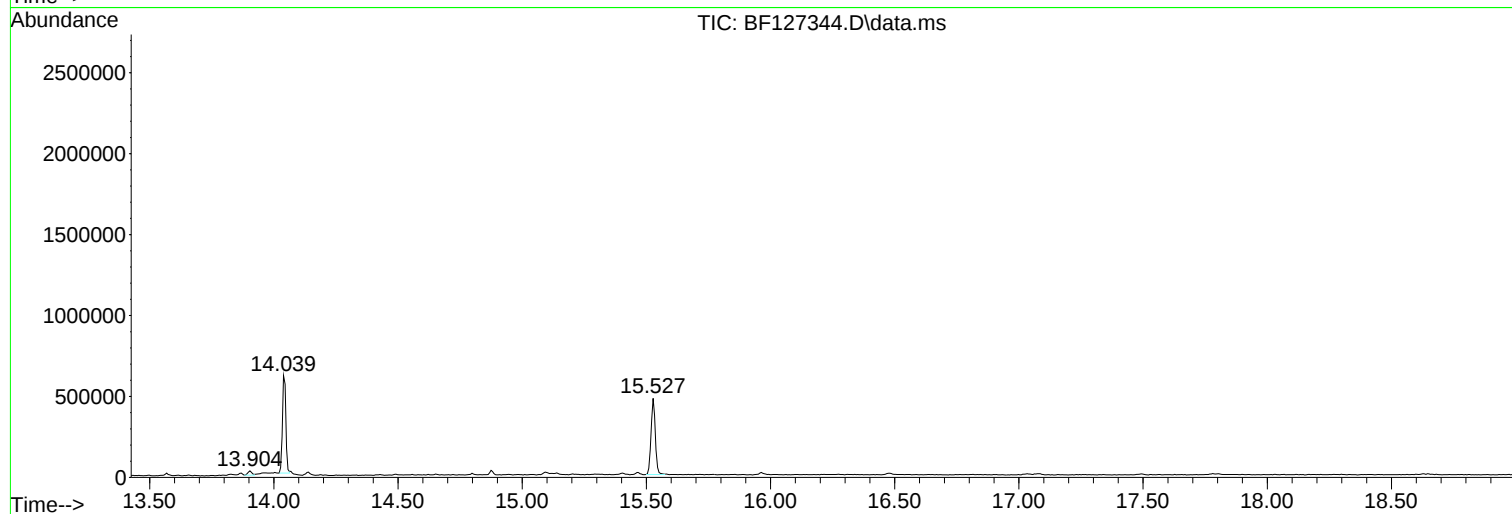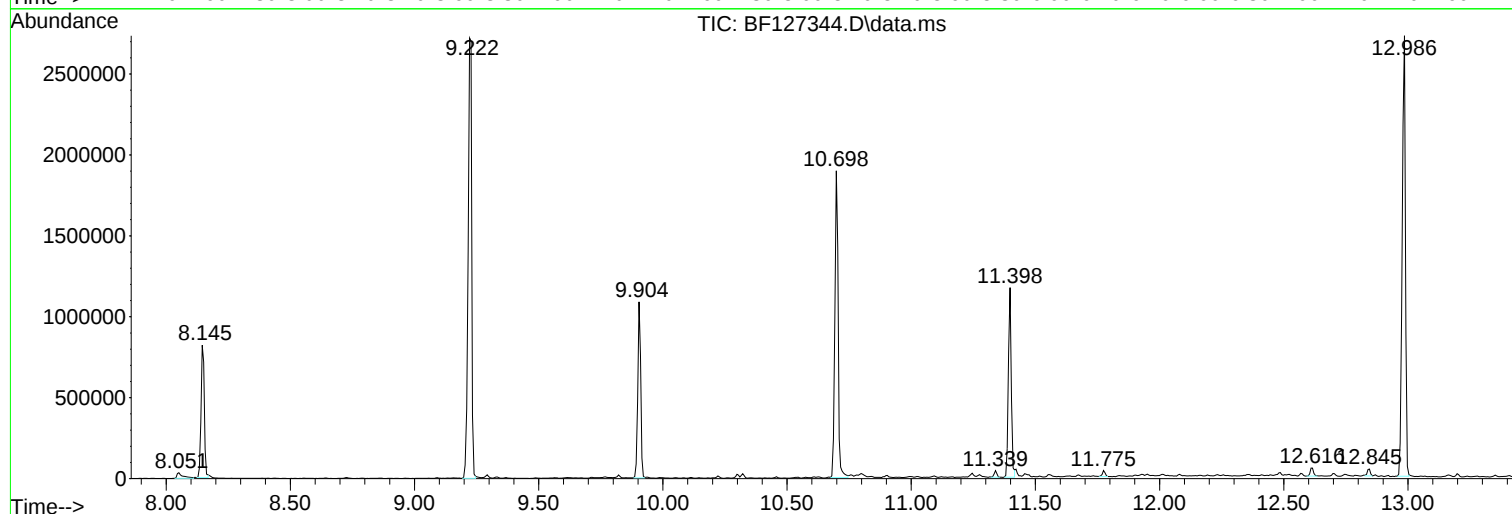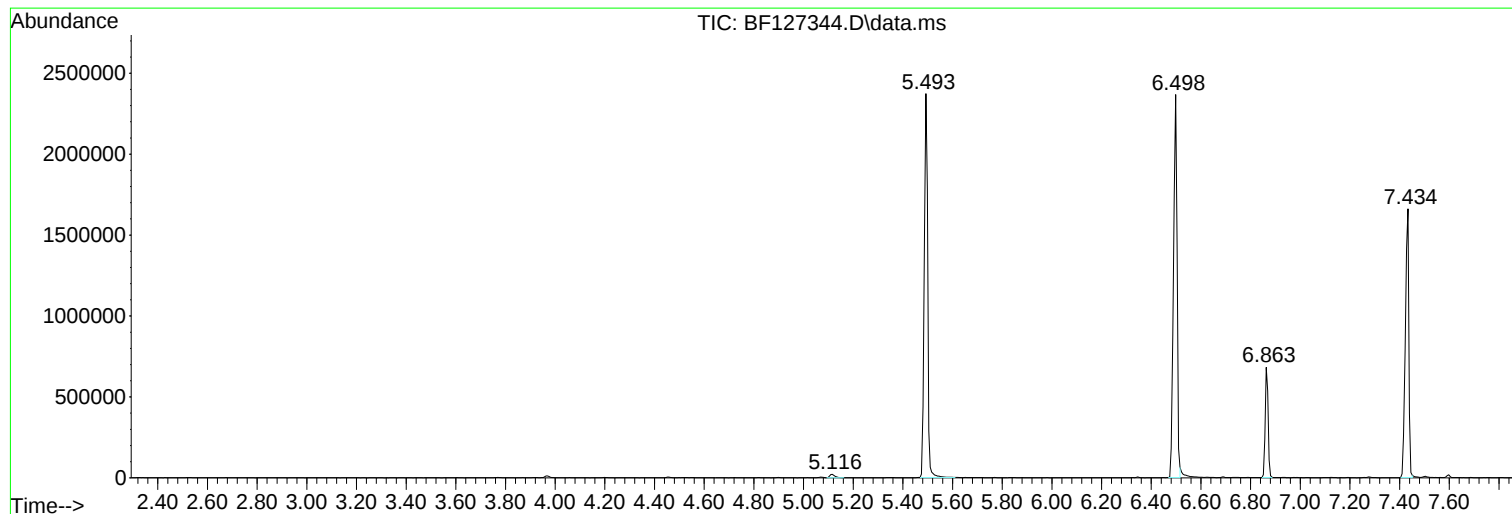

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127344.D
Acq On : 16 Mar 2022 01:01
Operator : CG\JU
Sample : N1914-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127344.D
Acq On : 16 Mar 2022 01:01
Operator : CG\JU
Sample : N1914-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------