
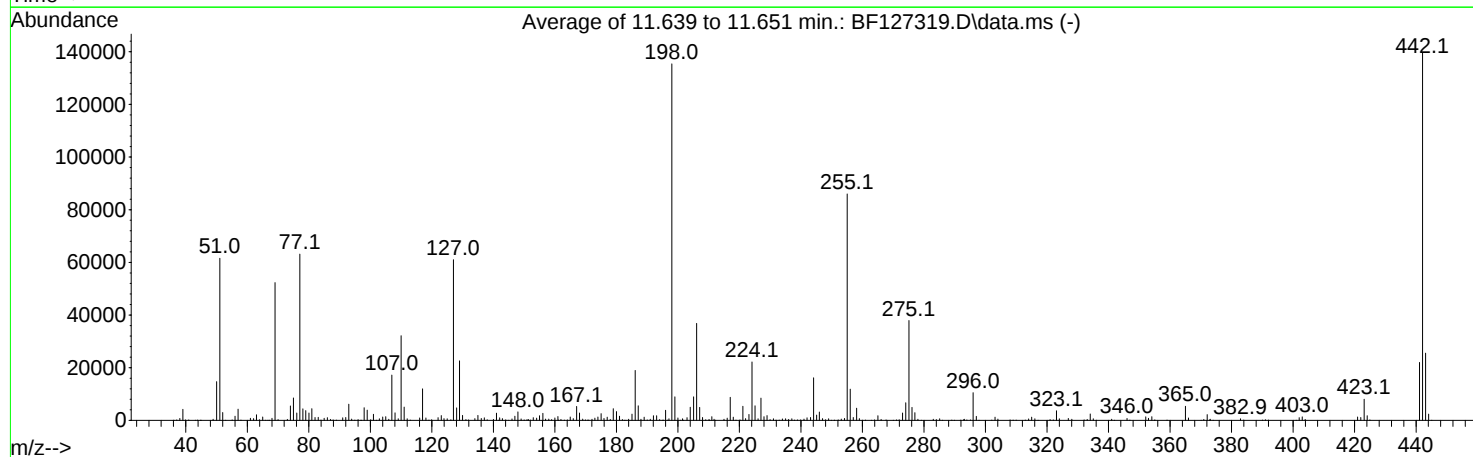


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
 Data File : BF127319.D
 Acq On : 15 Mar 2022 11:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 16:51:53 2022

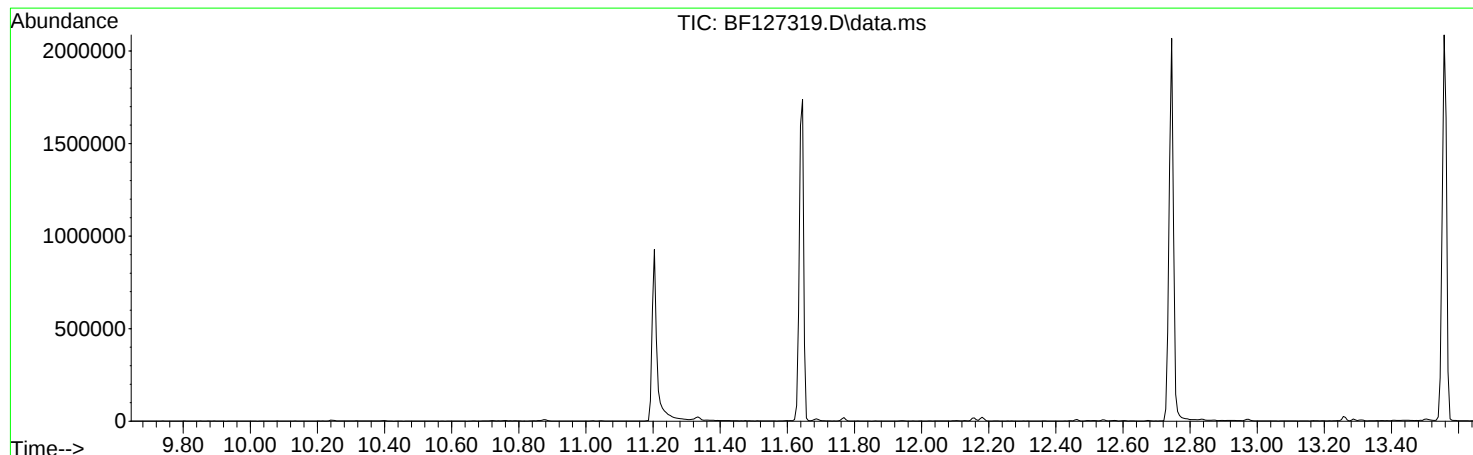

AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	61580	PASS
68	69	0.00	2	1.5	804	PASS
69	198	0.00	100	38.6	52340	PASS
70	69	0.00	2	0.6	299	PASS
127	198	10	80	45.0	60992	PASS
197	198	0.00	2	0.5	618	PASS
198	198	100	100	100.0	135424	PASS
199	198	5	9	6.6	8914	PASS
275	198	10	60	28.0	37956	PASS
365	198	1	100	4.0	5379	PASS
441	198	0.01	100	16.3	22030	PASS
442	442	50	100	100.0	139717	PASS
443	442	15	24	18.3	25511	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/15/2022	BNA_F	<u>BF127319.D</u>
Compound Name	Response	Retention Time
DDT	380014	13.55
DDD	4873	13.26
DDE	269	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5142	385156	1.34

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127319.D
Acq On : 15 Mar 2022 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 15 14:18:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

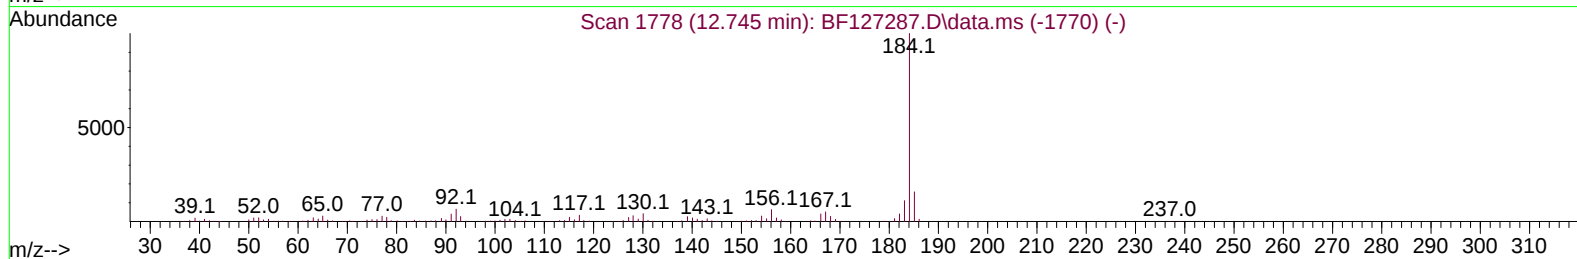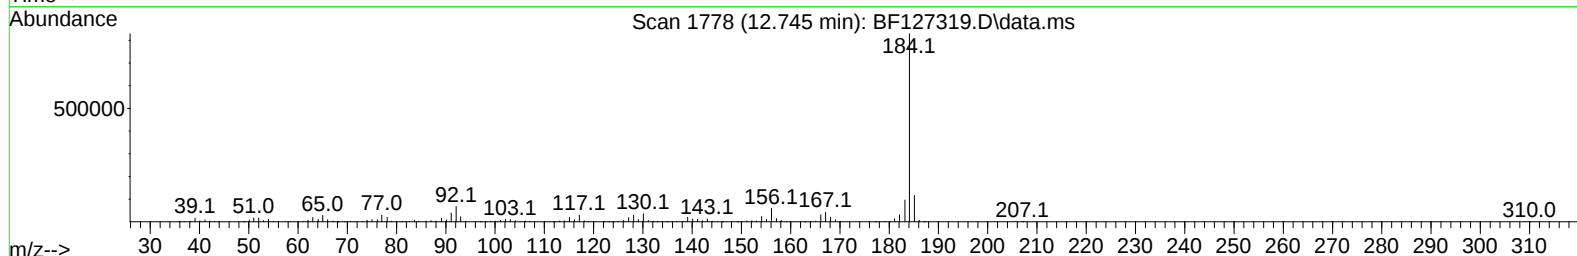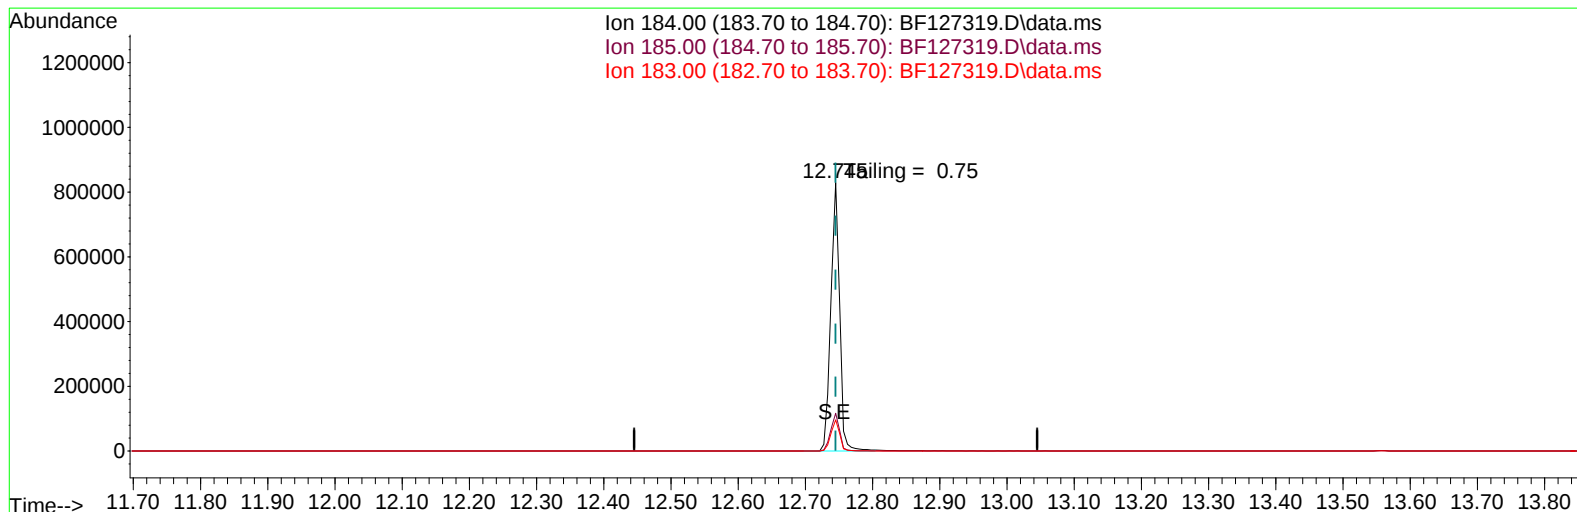

TIC: BF127319.D\data.ms

(77) Benzidine

12.745min (-0.000) 32053.87 ng




response 757254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.08
183.00	10.20	11.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127319.D
Acq On : 15 Mar 2022 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 15 14:18:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

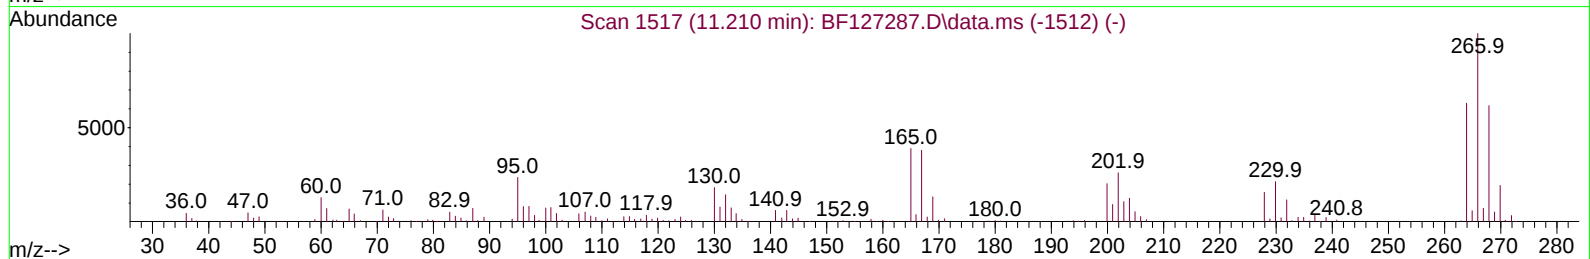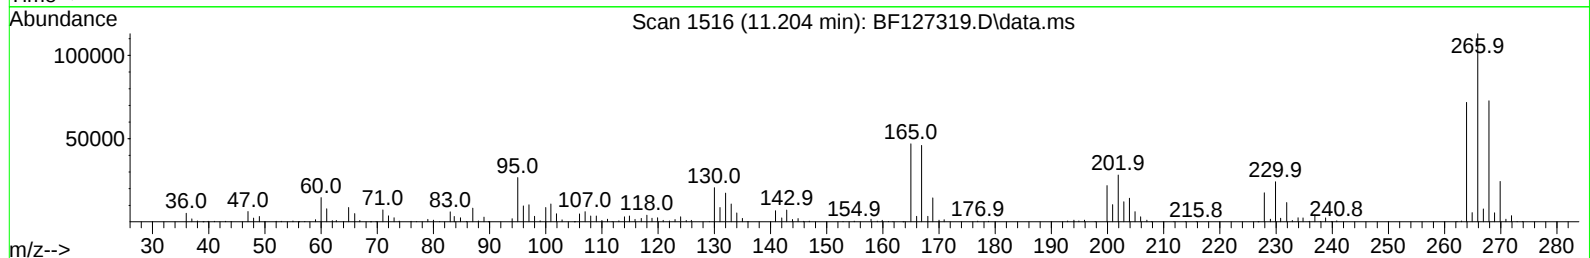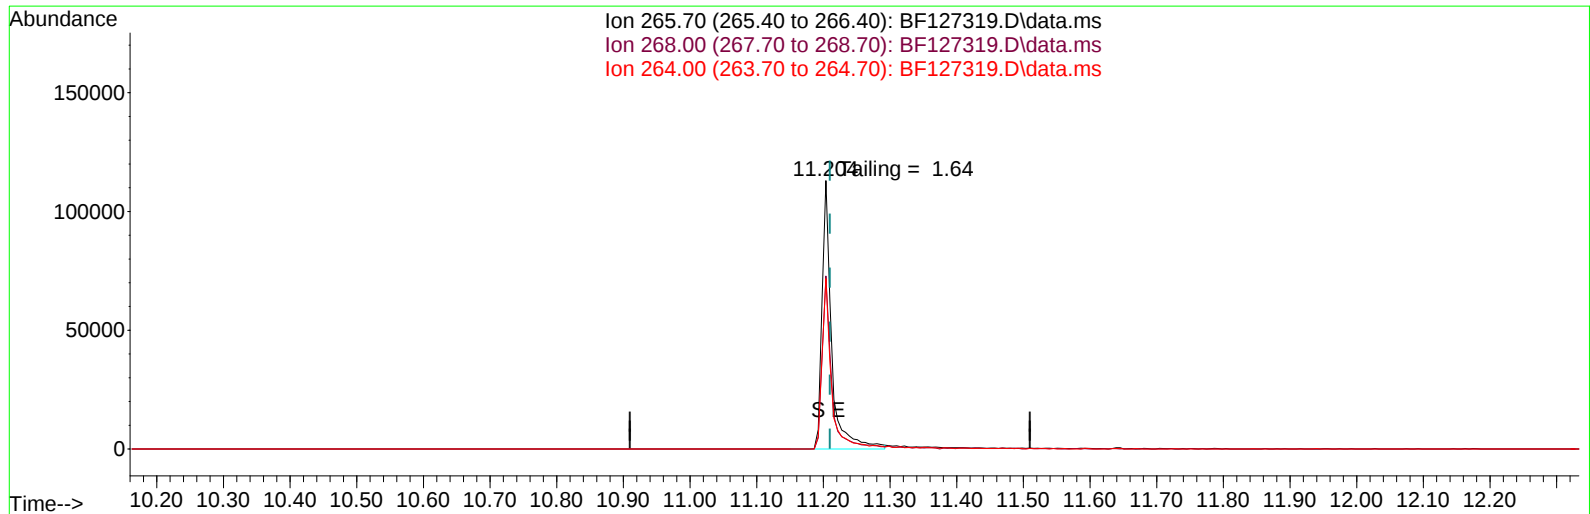

TIC: BF127319.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 394197.19 ng

response 117092

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.43
264.00	63.00	63.50
0.00	0.00	0.00