


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
 Data File : BF127324.D
 Acq On : 15 Mar 2022 15:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 16:51:53 2022

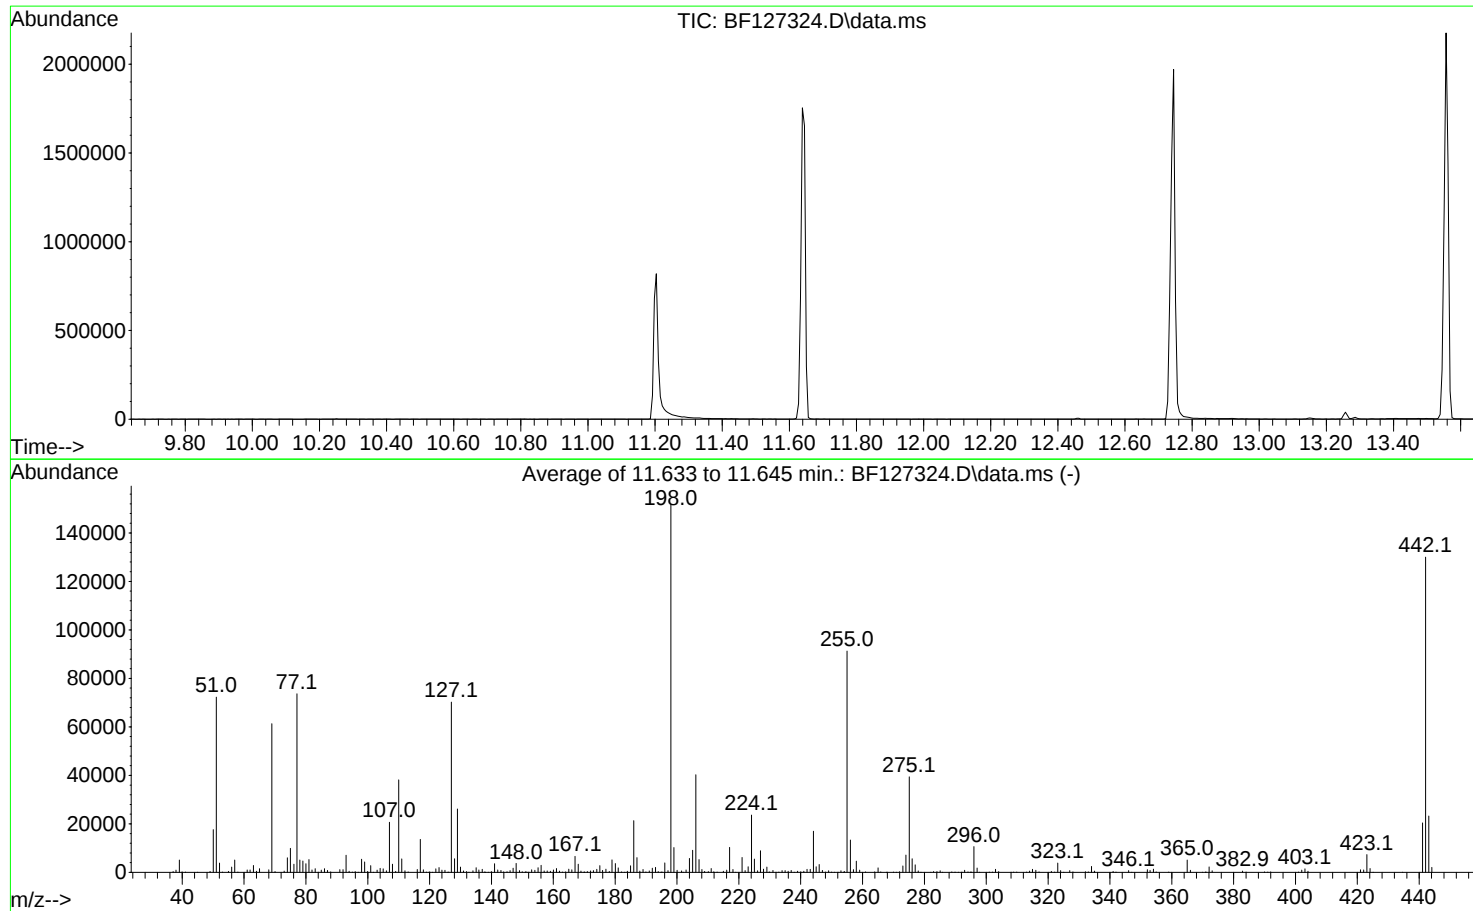




AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	72251	PASS
68	69	0.00	2	1.8	1095	PASS
69	198	0.00	100	40.4	61325	PASS
70	69	0.00	2	0.5	320	PASS
127	198	10	80	46.3	70240	PASS
197	198	0.00	2	0.5	759	PASS
198	198	100	100	100.0	151723	PASS
199	198	5	9	6.7	10212	PASS
275	198	10	60	26.0	39387	PASS
365	198	1	100	3.4	5100	PASS
441	198	0.01	100	13.5	20423	PASS
442	442	50	100	100.0	129984	PASS
443	442	15	24	17.9	23211	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127324.D
Acq On : 15 Mar 2022 15:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 16 06:19:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

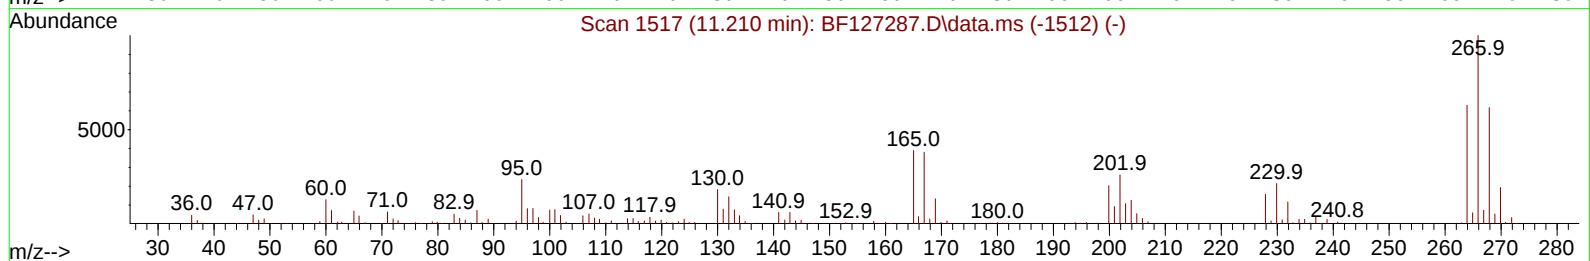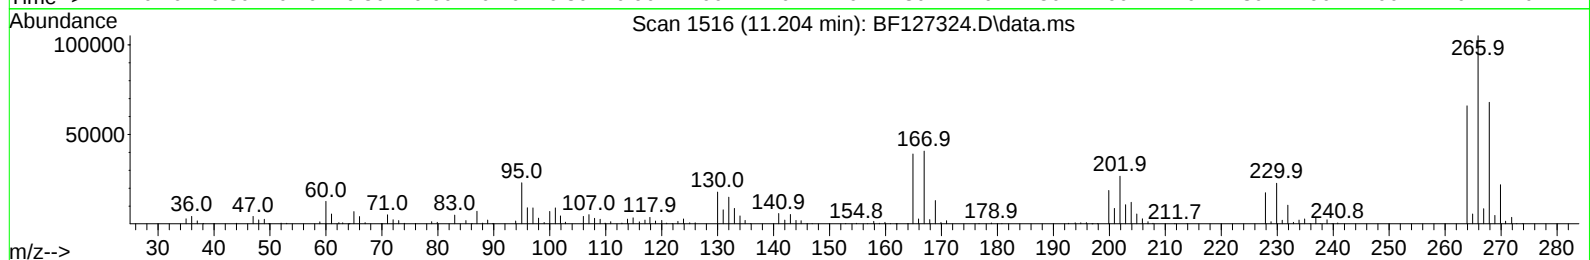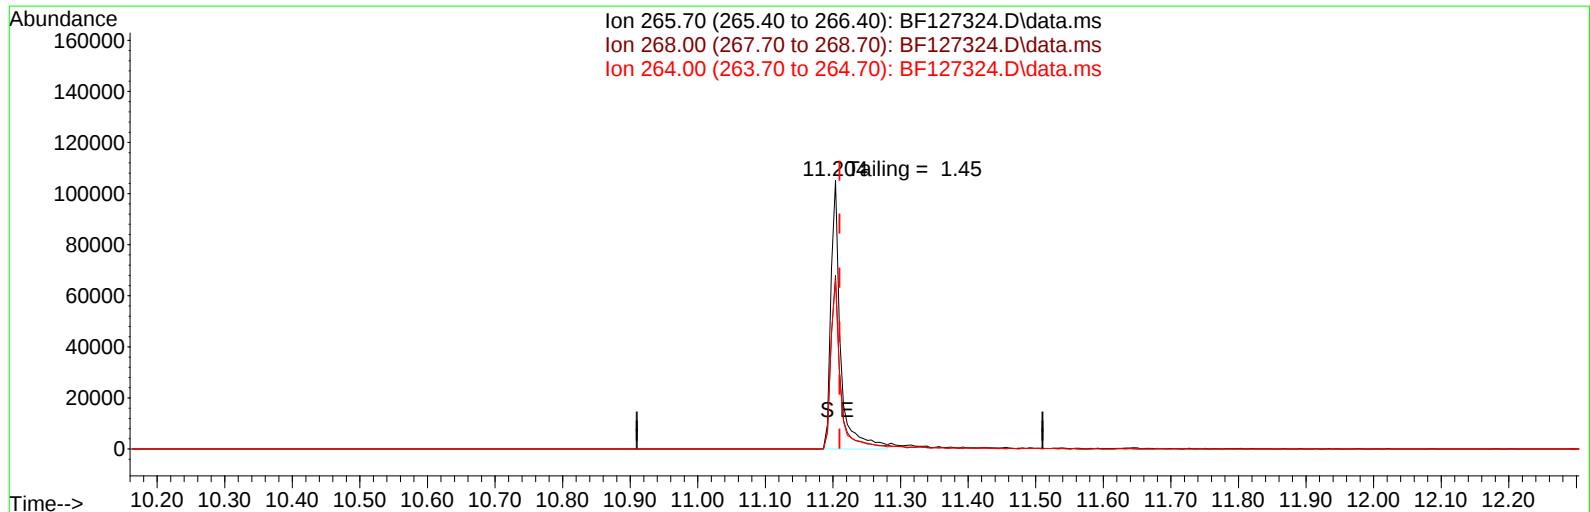

TIC: BF127324.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 34076.55 ng




response 106824

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.63
264.00	63.00	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031522\
Data File : BF127324.D
Acq On : 15 Mar 2022 15:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 16 06:19:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 16:51:53 2022
Response via : Initial Calibration

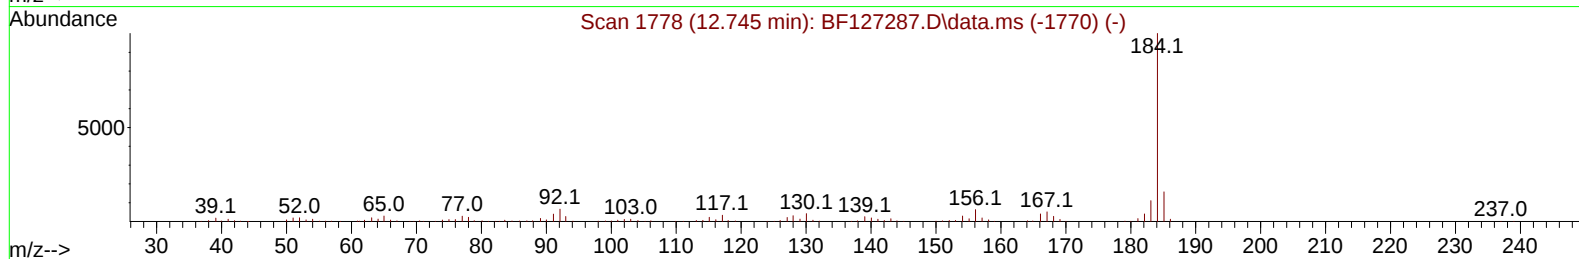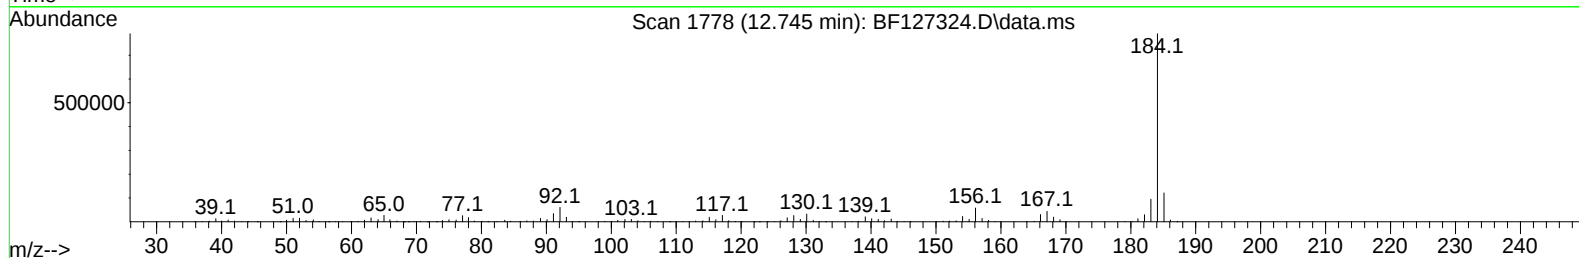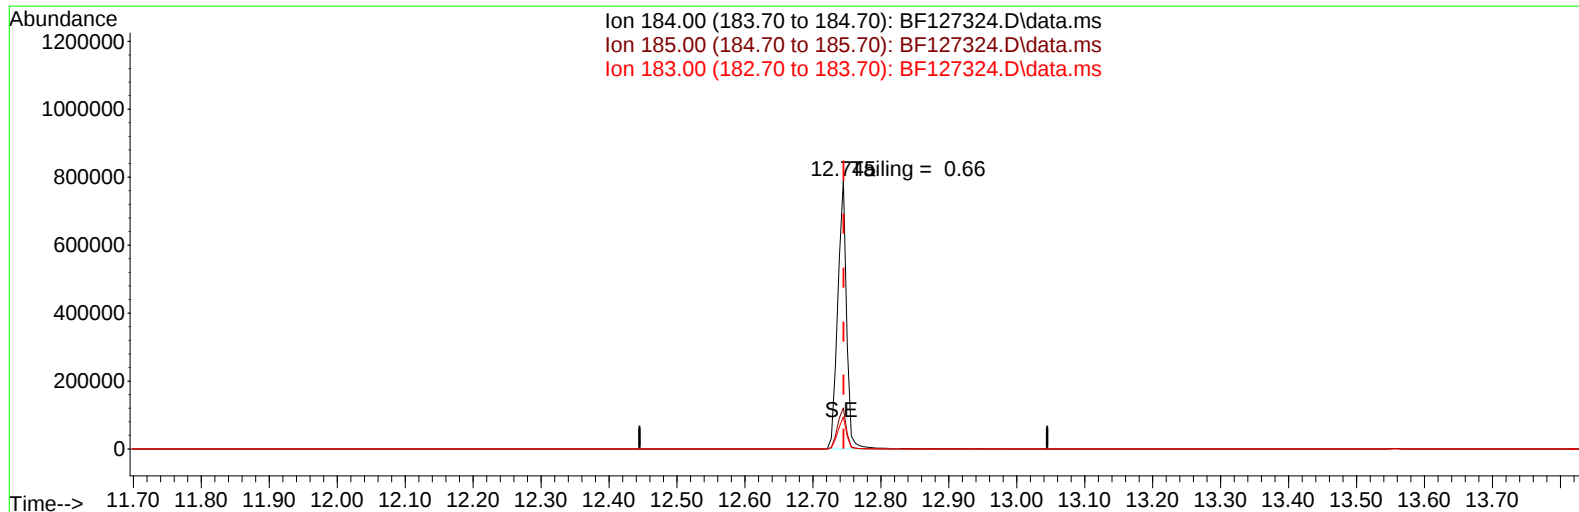

TIC: BF127324.D\data.ms

(77) Benzidine

12.745min (-0.000) 0.00 ng

response 713733

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.32
183.00	10.20	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/15/2022	BNA_F	<u>BF127324.D</u>
Compound Name	Response	Retention Time
DDT	379180	13.557
DDD	9167	13.257
DDE	407	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9574	388754	2.46

Instrument :
BNA_F
ClientSampleId :
DFTPP