
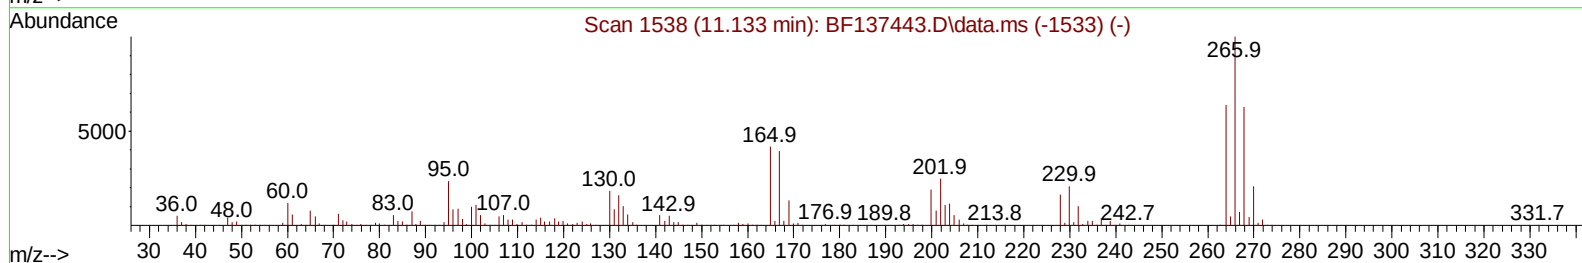
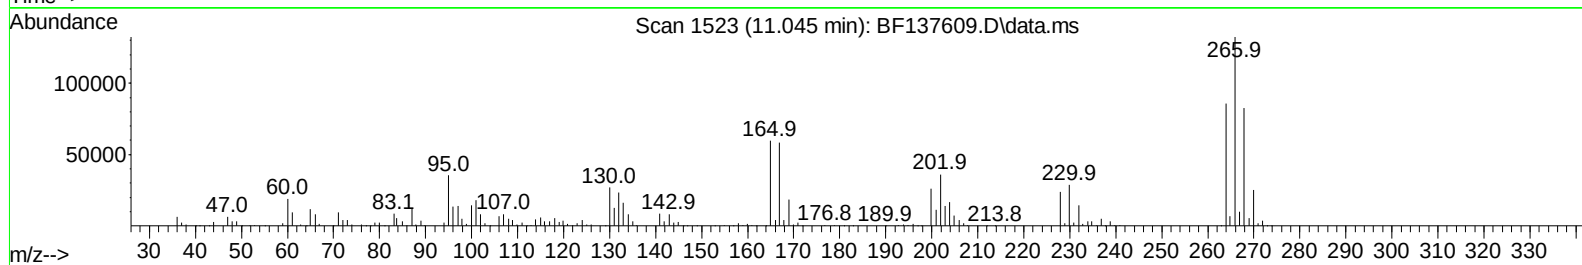


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031524\
Data File : BF137609.D
Acq On : 15 Mar 2024 13:52
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 00:12:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

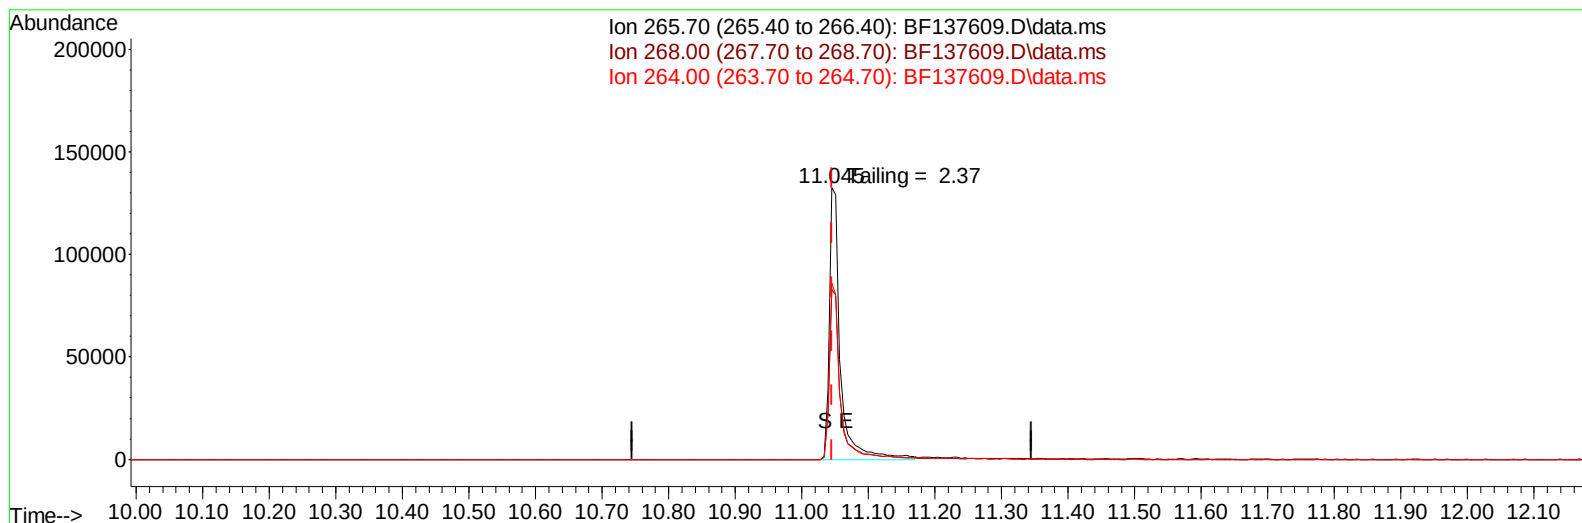

TIC: BF137609.D\data.ms

(70) Pentachlorophenol (C)




11.045min (-0.000) 33669.70 ng

response 154051

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.51
264.00	63.60	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031524\
Data File : BF137609.D
Acq On : 15 Mar 2024 13:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 00:12:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

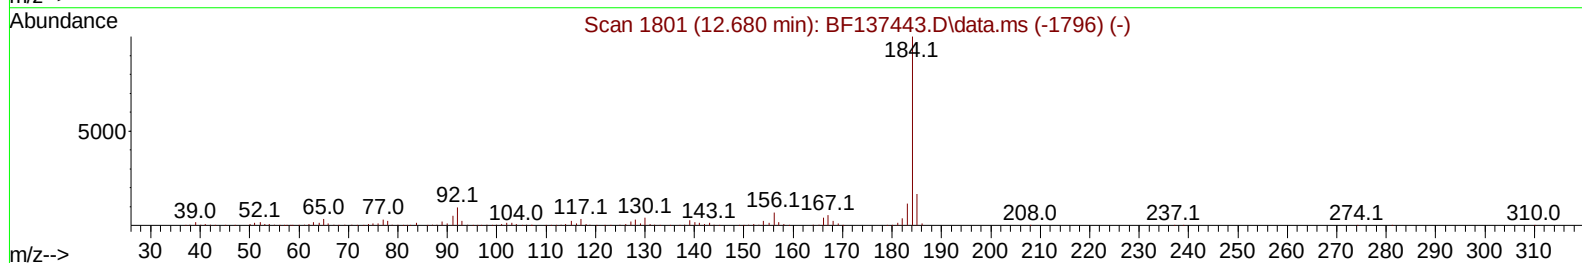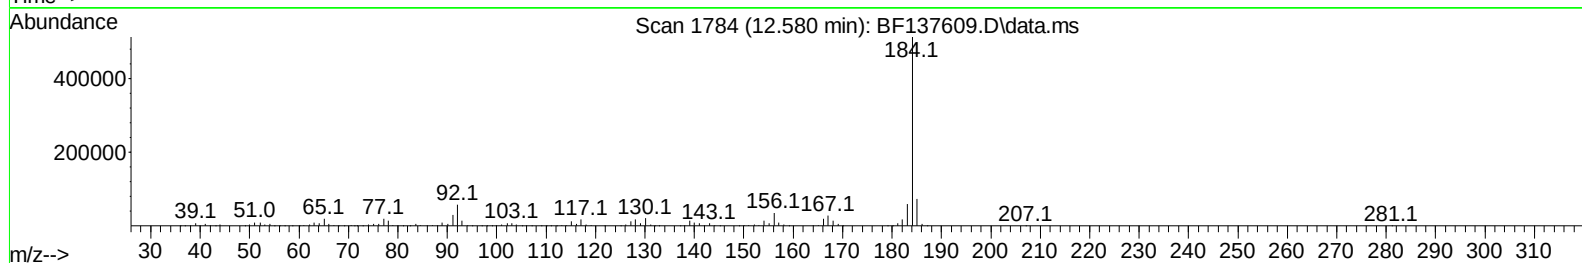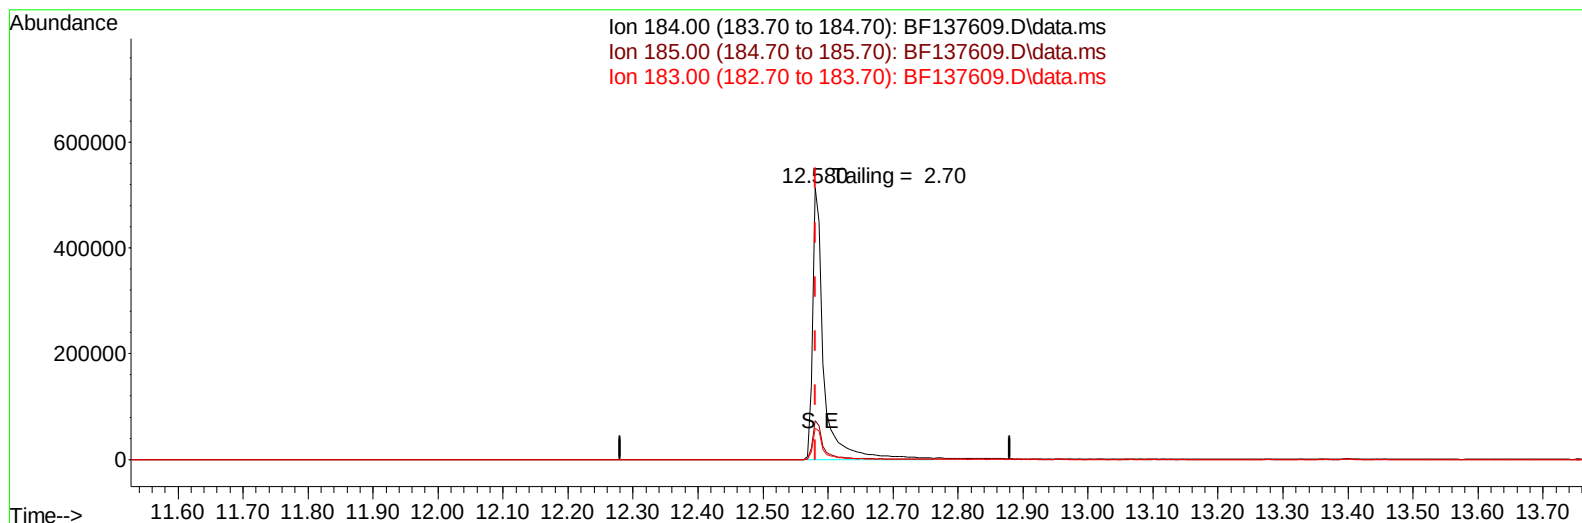

TIC: BF137609.D\data.ms

(77) Benzidine

12.580min (-0.000) 0.00 ng

response 609901

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.38
183.00	11.60	11.44
0.00	0.00	0.00