


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031524\
Data File : BF137609.D
Acq On : 15 Mar 2024 13:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 14:45:20 2024

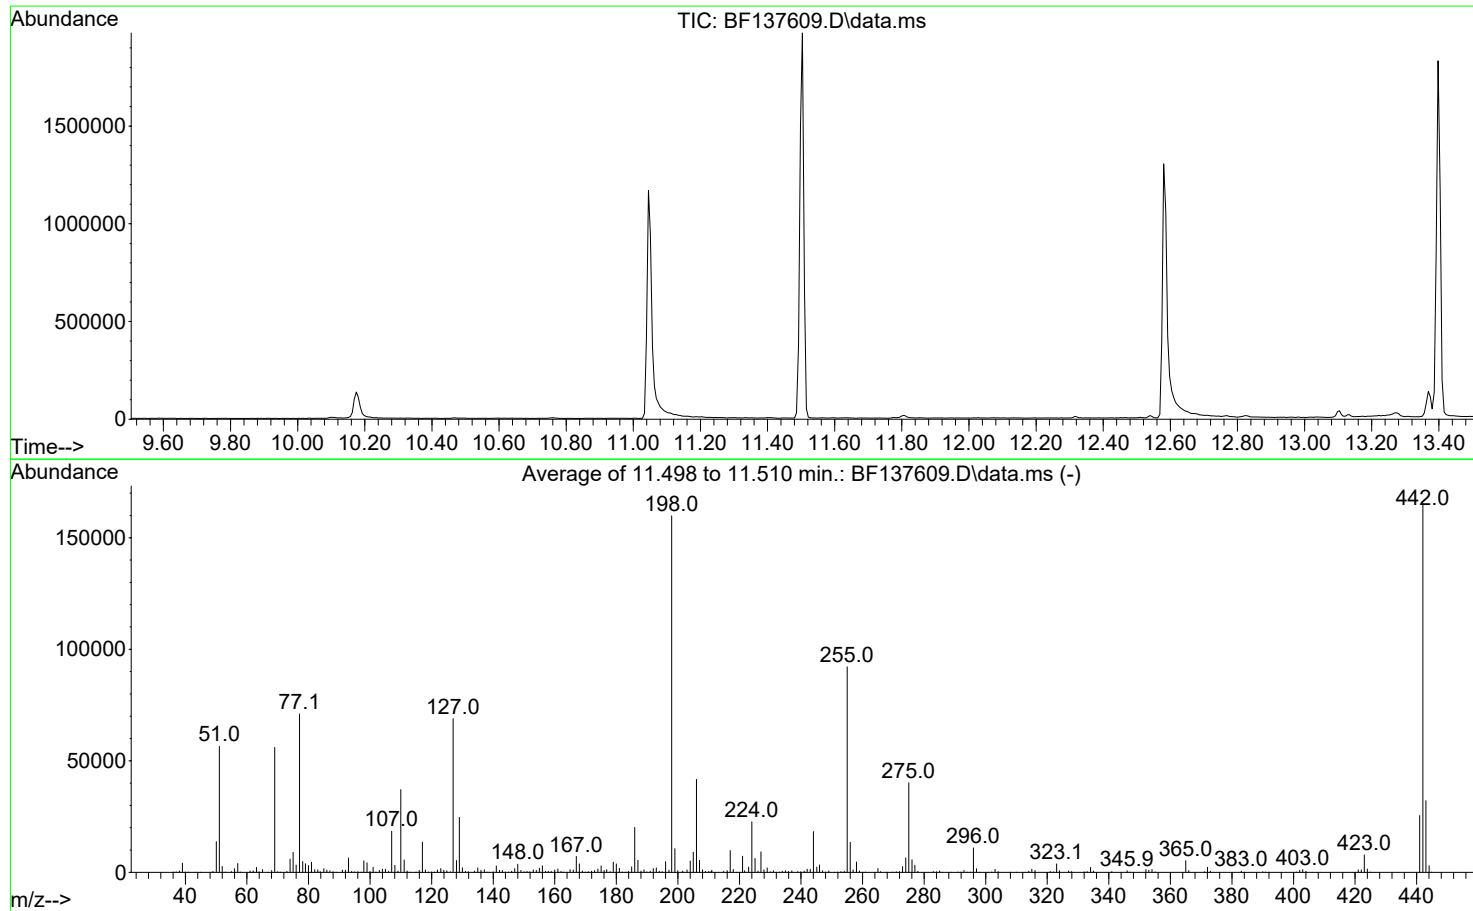

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	56472	PASS
68	69	0.00	2	1.4	790	PASS
69	198	0.00	100	35.0	56007	PASS
70	69	0.00	2	0.5	302	PASS
127	198	10	80	43.1	68904	PASS
197	198	0.00	2	0.6	1025	PASS
198	198	100	100	100.0	159851	PASS
199	198	5	9	6.7	10648	PASS
275	198	10	60	25.1	40149	PASS
365	198	1	100	3.3	5249	PASS
441	198	0.01	100	15.9	25447	PASS
442	442	50	100	100.0	164912	PASS
443	442	15	24	19.5	32165	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/15/2024	BNA_F	<u>BF137609.D</u>
Compound Name	Response	Retention Time
DDT	290744	13.398
DDD	8640	13.104
DDE	973	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9613	300357	3.20

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031524\
Data File : BF137609.D
Acq On : 15 Mar 2024 13:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 16 00:12:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

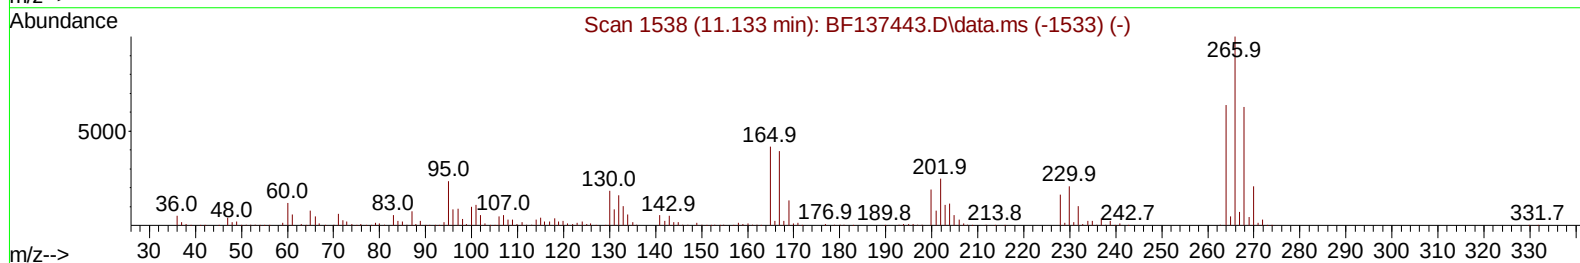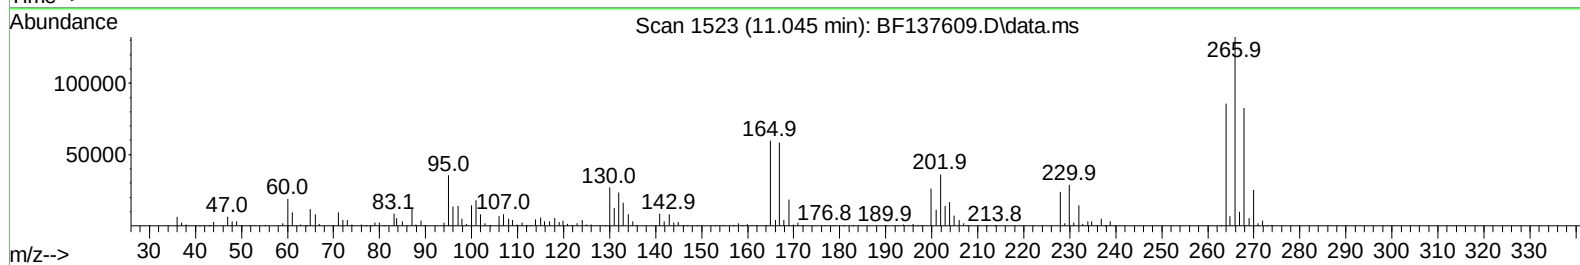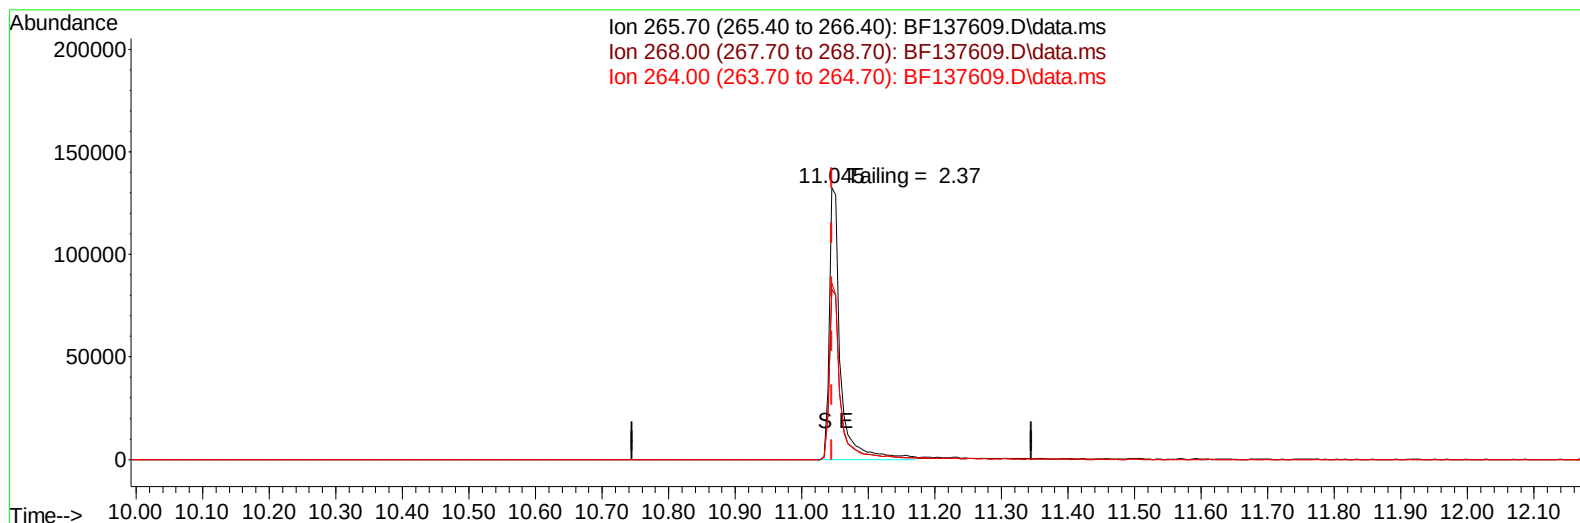

TIC: BF137609.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.000) 33669.70 ng




response 154051

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.51
264.00	63.60	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031524\
Data File : BF137609.D
Acq On : 15 Mar 2024 13:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 16 00:12:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

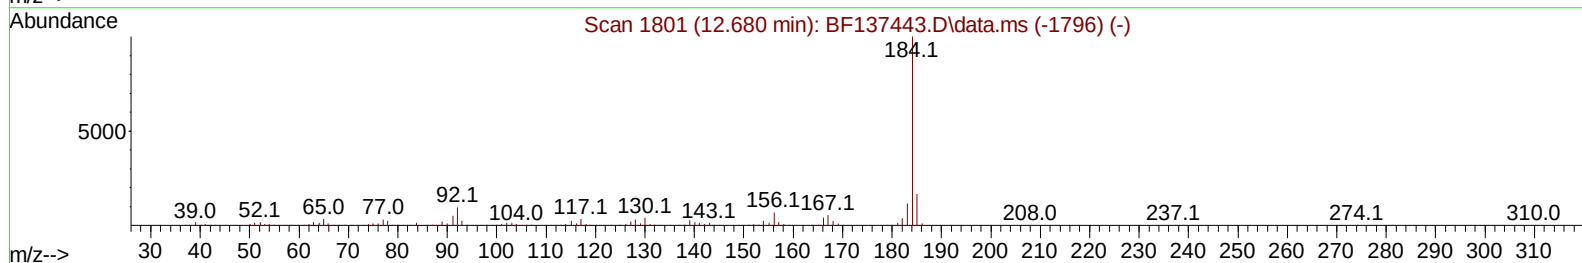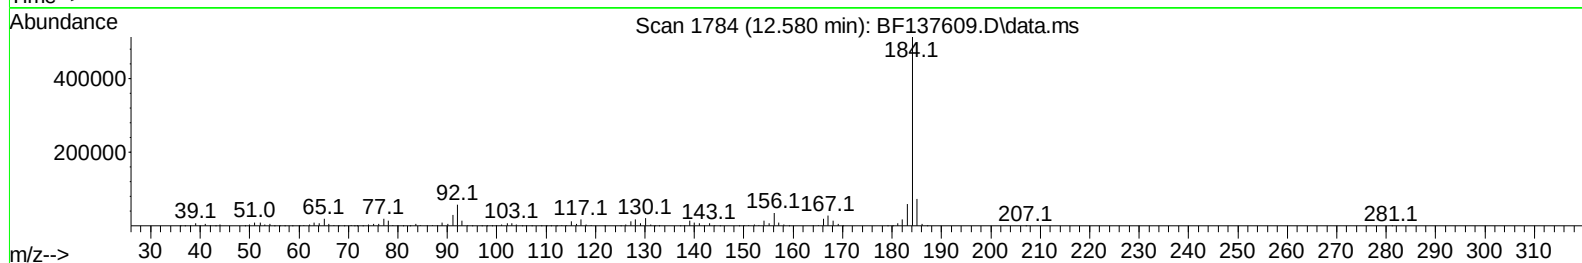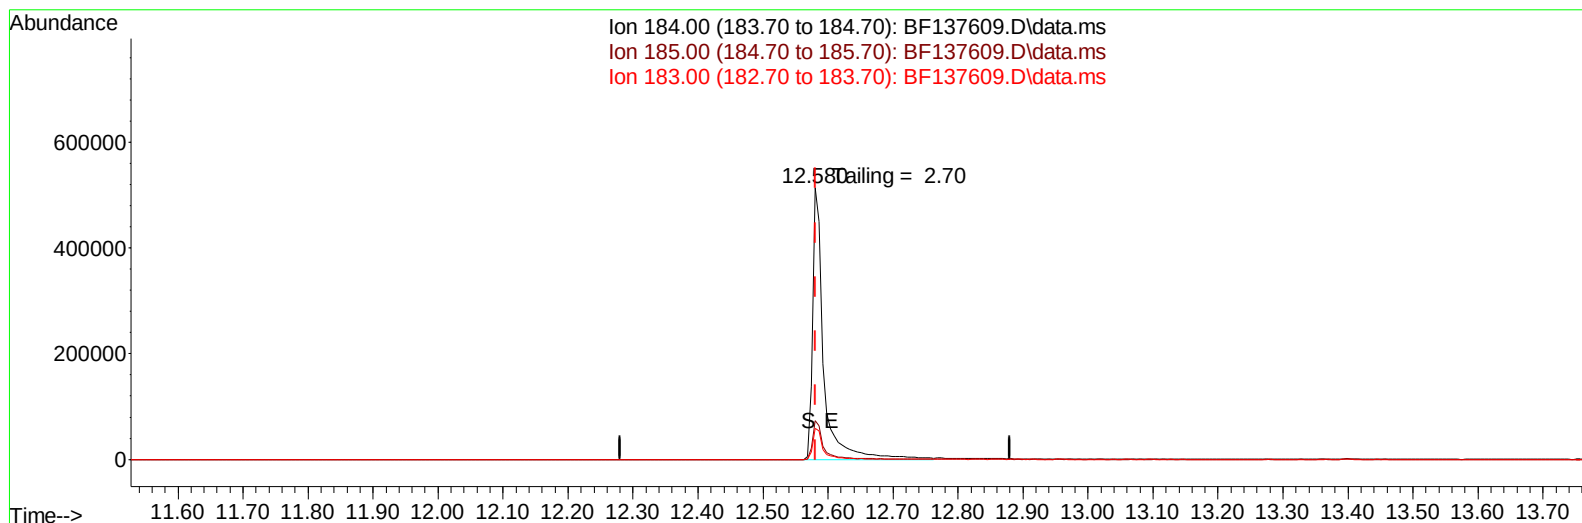

TIC: BF137609.D\data.ms

(77) Benzidine

12.580min (-0.000) 0.00 ng

response 609901

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.38
183.00	11.60	11.44
0.00	0.00	0.00