

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031616\
 Data File : BF085489.D
 Acq On : 17 Mar 2016 4:20
 Operator : UM/SJ
 Sample : H1803-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-01

Quant Time: Mar 17 03:48:23 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 18:57:05 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	125813	20.00	ng	-0.01
21) Naphthalene-d8	8.18	136	518478	20.00	ng	-0.02
38) Acenaphthene-d10	9.94	164	221097	20.00	ng	-0.01
63) Phenanthrene-d10	11.43	188	357534	20.00	ng	-0.01
75) Chrysene-d12	14.06	240	244289	20.00	ng	-0.02
86) Perylene-d12	15.51	264	266639	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	15697	2.14	ng	-0.01
7) Phenol-d6	6.52	99	22282	2.35	ng	-0.03
23) Nitrobenzene-d5	7.46	82	12134	1.38	ng	-0.02
41) 2,4,6-Tribromophenol	10.73	330	2977	1.46	ng	-0.02
44) 2-Fluorobiphenyl	9.26	172	26973	2.12	ng	-0.02
78) Terphenyl-d14	13.01	244	16012	1.48	ng	-0.02
Target Compounds						
50) 2,6-Dinitrotoluene	9.94	165	27623	7.75	ng	# 26
56) 2,4-Dinitrotoluene	9.94	165	27623	6.18	ng	# 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031616\
Data File : BF085489.D
Acq On : 17 Mar 2016 4:20
Operator : UM/SJ
Sample : H1803-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-01

Quant Time: Mar 17 03:48:23 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

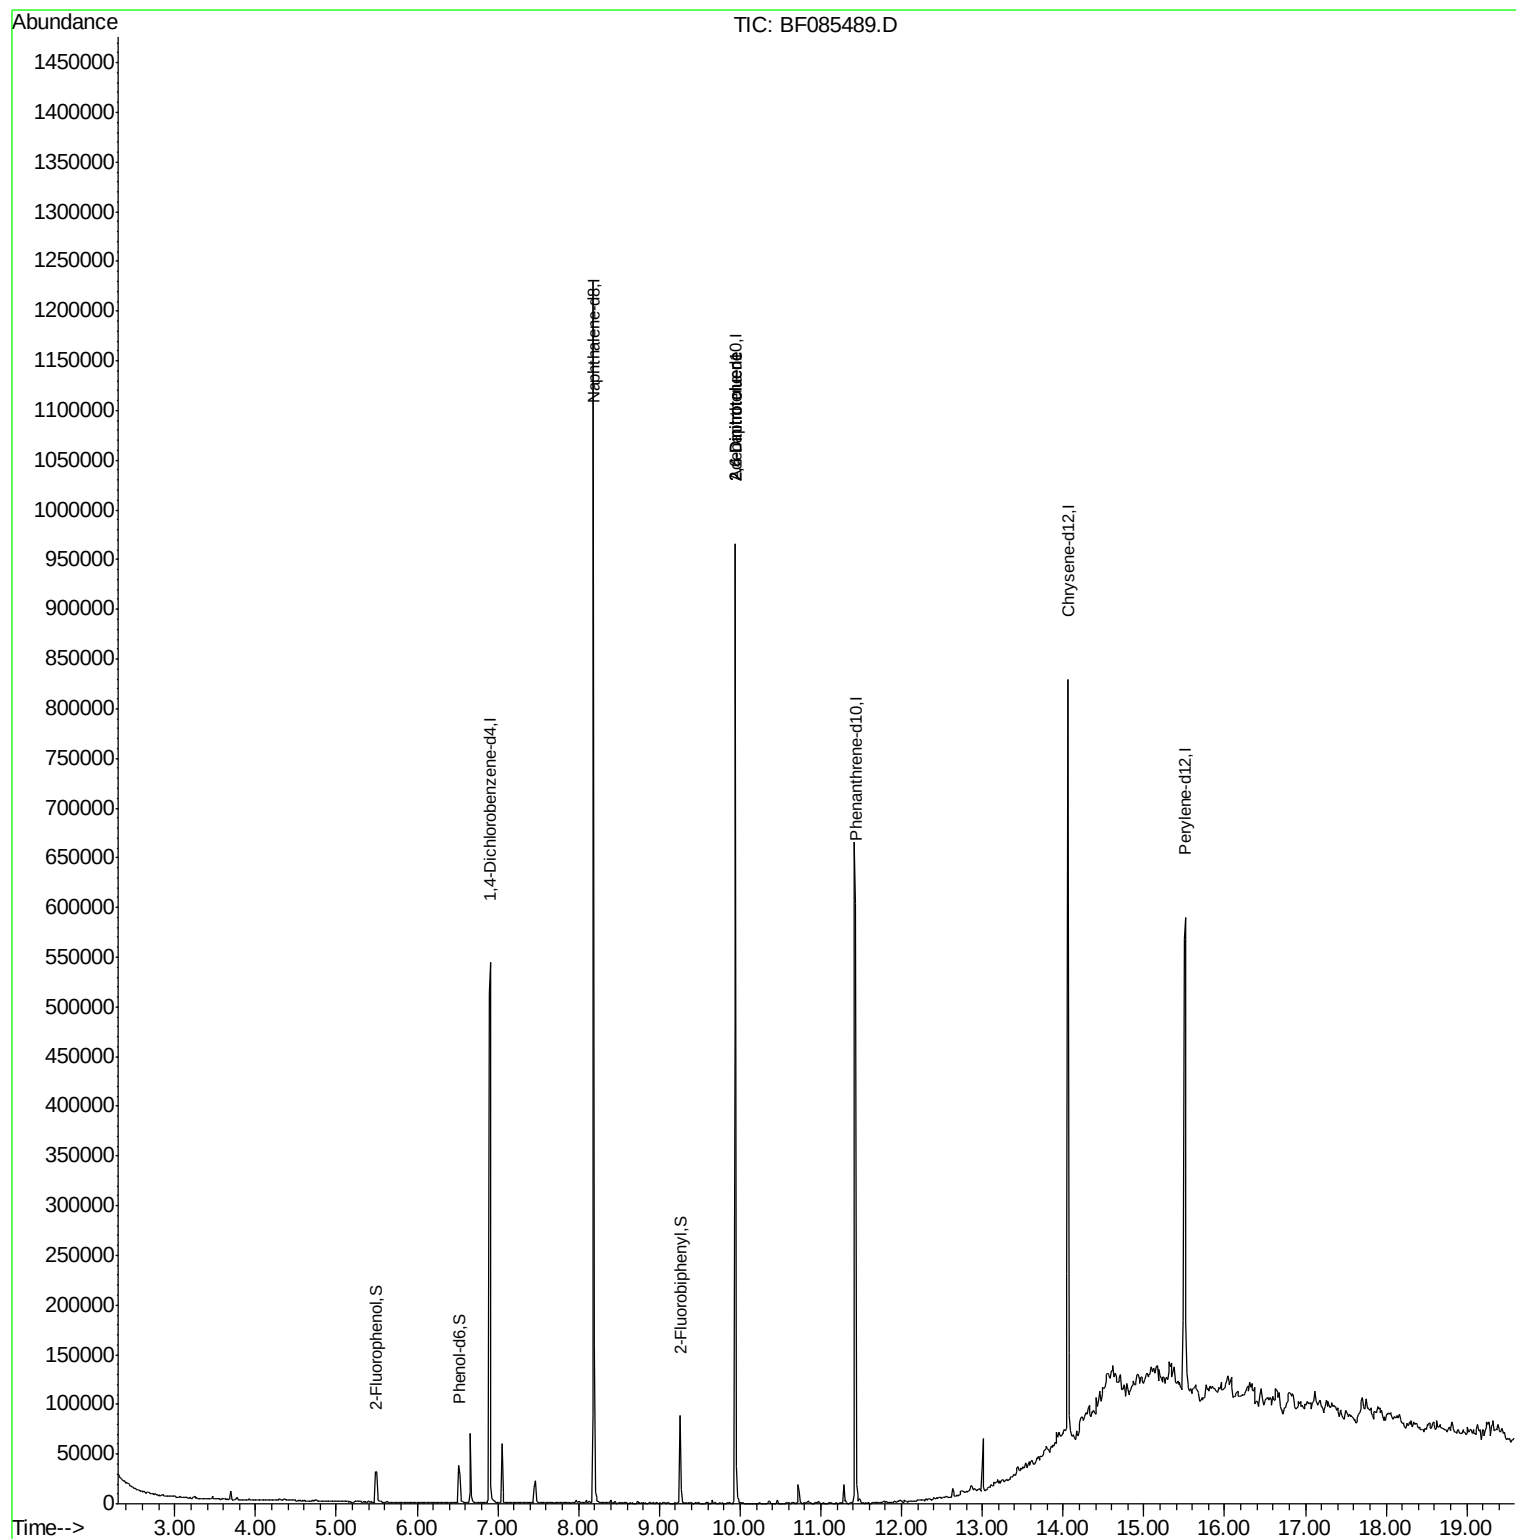

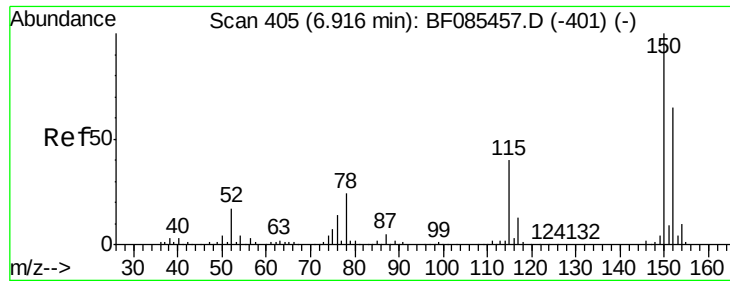

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.90 min Scan# 404

Delta R.T. -0.01 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20

Instrument :

BNA_F

ClientSampleId :

SP-01


Tgt Ion:152 Resp: 125813

Ion Ratio Lower Upper

152 100

150 152.5 124.6 186.8




115 52.6 46.6 70.0

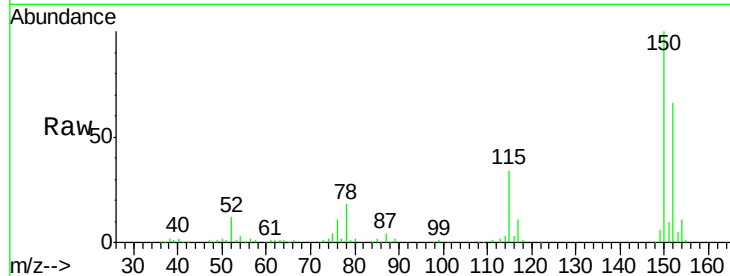

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

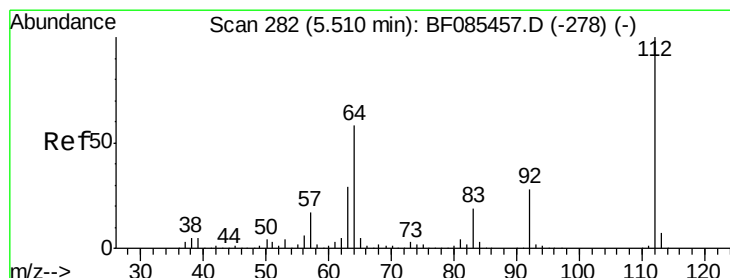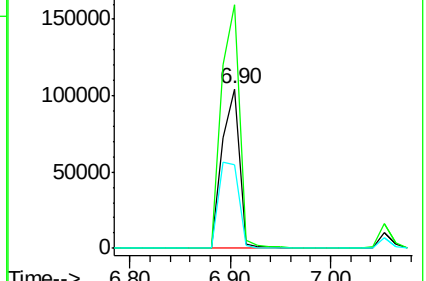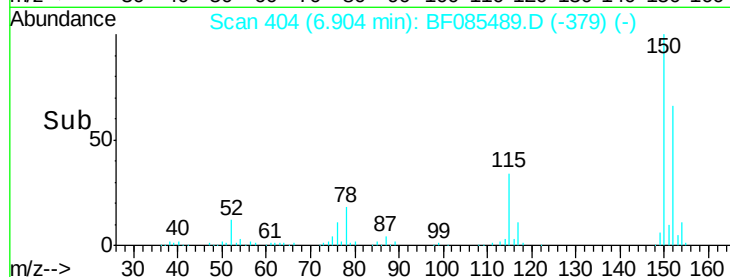

#5

2-Fluorophenol

Concen: 2.14 ng

RT: 5.50 min Scan# 281

Delta R.T. -0.01 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20


Tgt Ion:112 Resp: 15697

Ion Ratio Lower Upper

112 100

64 43.4 49.0 73.4#



63 25.0 24.8 37.2

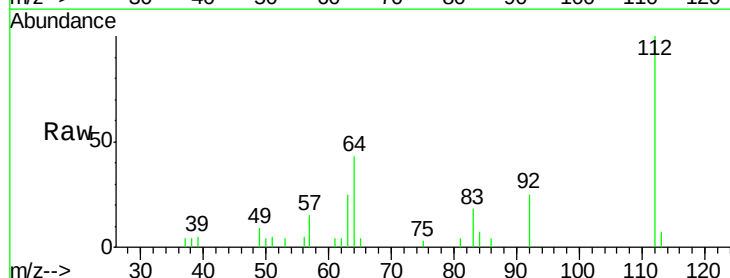


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

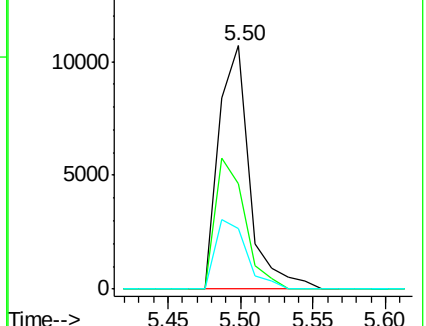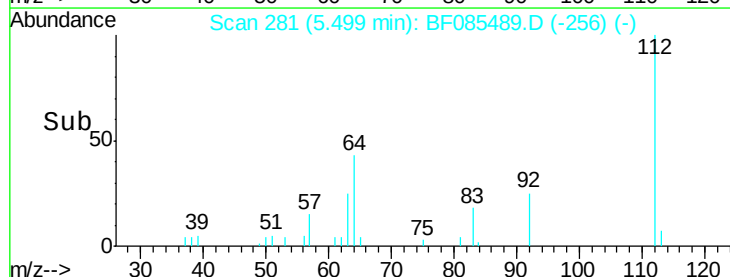

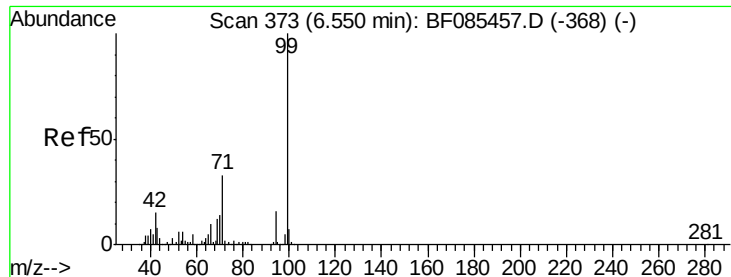

#7

Phenol-d6

Concen: 2.35 ng

RT: 6.52 min Scan# 370

Delta R.T. -0.03 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20

Instrument :

BNA_F

ClientSampleId :

SP-01


Tgt Ion: 99 Resp: 22282

Ion Ratio Lower Upper

99 100

42 22.3 13.6 20.4#




71 35.1 26.7 40.1



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

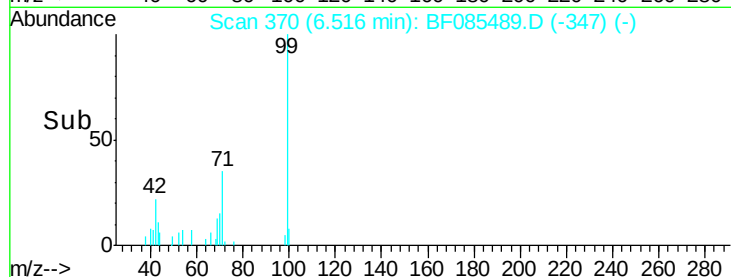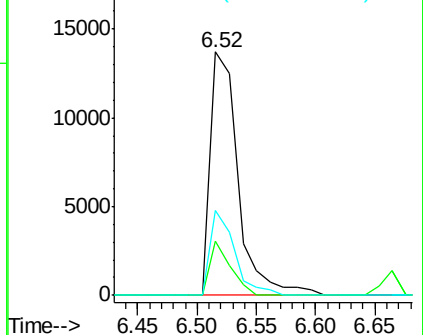

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 516

Delta R.T. -0.02 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20

Tgt Ion: 136 Resp: 518478


Ion Ratio Lower Upper

136 100

137 11.3 9.3 13.9

54 7.4 7.4 11.2#

68 6.2 6.0 9.0






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



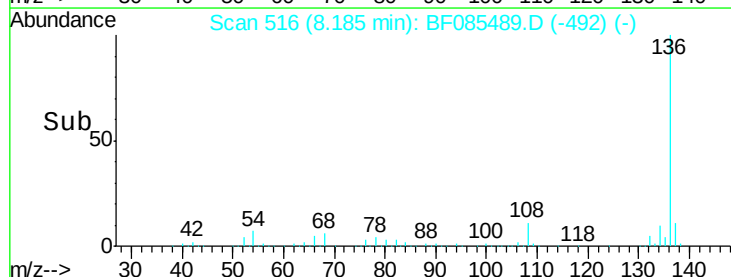
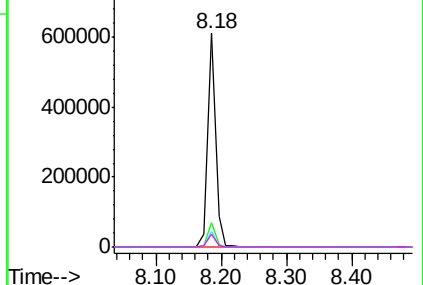


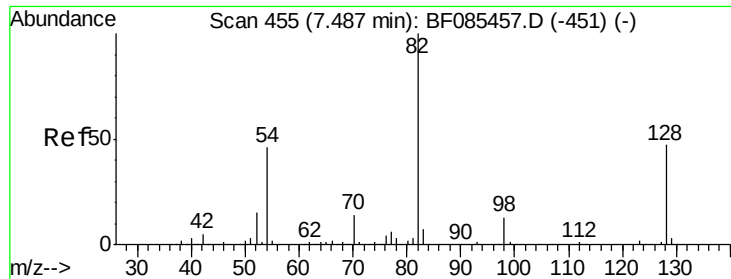

#23
 Nitrobenzene-d5
 Concen: 1.38 ng
 RT: 7.46 min Scan# 453
 Delta R.T. -0.02 min
 Lab File: BF085489.D
 Acq: 17 Mar 2016 4:20




Instrument :
 BNA_F
 ClientSampleId :
 SP-01


Tgt Ion: 82 Resp: 12134
 Ion Ratio Lower Upper
 82 100
 128 48.0 34.5 51.7
 54 42.8 39.3 58.9

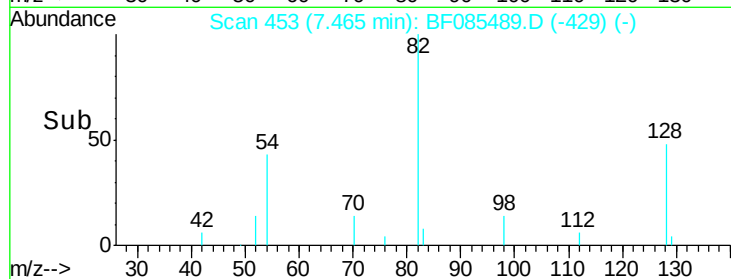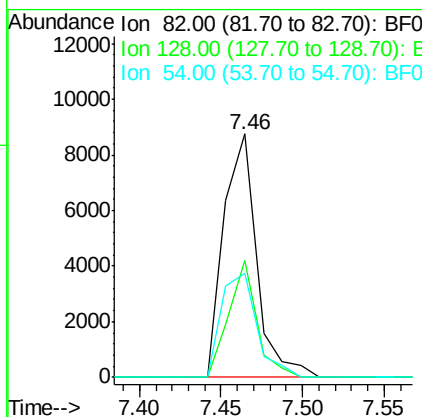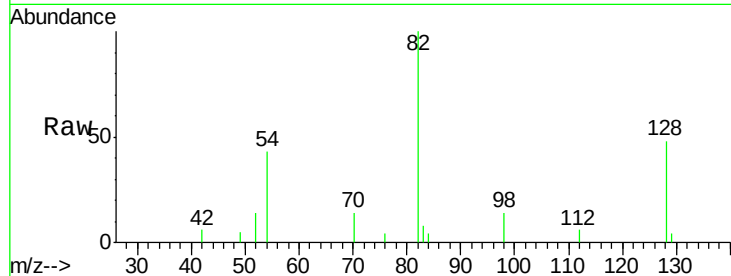

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.94 min Scan# 670
 Delta R.T. -0.01 min
 Lab File: BF085489.D
 Acq: 17 Mar 2016 4:20

Tgt Ion: 164 Resp: 221097
 Ion Ratio Lower Upper
 164 100
 162 103.9 83.3 124.9
 160 48.7 37.9 56.9


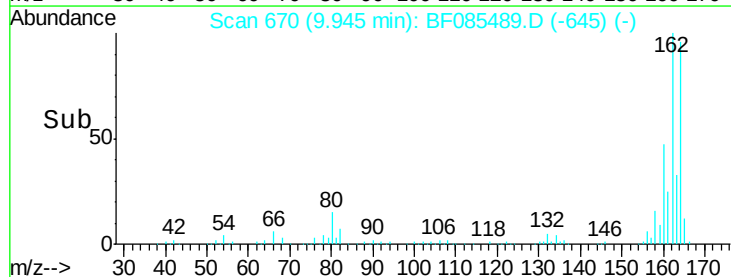
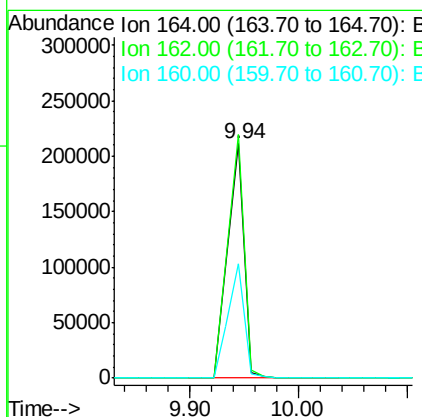



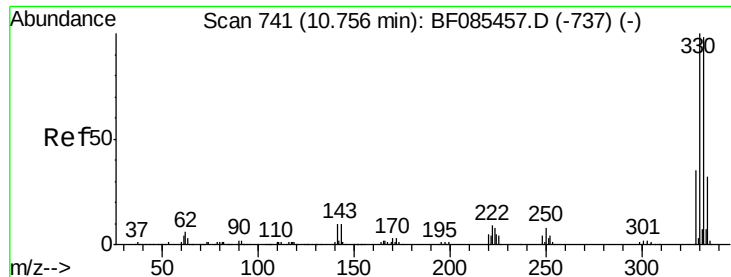

#41
 2,4,6-Tribromophenol
 Concen: 1.46 ng
 RT: 10.73 min Scan# 739
 Delta R.T. -0.02 min
 Lab File: BF085489.D
 Acq: 17 Mar 2016 4:20




Instrument :
 BNA_F
 ClientSampleId :
 SP-01


Tgt Ion	Ratio	Lower	Upper
330	100		
332	99.9	77.1	115.7
141	48.3	35.0	52.6

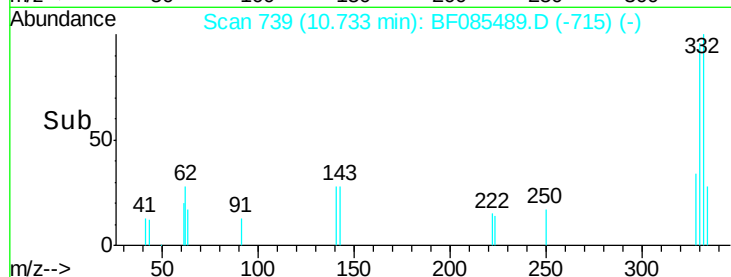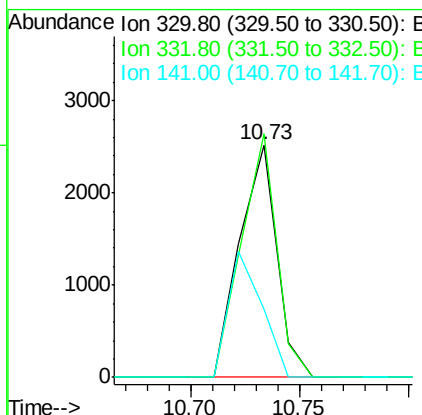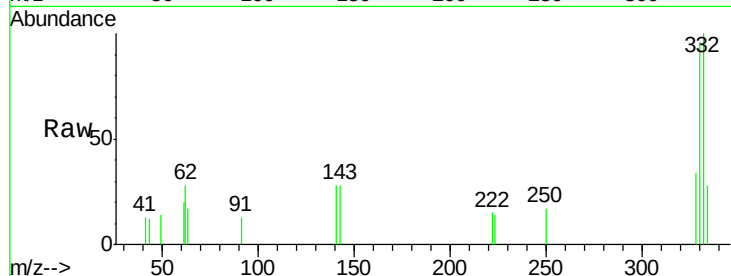

#44
 2-Fluorobiphenyl
 Concen: 2.12 ng
 RT: 9.26 min Scan# 610
 Delta R.T. -0.02 min
 Lab File: BF085489.D
 Acq: 17 Mar 2016 4:20

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.2	29.3	43.9
170	23.5	20.0	30.0

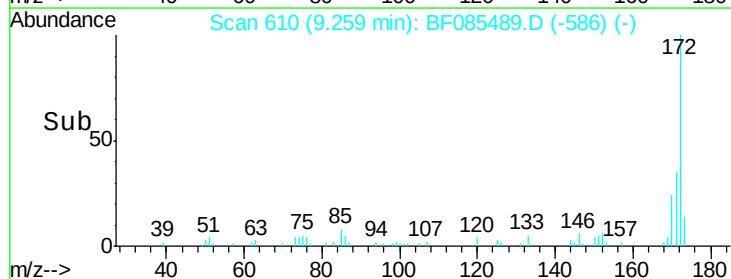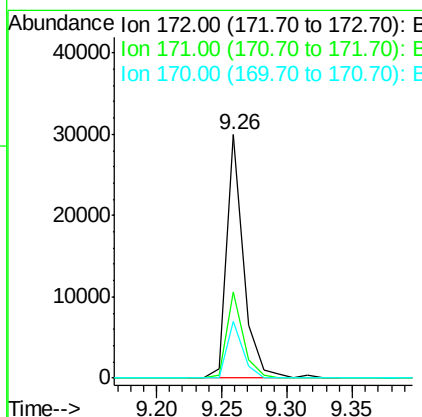

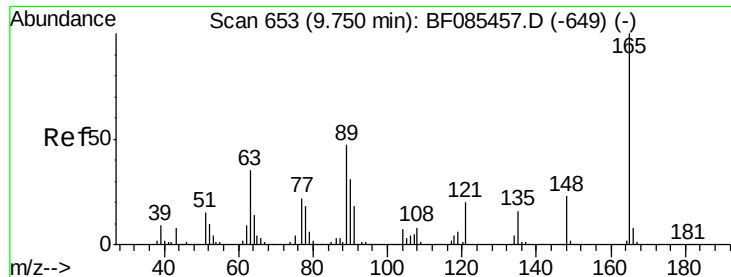

#50

2,6-Dinitrotoluene

Concen: 7.75 ng

RT: 9.94 min Scan# 670

Delta R.T. 0.19 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20

Instrument :

BNA_F

ClientSampleId :

SP-01


Tgt Ion:165 Resp: 27623

Ion Ratio Lower Upper

165 100

63 1.2 41.8 62.8#




89 2.1 46.7 70.1#



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

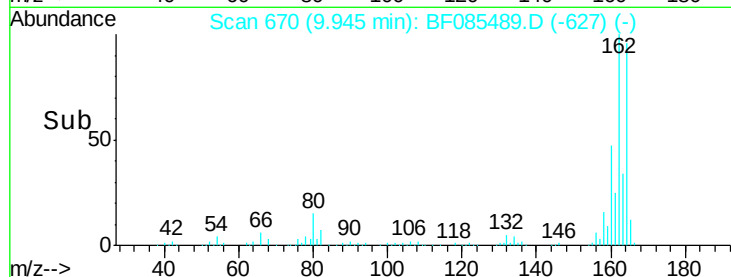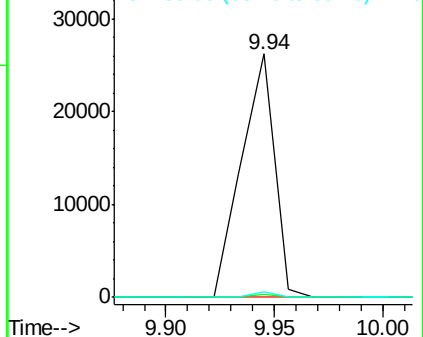

#56

2,4-Dinitrotoluene

Concen: 6.18 ng

RT: 9.94 min Scan# 670

Delta R.T. -0.21 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20

Tgt Ion:165 Resp: 27623


Ion Ratio Lower Upper

165 100

63 1.2 35.4 53.0#

89 2.1 61.9 92.9#

182 0.0 1.9 2.9#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

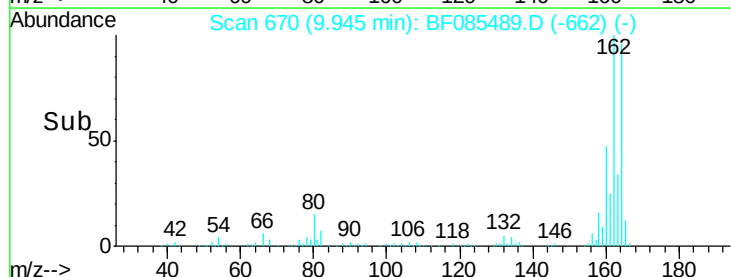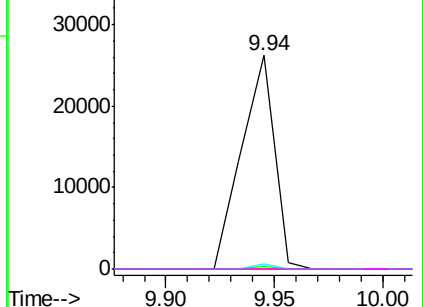


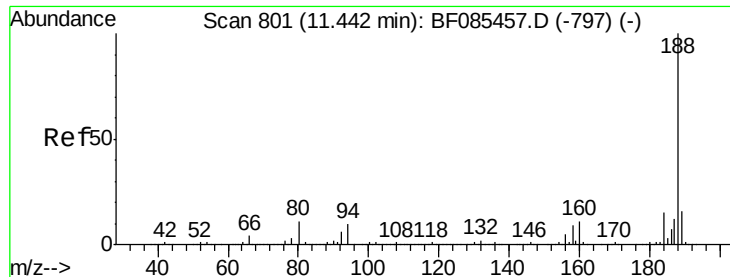




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.43 min Scan# 800
Delta R.T. -0.01 min
Lab File: BF085489.D
Acq: 17 Mar 2016 4:20

Instrument :
BNA_F
ClientSampleId :
SP-01

Tgt Ion:188 Resp: 357534
Ion Ratio Lower Upper
188 100
94 5.8 7.0 10.6#
80 5.9 7.4 11.0#

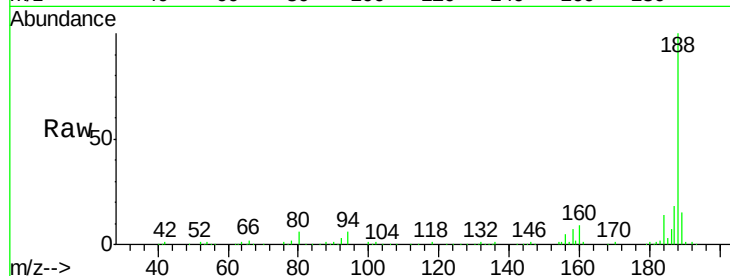


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

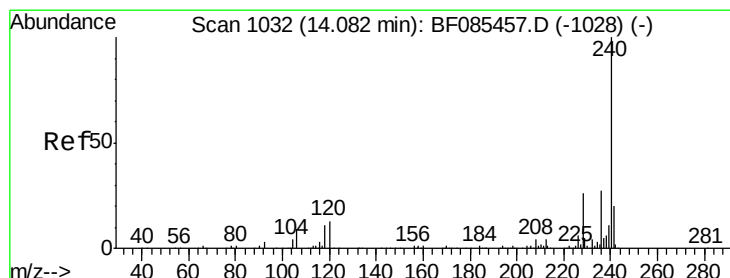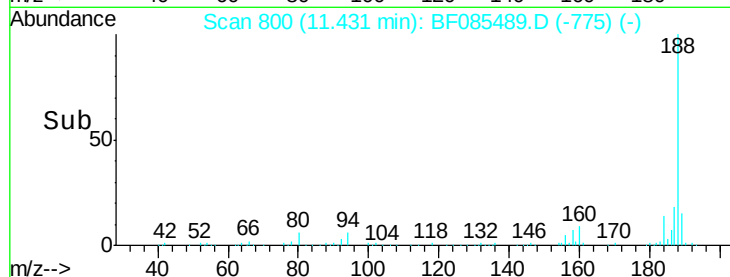
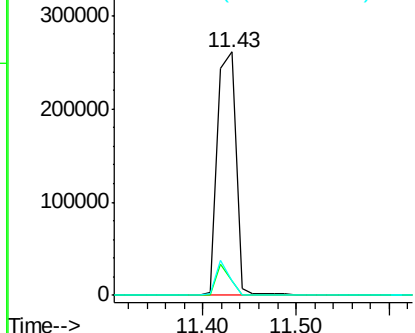



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.06 min Scan# 1030
Delta R.T. -0.02 min
Lab File: BF085489.D
Acq: 17 Mar 2016 4:20

Tgt Ion:240 Resp: 244289
Ion Ratio Lower Upper
240 100
120 12.3 5.3 7.9#
236 26.3 20.7 31.1

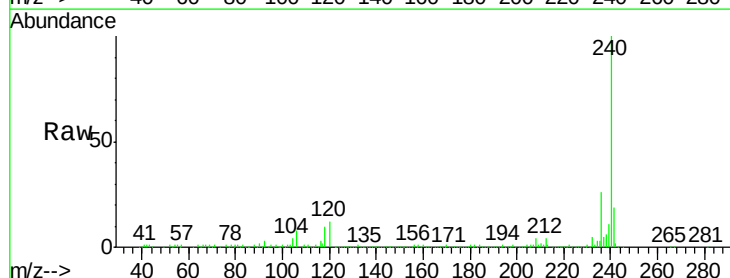

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

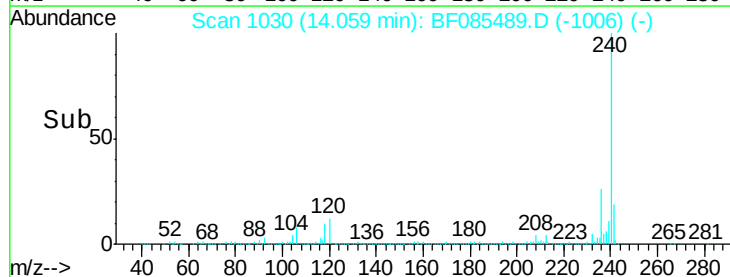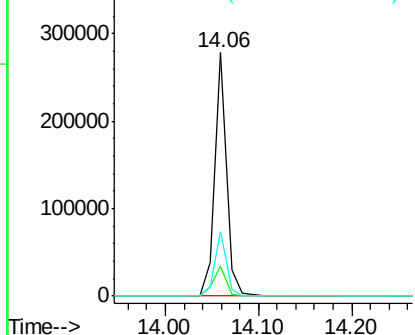

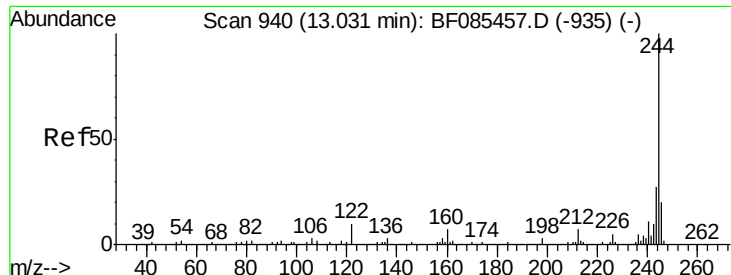

#78

Terphenyl-d14

Concen: 1.48 ng

RT: 13.01 min Scan# 938

Delta R.T. -0.02 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20

Instrument :

BNA_F

ClientSampleId :

SP-01


Tgt Ion:244 Resp: 16012

Ion Ratio Lower Upper

244 100

212 7.2 6.4 9.6




122 10.3 11.4 17.2#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

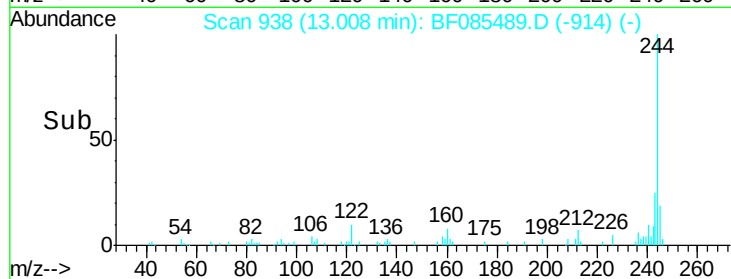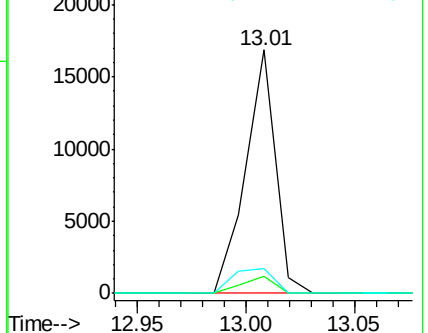

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.51 min Scan# 1157

Delta R.T. -0.02 min

Lab File: BF085489.D

Acq: 17 Mar 2016 4:20


Tgt Ion:264 Resp: 266639

Ion Ratio Lower Upper

264 100

260 24.4 19.2 28.8

265 21.2 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

