
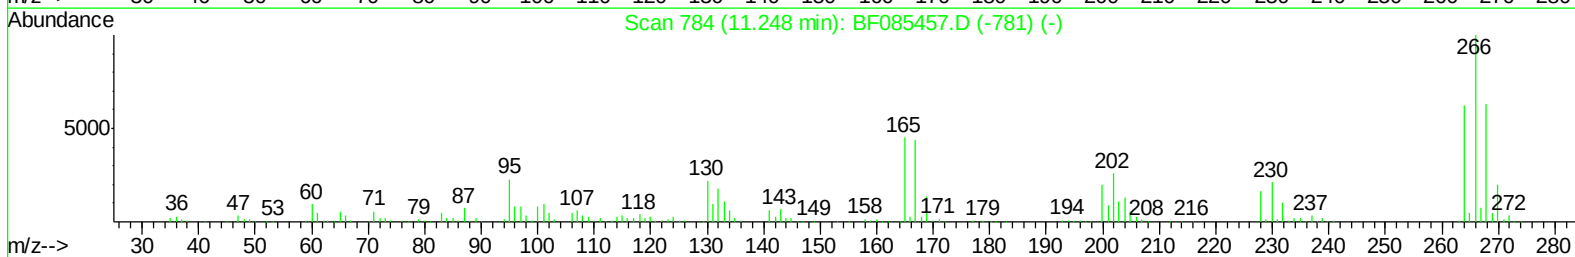
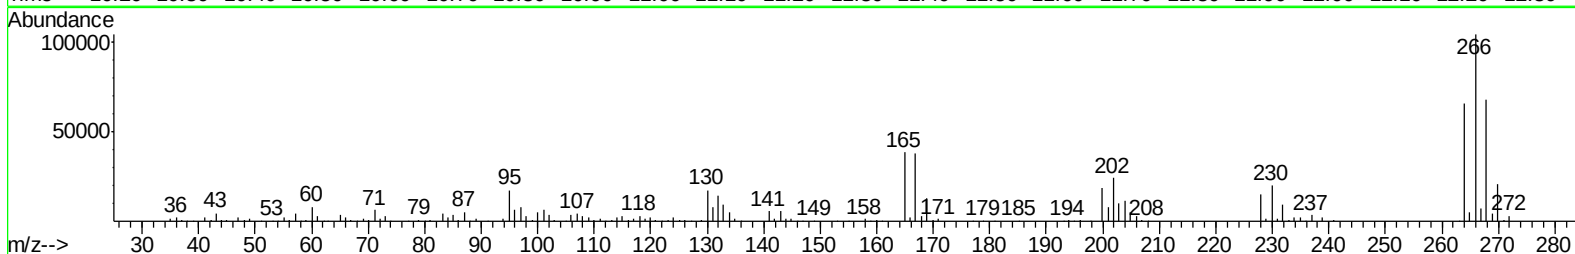


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031616\
Data File : BF085467.D
Acq On : 16 Mar 2016 17:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 03:33:40 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

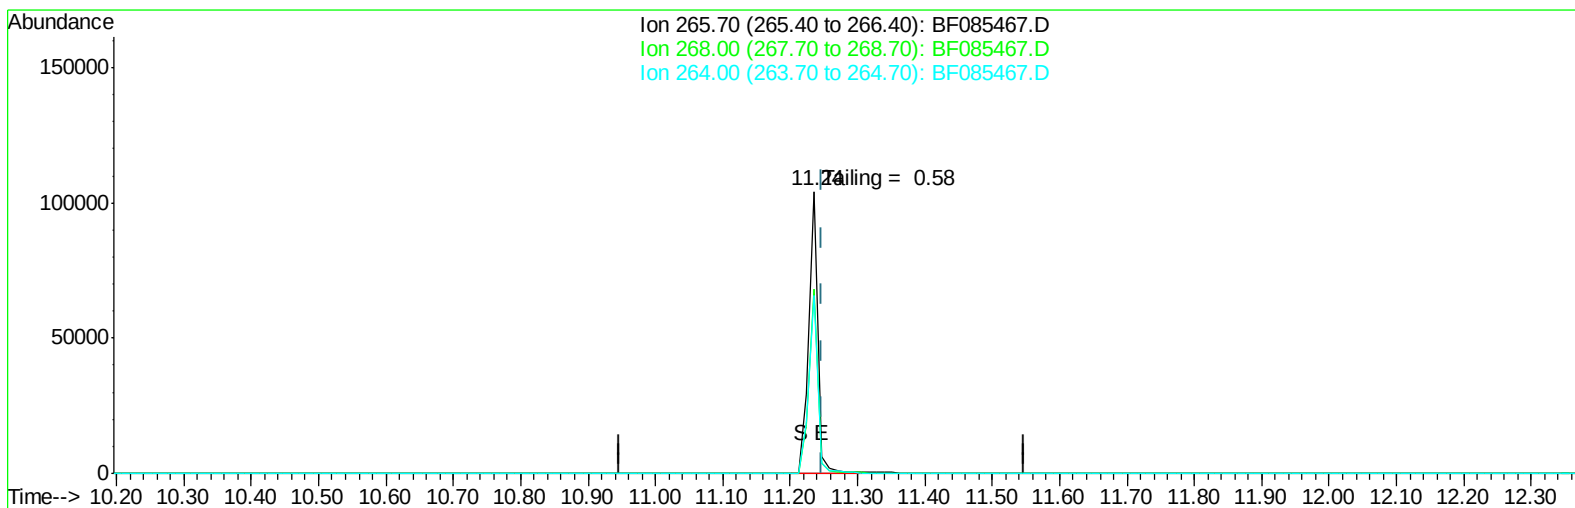

TIC: BF085467.D

(69) Pentachlorophenol (C)




11.236min (-0.012) 33691.08ng

response 99962

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	65.37
264.00	64.30	63.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031616\
Data File : BF085467.D
Acq On : 16 Mar 2016 17:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 03:33:40 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

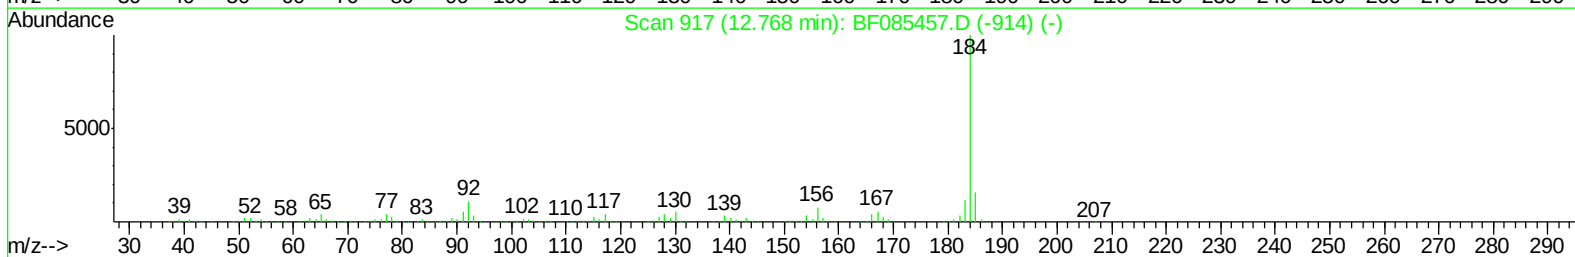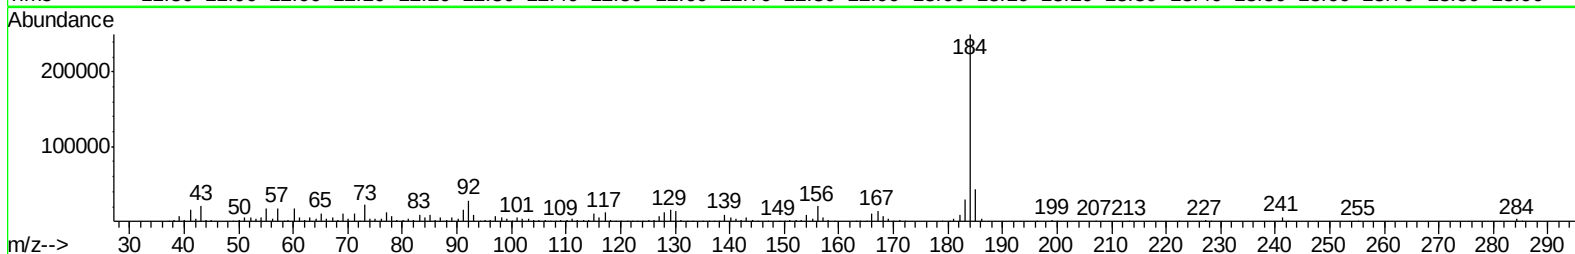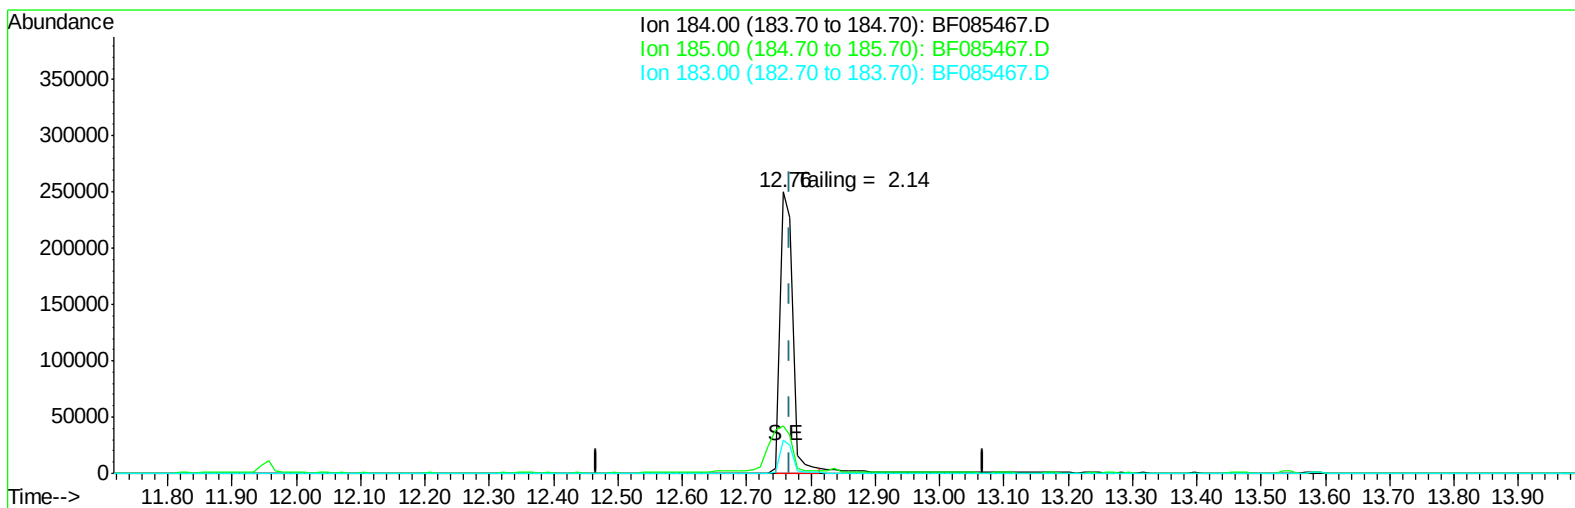

TIC: BF085467.D

(76) Benzidine

12.756min (-0.012) 18930.69ng

response 371623

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	17.05
183.00	11.80	11.61
0.00	0.00	0.00