

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031616\
 Data File : BF085489.D
 Acq On : 17 Mar 2016 4:20
 Operator : UM/SJ
 Sample : H1803-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	278	280	284	rBV	30952	47543	4.63%	0.847%
2	6.516	368	370	379	rVB3	37886	53388	5.19%	0.951%
3	6.664	381	383	385	rBV	69896	61268	5.96%	1.092%
4	6.904	401	404	406	rBV	543523	740632	72.06%	13.199%
5	7.053	415	417	420	rBV	59479	51512	5.01%	0.918%
6	7.465	451	453	455	rBV	22812	30159	2.93%	0.537%
7	8.185	514	516	518	rBV	1229190	1020862	99.32%	18.193%
8	9.259	608	610	613	rVB	87123	70377	6.85%	1.254%
9	9.945	667	670	672	rBV	966177	1027860	100.00%	18.317%
10	10.722	737	738	740	rBV	18889	20913	2.03%	0.373%
11	11.282	786	787	788	rBV	19070	15103	1.47%	0.269%
12	11.419	797	799	802	rBV	664206	890988	86.68%	15.878%
13	13.008	935	938	940	rVB	52360	55182	5.37%	0.983%
14	13.077	940	944	946	rBV4	4331	11689	1.14%	0.208%
15	13.191	948	954	955	rVV4	6302	16097	1.57%	0.287%
16	13.442	973	976	978	rBV4	8707	19121	1.86%	0.341%
17	14.059	1027	1030	1032	rBV	755874	692398	67.36%	12.339%
18	14.414	1060	1061	1062	rBV	16657	16529	1.61%	0.295%
19	15.511	1154	1157	1164	rVB	478975	769743	74.89%	13.718%


Sum of corrected areas: 5611364

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031616\
Data File : BF085489.D
Acq On : 17 Mar 2016 4:20
Operator : UM/SJ
Sample : H1803-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

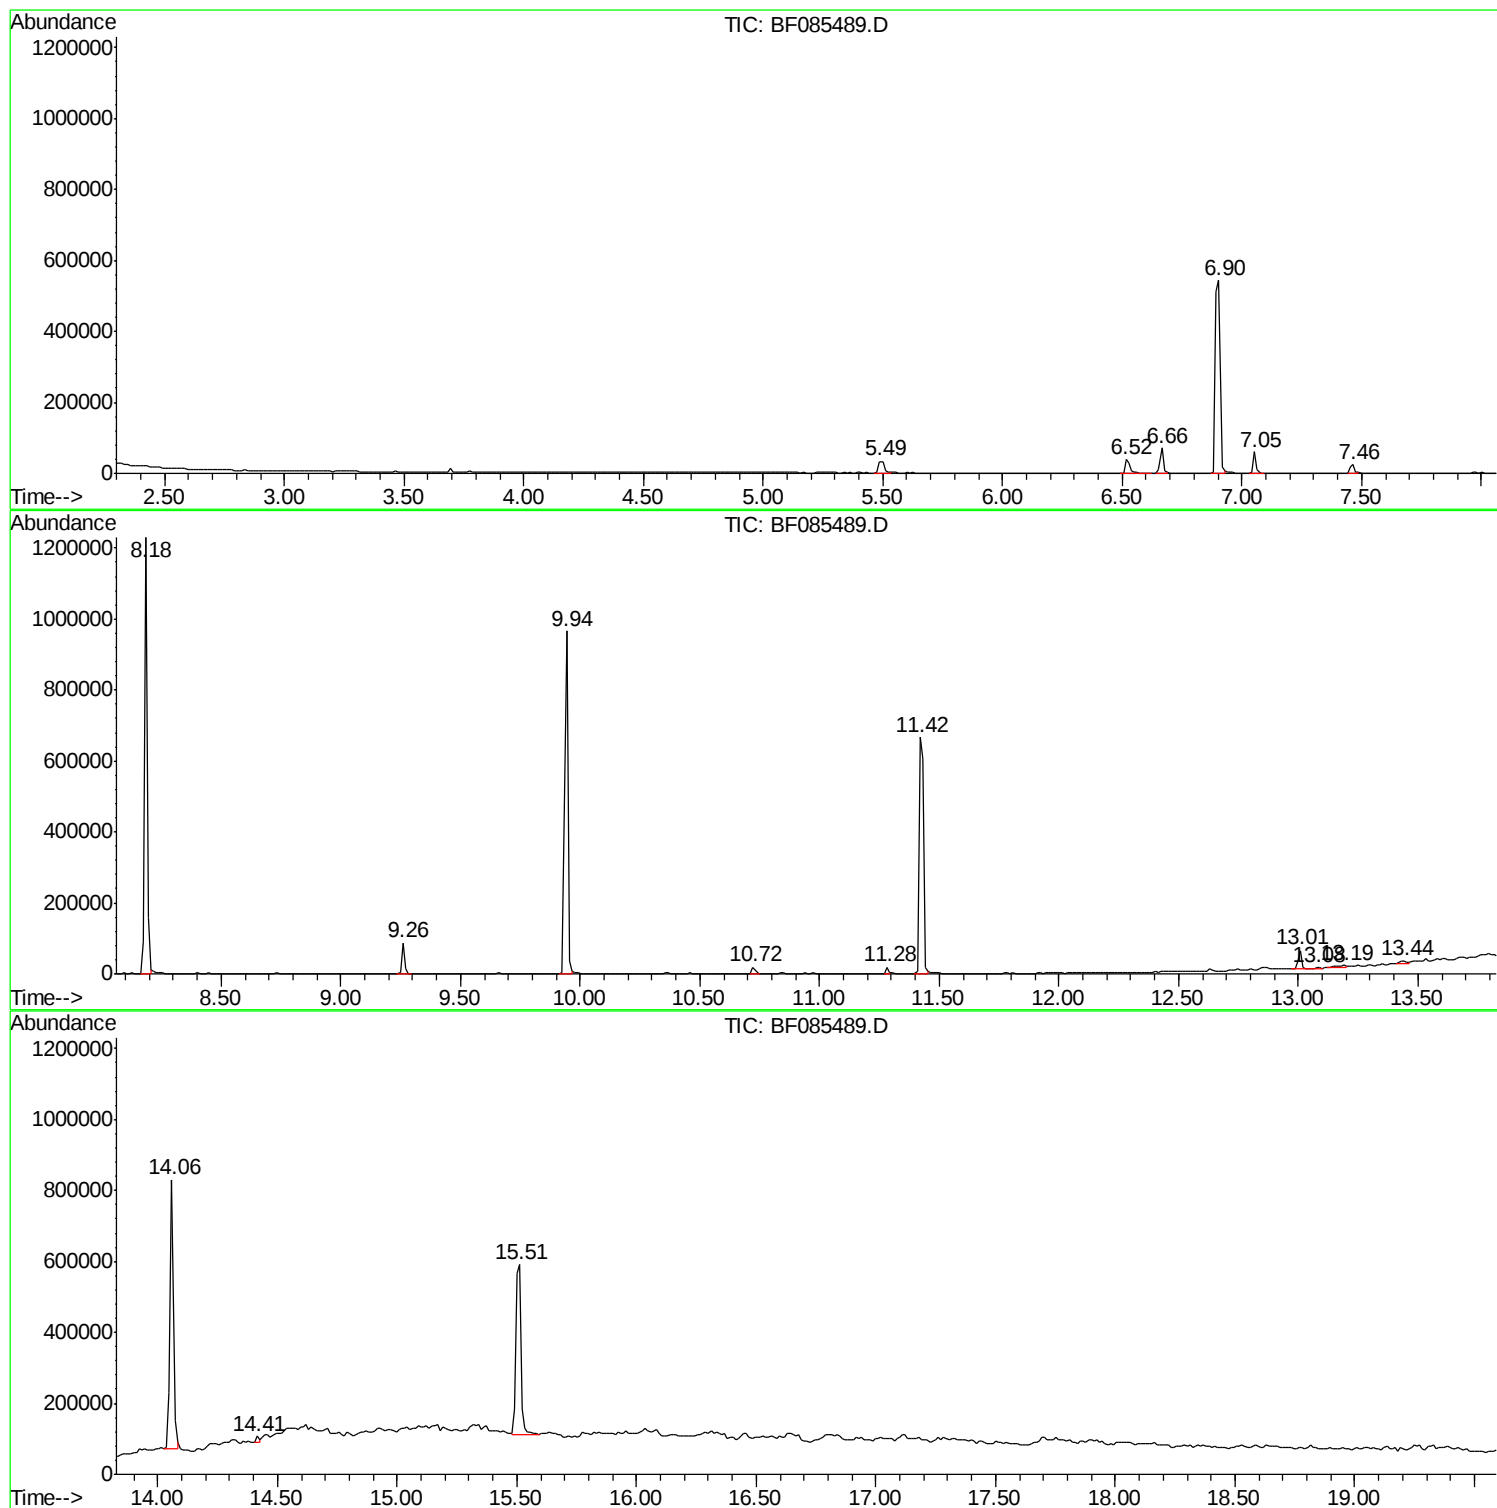

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF031616\
Data_File : BF085489.D
Acq_On : 17 Mar 2016 4:200
Operator : UM/SJJ
Sample : H1803-01_5XX
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SP-01

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
