


```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF031616\  
Data File : BF085467.D  
Acq On    : 16 Mar 2016  17:43  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

```
Method      : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Title       : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update  : Tue Mar 15 18:57:05 2016
```

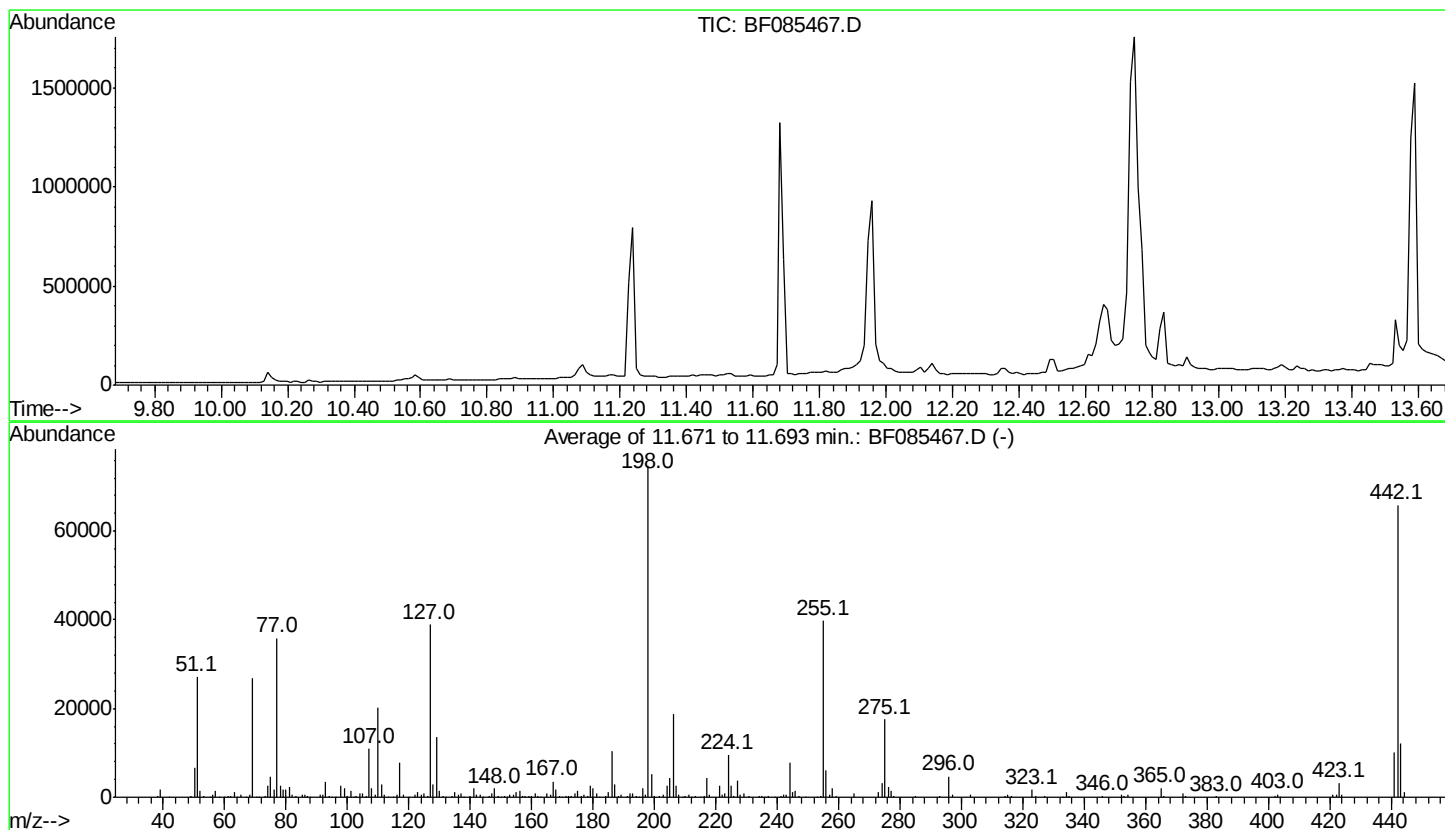

AutoFind: Scans 821, 822, 823; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	27250	PASS
68	69	0.00	2	1.7	466	PASS
69	198	0.00	100	36.0	26894	PASS
70	69	0.00	2	0.5	133	PASS
127	198	10	80	51.9	38849	PASS
197	198	0.00	2	0.7	551	PASS
198	198	100	100	100.0	74788	PASS
199	198	5	9	6.9	5173	PASS
275	198	10	60	23.5	17602	PASS
365	198	1	100	2.9	2175	PASS
441	442	0.01	24	15.6	10255	PASS
442	198	50	100	88.1	65912	PASS
443	442	15	24	18.5	12220	PASS