


Data Path : Z:\HPCHEM1\BNA F\Data\BF031617\
 Data File : BF093702.D
 Acq On : 16 Mar 2017 12:49
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

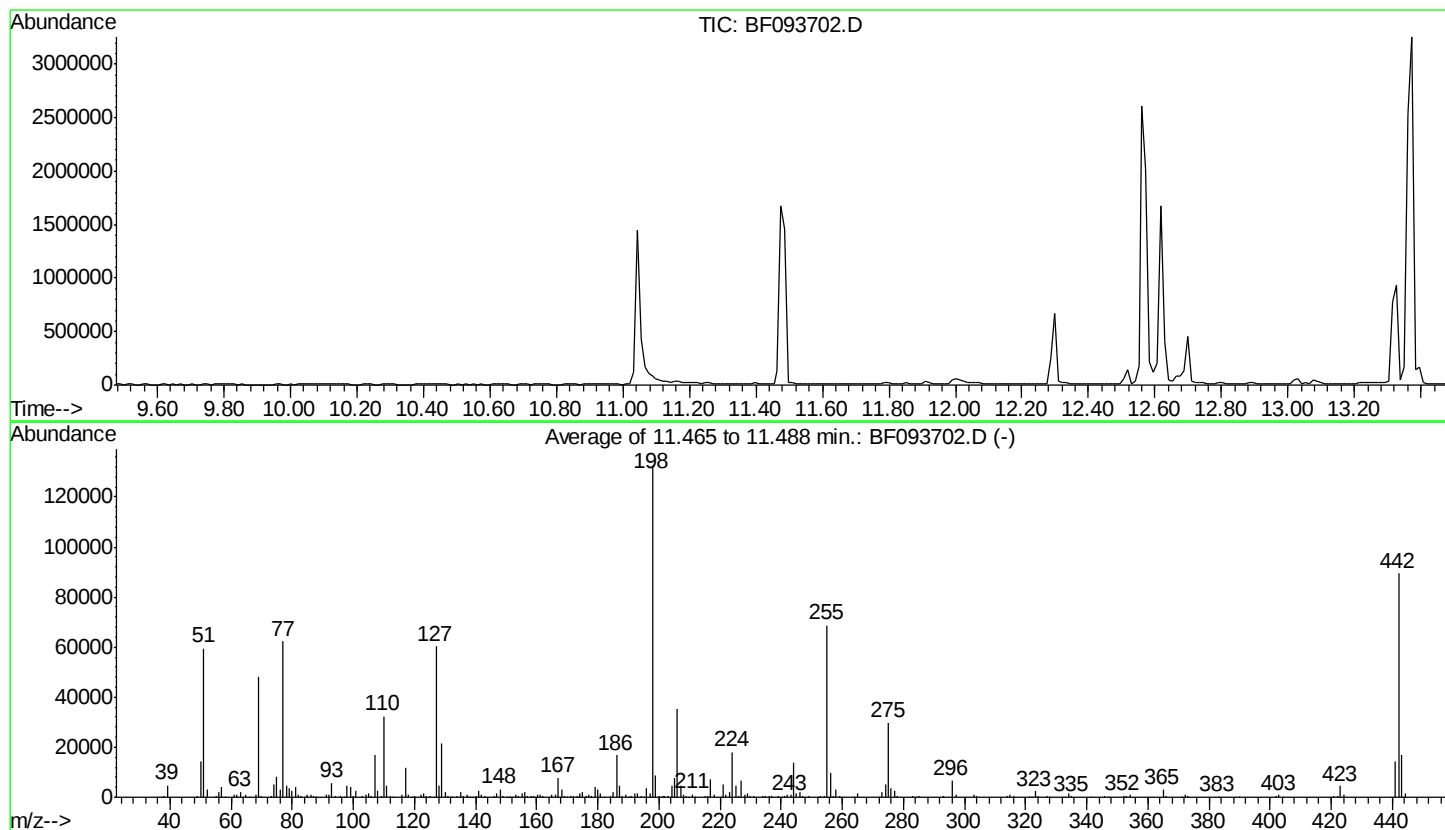

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	59442	PASS
68	69	0.00	2	2.0	960	PASS
69	198	0.00	100	36.5	48350	PASS
70	69	0.00	2	0.7	315	PASS
127	198	10	80	45.5	60265	PASS
197	198	0.00	2	1.0	1368	PASS
198	198	100	100	100.0	132540	PASS
199	198	5	9	6.7	8864	PASS
275	198	10	60	22.5	29789	PASS
365	198	1	100	2.2	2942	PASS
441	442	0.01	24	16.2	14523	PASS
442	198	50	100	67.5	89517	PASS
443	442	15	24	18.7	16739	PASS