
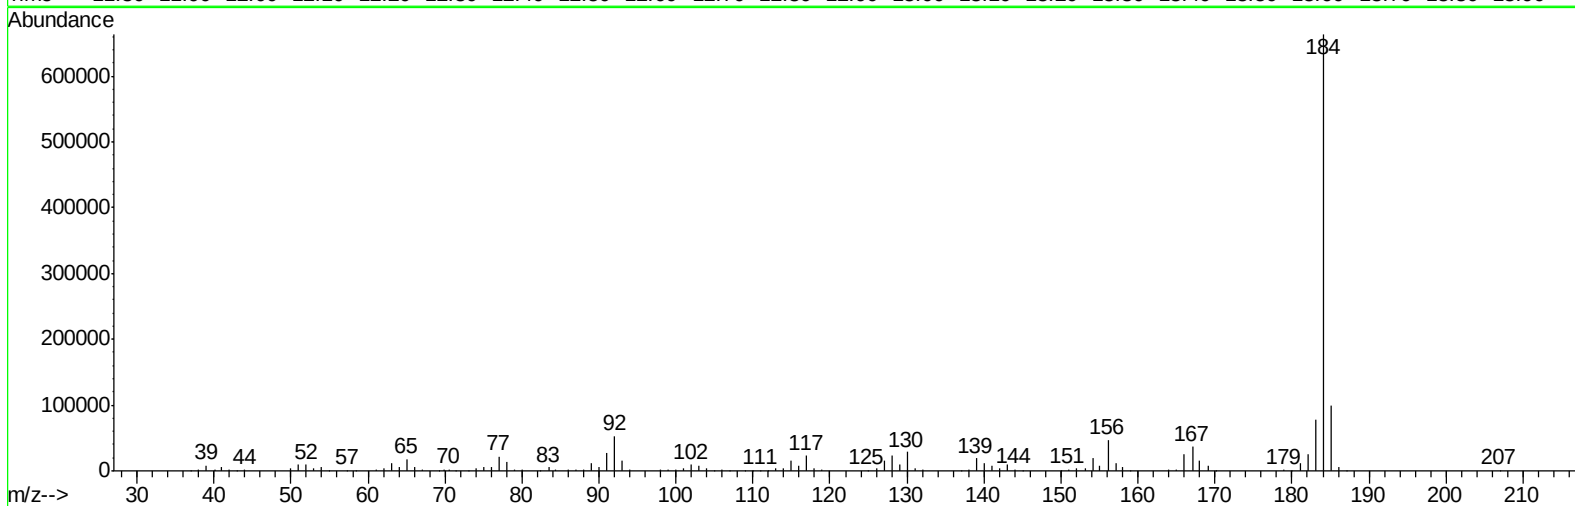


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031618\
Data File : BF103683.D
Acq On : 16 Mar 2018 8:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 09:09:55 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

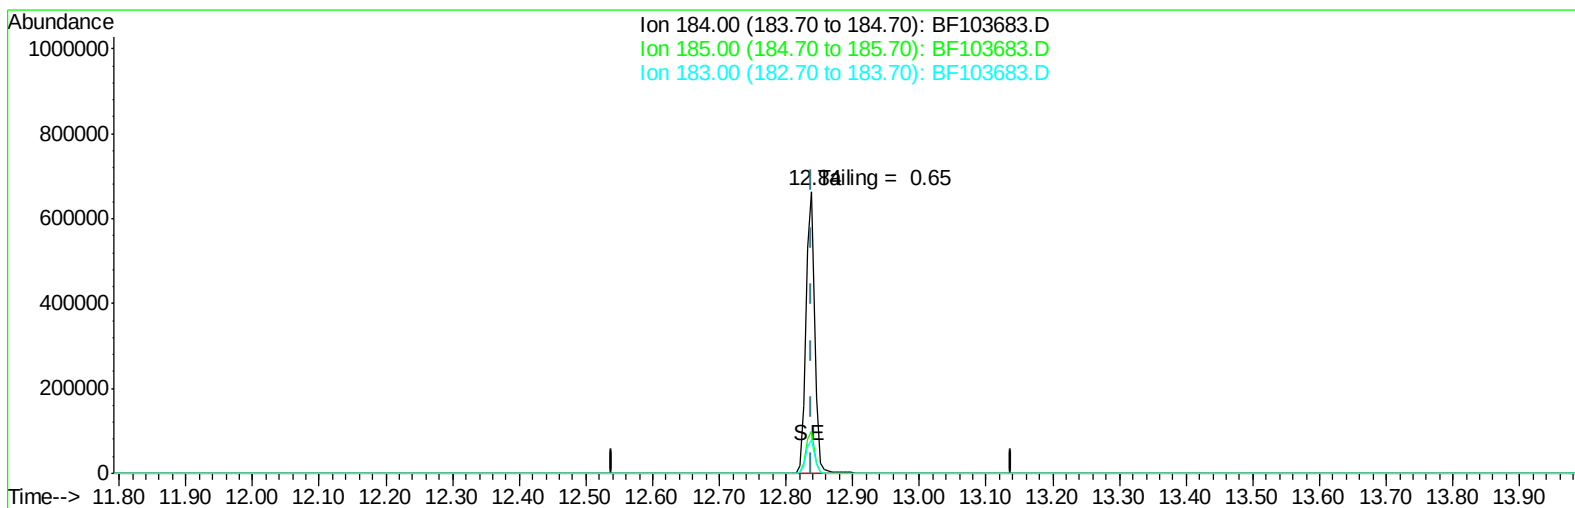

TIC: BF103683.D

(76) Benzidine



12.839min (-0.000) 4517.15ng

response 572388

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.83
183.00	11.60	11.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031618\
Data File : BF103683.D
Acq On : 16 Mar 2018 8:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 09:09:55 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

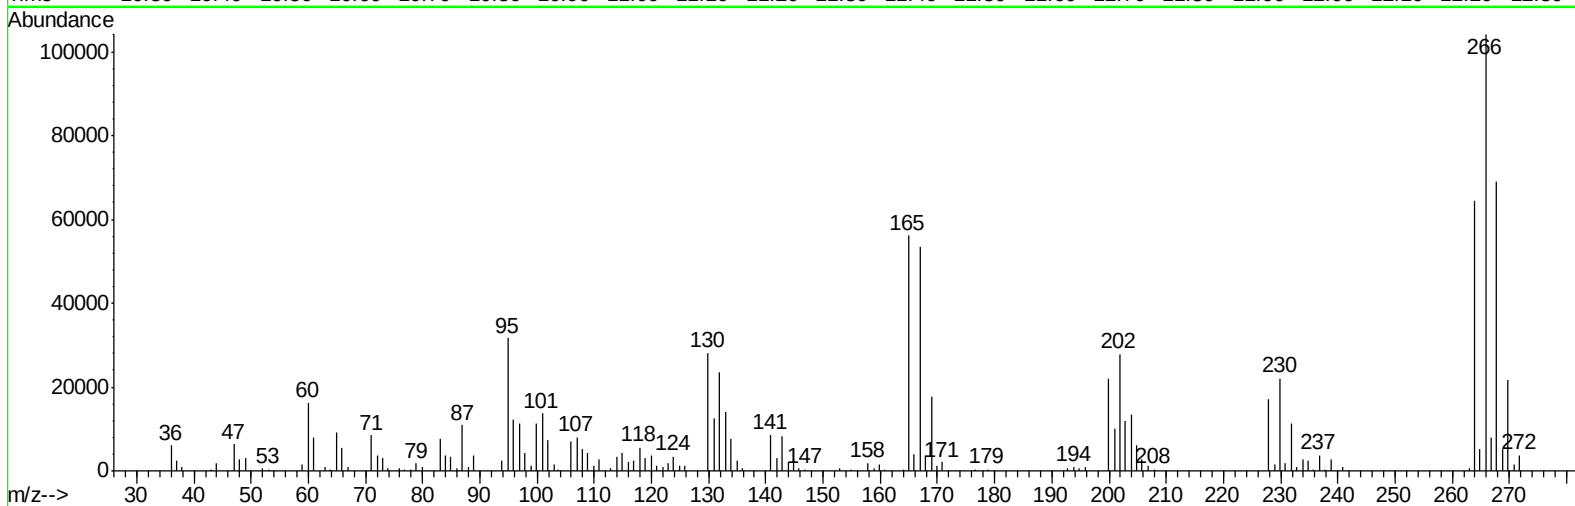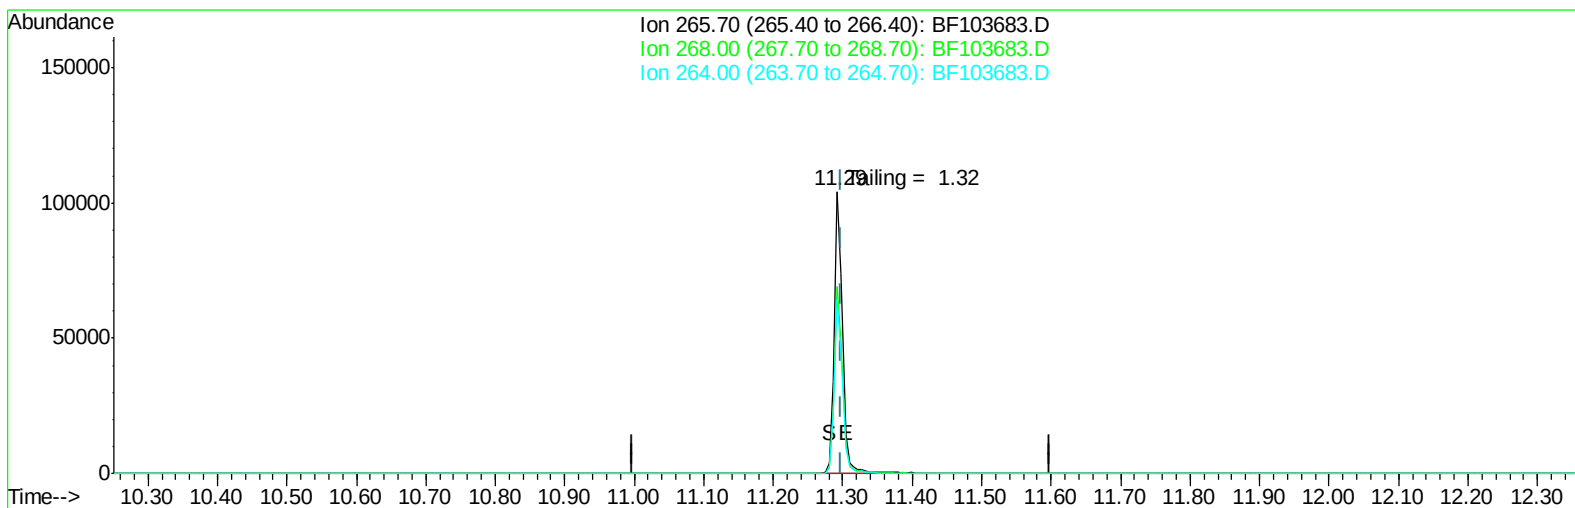

TIC: BF103683.D

(69) Pentachlorophenol (C)

11.292min (-0.006) 109792.40ng

response 85804

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.23
264.00	61.90	61.74
0.00	0.00	0.00