
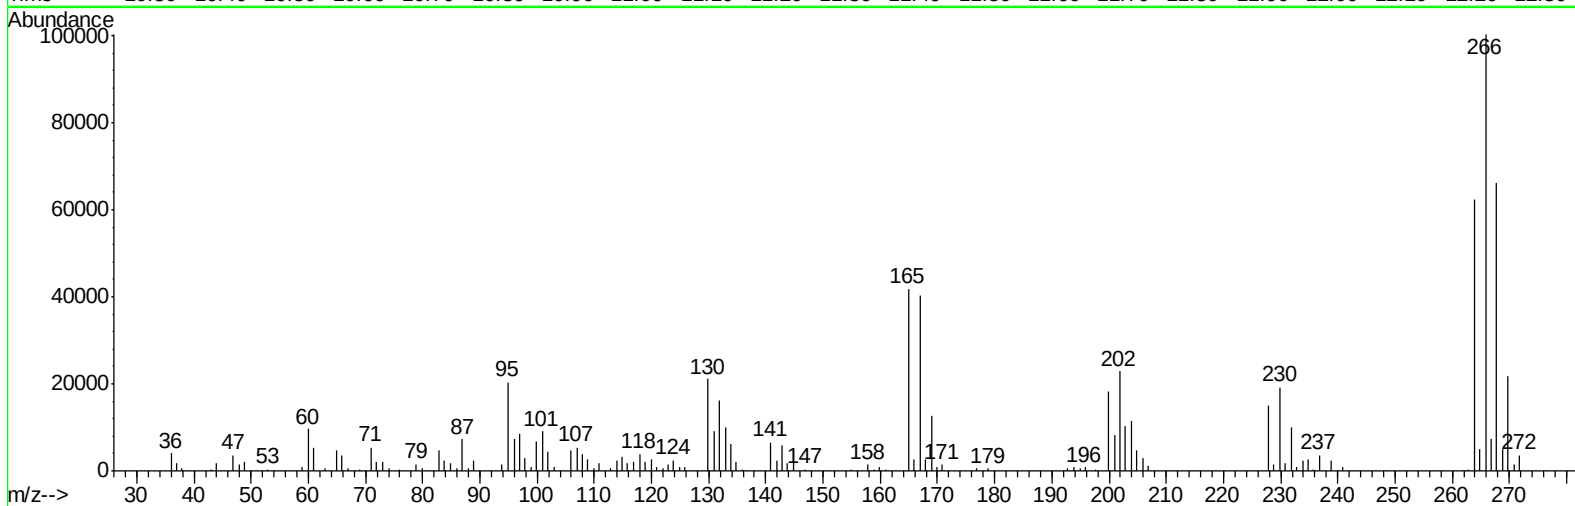


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031618\
Data File : BF103698.D
Acq On : 16 Mar 2018 16:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 09:11:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

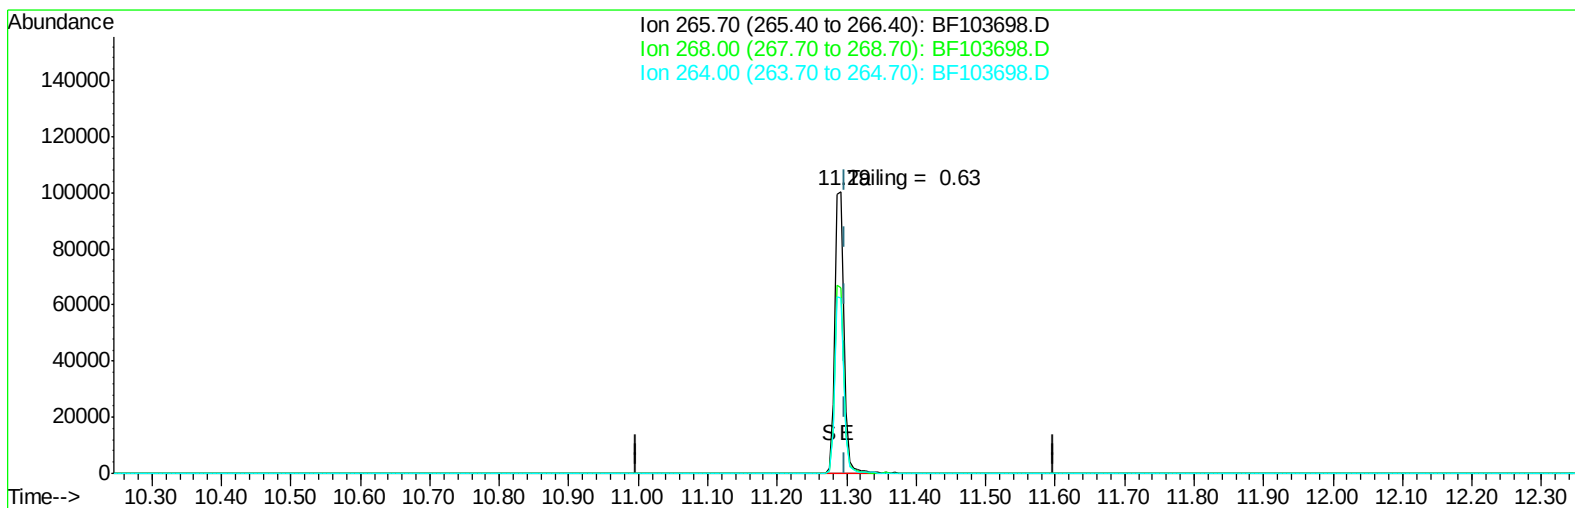

TIC: BF103698.D

(69) Pentachlorophenol (C)



11.292min (-0.006) 33950.65ng

response 91035

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.04
264.00	61.90	62.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031618\
Data File : BF103698.D
Acq On : 16 Mar 2018 16:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 09:11:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

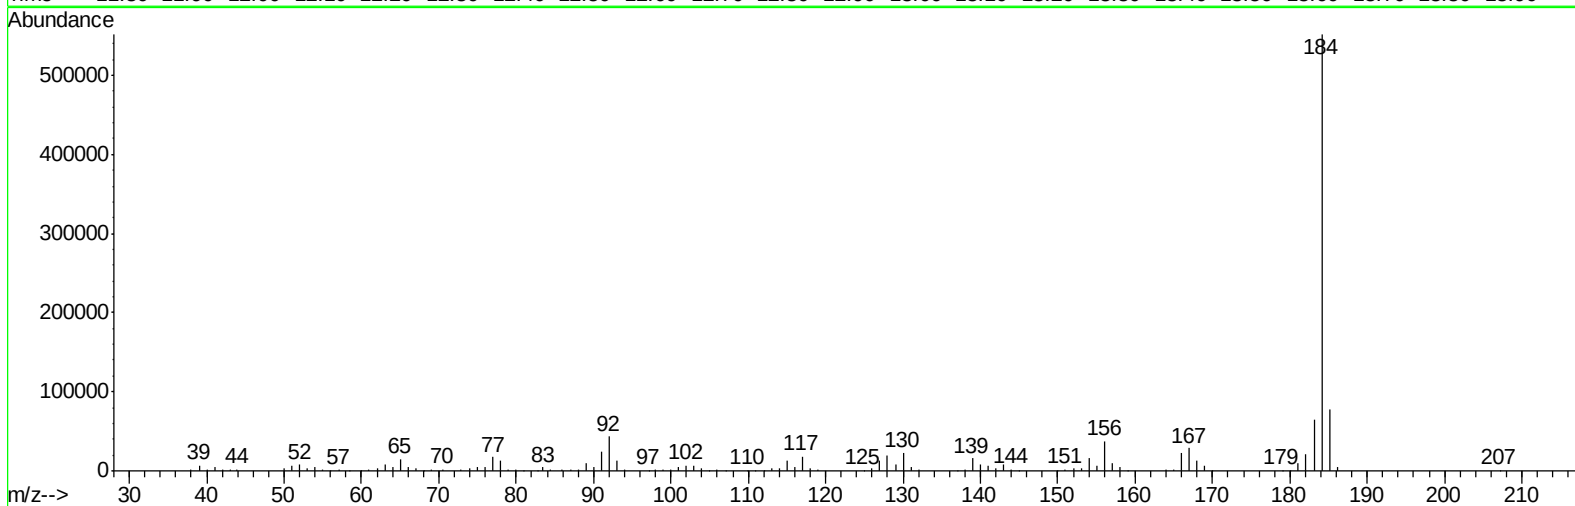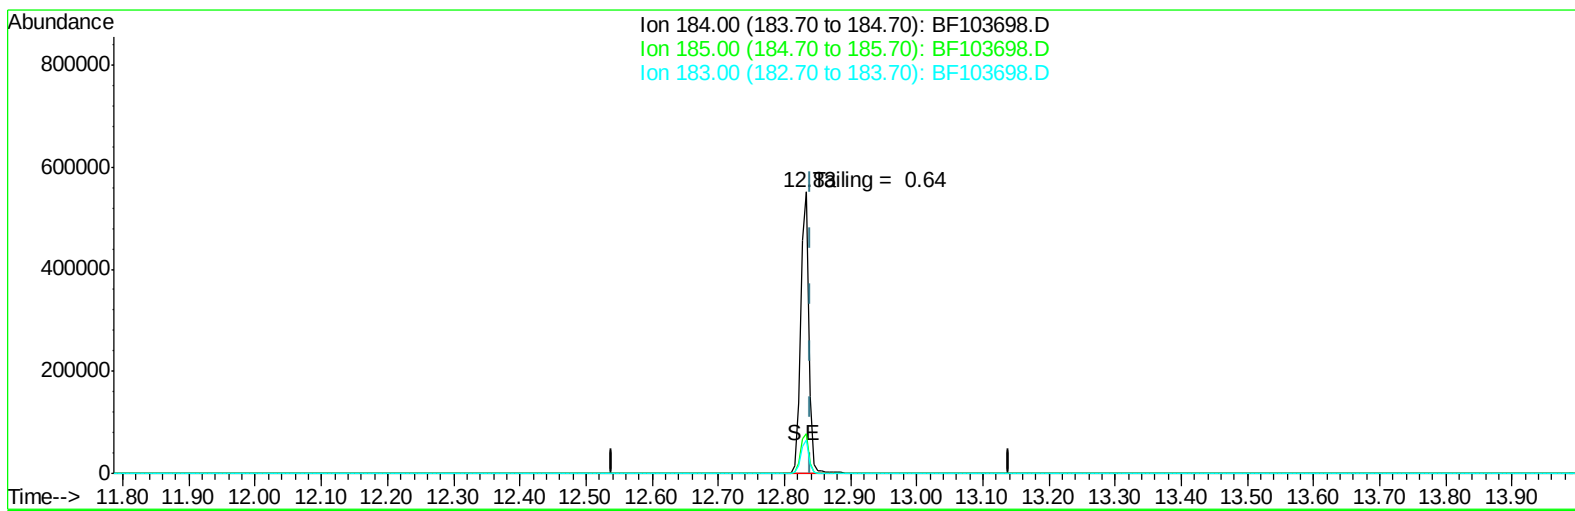

TIC: BF103698.D

(76) Benzidine

12.833min (-0.006) 0.00ng

response 480116

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.18
183.00	11.60	11.79
0.00	0.00	0.00