


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF031618\
Data File : BF103683.D
Acq On : 16 Mar 2018 8:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 15 18:31:53 2018

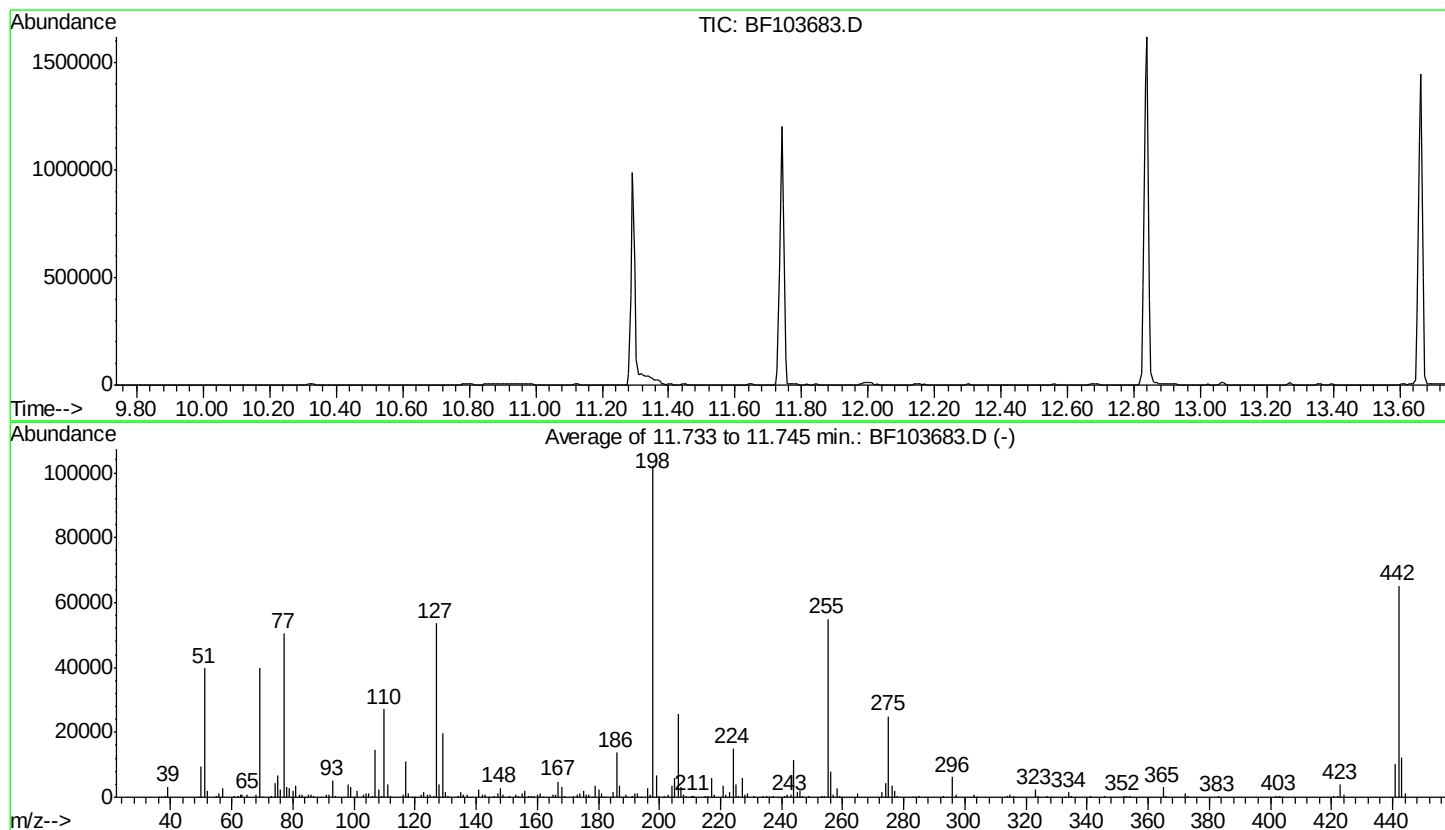

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	39850	PASS
68	69	0.00	2	2.0	792	PASS
69	198	0.00	100	39.0	39826	PASS
70	69	0.00	2	0.3	125	PASS
127	198	10	80	52.5	53648	PASS
197	198	0.00	2	0.8	828	PASS
198	198	100	100	100.0	102221	PASS
199	198	5	9	6.5	6684	PASS
275	198	10	60	24.5	24999	PASS
365	198	1	100	3.0	3057	PASS
441	443	0.01	100	82.5	10101	PASS
442	198	50	100	63.8	65250	PASS
443	442	15	24	18.8	12238	PASS