


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF031618\
 Data File : BF103698.D
 Acq On : 16 Mar 2018 16:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 15 18:31:53 2018

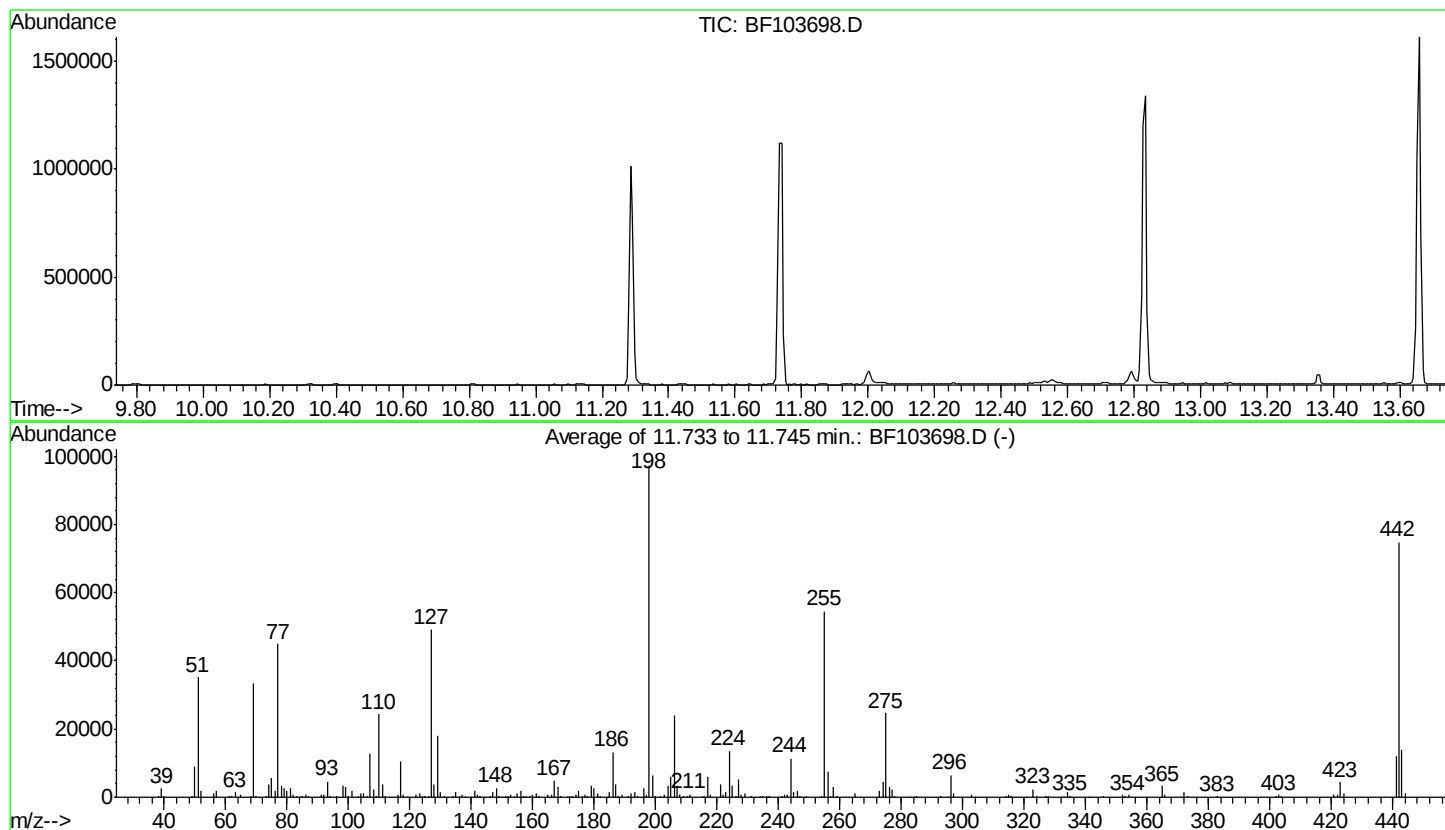

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	35215	PASS
68	69	0.00	2	1.6	533	PASS
69	198	0.00	100	34.5	33537	PASS
70	69	0.00	2	0.7	223	PASS
127	198	10	80	50.6	49151	PASS
197	198	0.00	2	0.8	802	PASS
198	198	100	100	100.0	97232	PASS
199	198	5	9	6.5	6330	PASS
275	198	10	60	25.3	24629	PASS
365	198	1	100	3.4	3339	PASS
441	443	0.01	100	88.4	12209	PASS
442	198	50	100	76.8	74704	PASS
443	442	15	24	18.5	13817	PASS