


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF031618\
 Data File : BF103725.D
 Acq On : 17 Mar 2018 5:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 15 18:31:53 2018

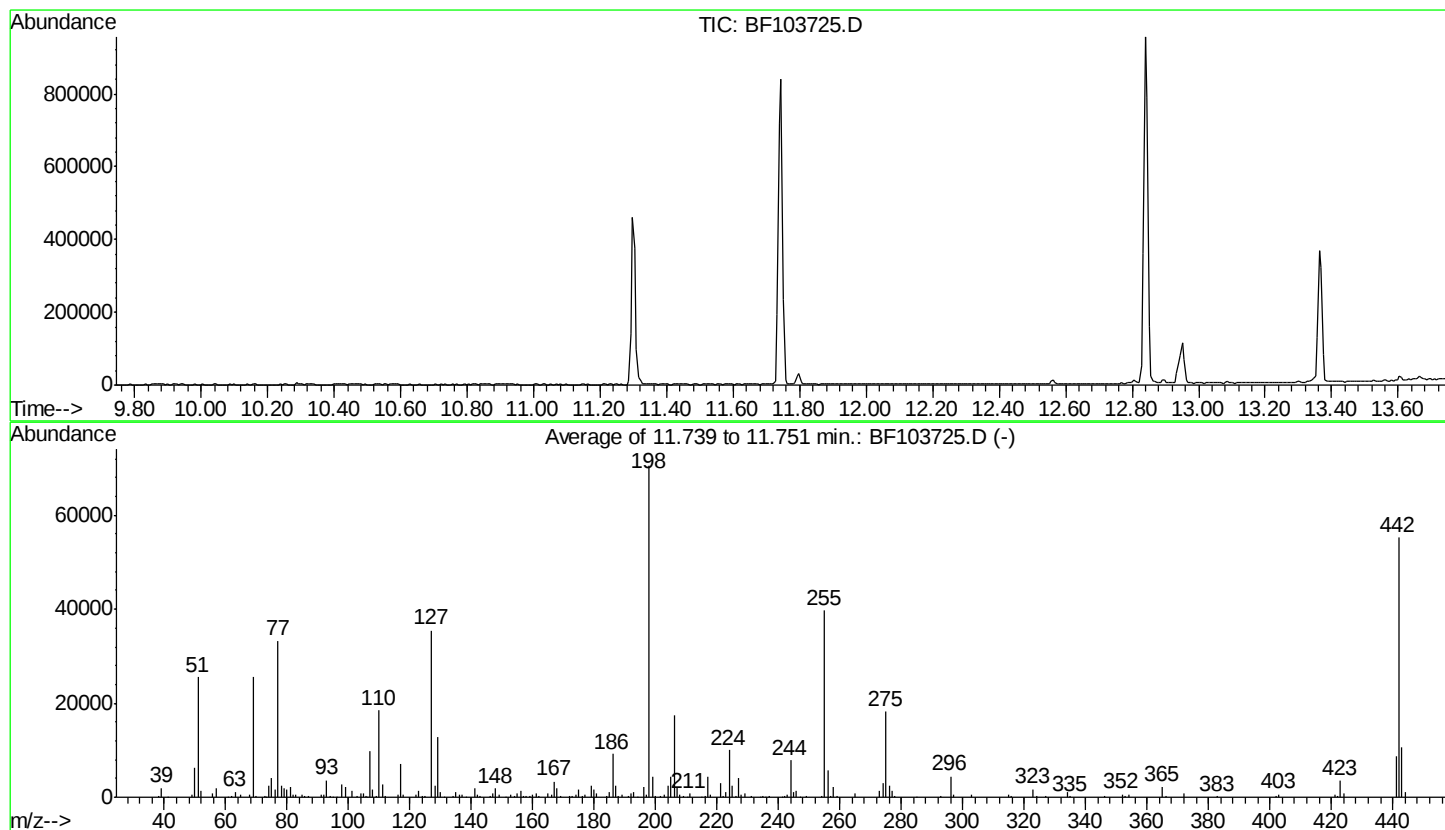

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	25505	PASS
68	69	0.00	2	1.7	430	PASS
69	198	0.00	100	36.2	25524	PASS
70	69	0.00	2	0.9	219	PASS
127	198	10	80	50.2	35430	PASS
197	198	0.00	2	0.8	543	PASS
198	198	100	100	100.0	70541	PASS
199	198	5	9	6.4	4488	PASS
275	198	10	60	25.8	18165	PASS
365	198	1	100	3.2	2238	PASS
441	443	0.01	100	82.7	8760	PASS
442	198	50	100	78.3	55264	PASS
443	442	15	24	19.2	10593	PASS