


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031623\
Data File : BF132810.D
Acq On : 16 Mar 2023 12:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 17 03:35:59 2023

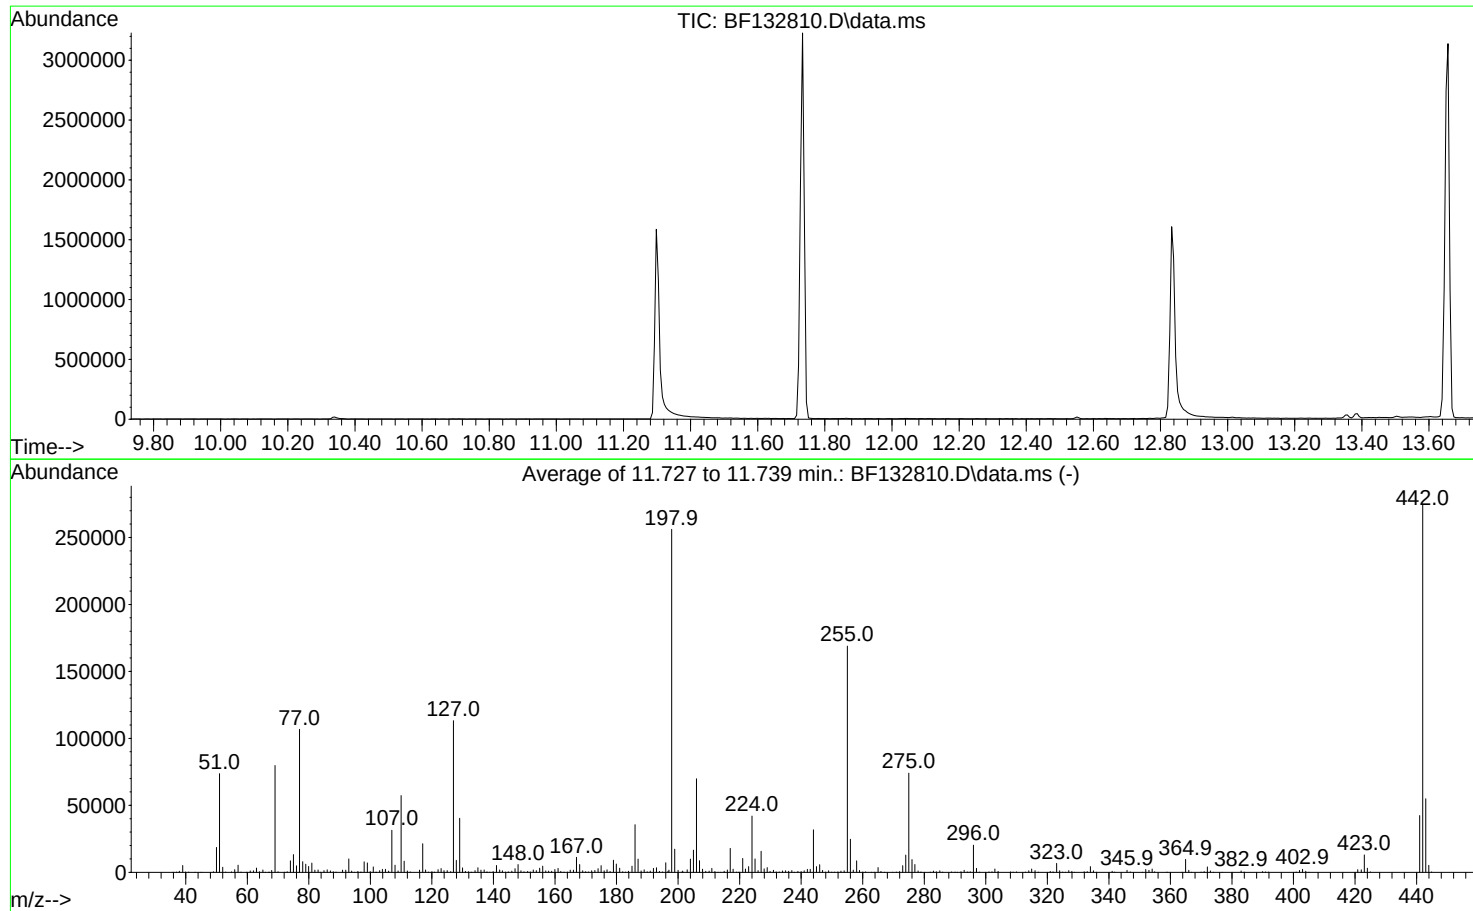




AutoFind: Scans 1554, 1555, 1556; Background Corrected with Scan 1549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	73651	PASS
68	69	0.00	2	1.7	1356	PASS
69	198	0.00	100	31.1	79733	PASS
70	69	0.00	2	0.5	426	PASS
127	198	10	80	44.2	113267	PASS
197	198	0.00	2	0.6	1643	PASS
198	198	100	100	100.0	256128	PASS
199	198	5	9	6.8	17317	PASS
275	198	10	60	28.9	74016	PASS
365	198	1	100	3.8	9642	PASS
441	198	0.01	100	16.5	42349	PASS
442	442	50	100	100.0	274688	PASS
443	442	15	24	20.0	54931	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031623\
 Data File : BF132810.D
 Acq On : 16 Mar 2023 12:58
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 08:04:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 03:35:59 2023
 Response via : Initial Calibration

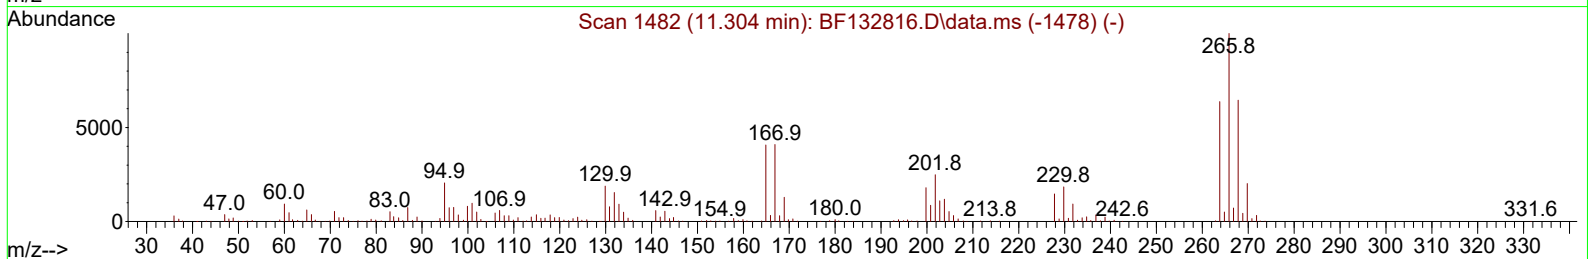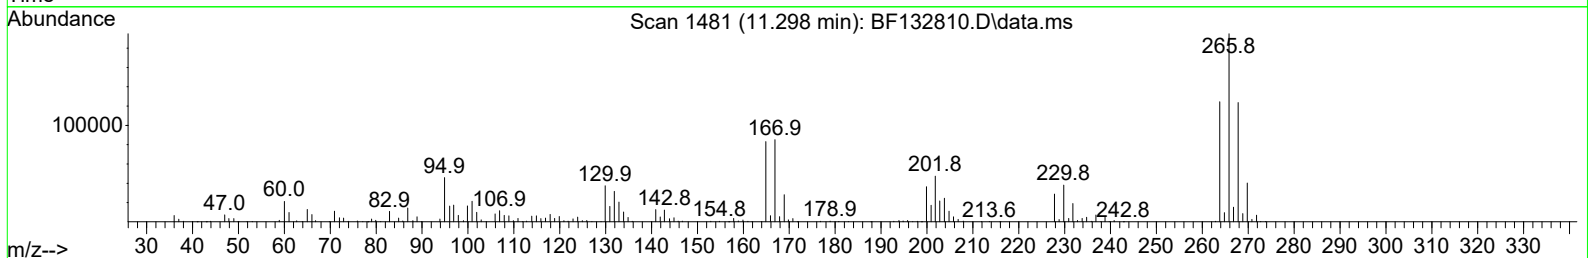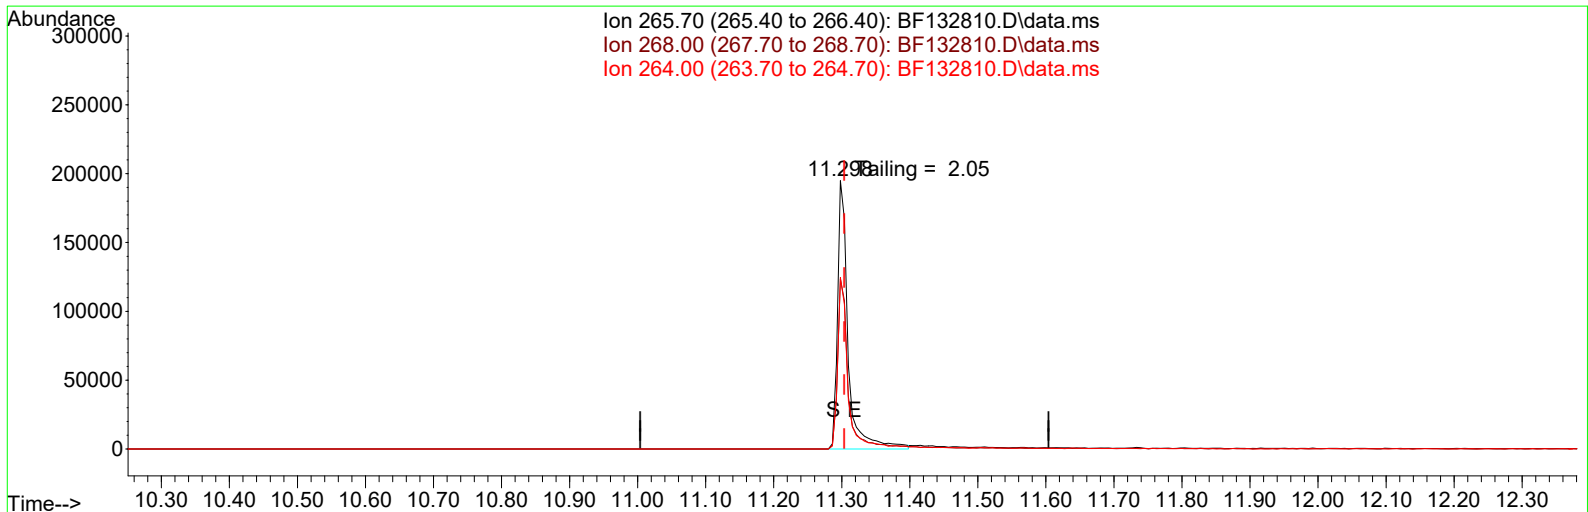

TIC: BF132810.D\data.ms

(70) Pentachlorophenol (C)

11.298min (-0.006) 507306.77 ng




response 208189

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.41
264.00	63.70	63.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031623\
Data File : BF132810.D
Acq On : 16 Mar 2023 12:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 17 08:04:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 03:35:59 2023
Response via : Initial Calibration

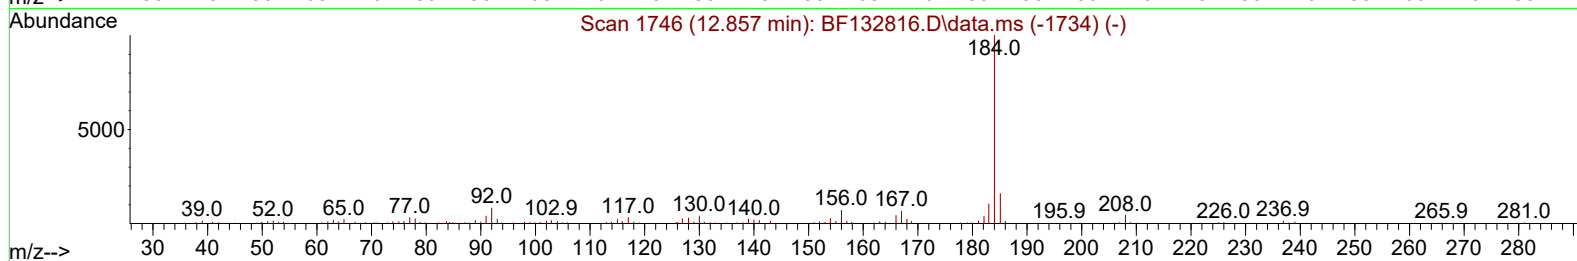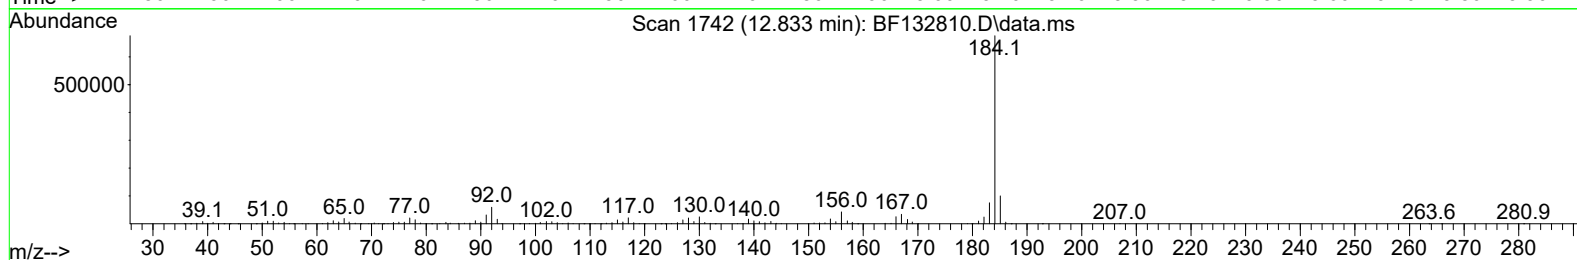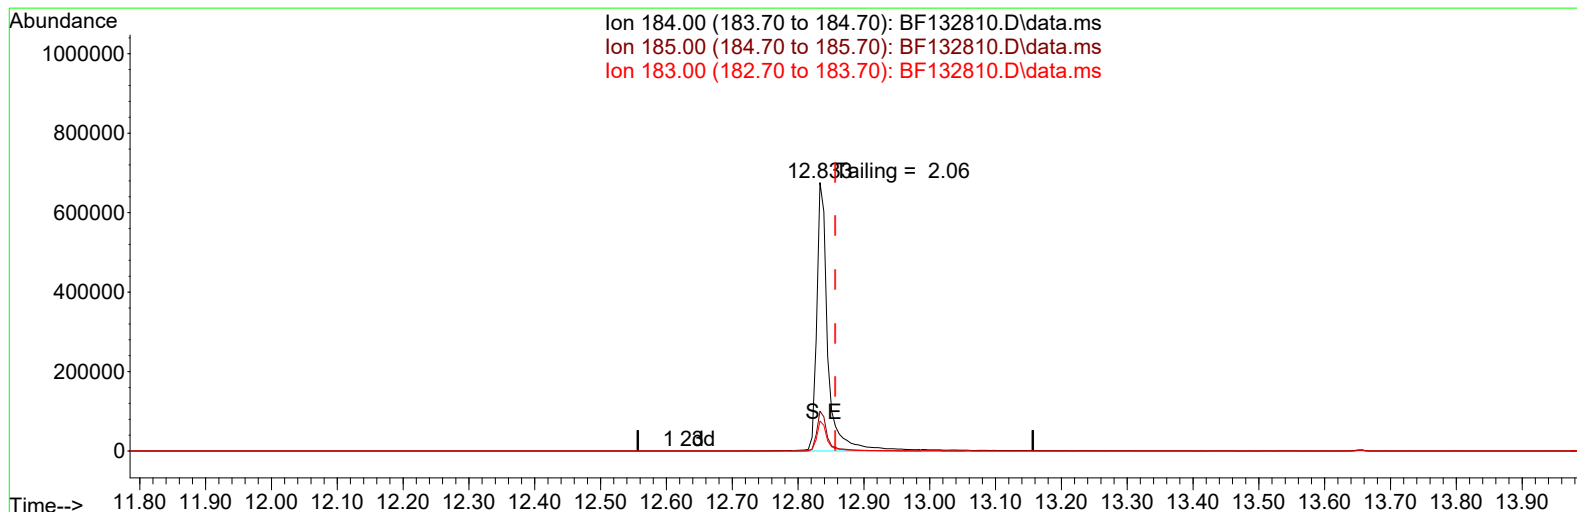

TIC: BF132810.D\data.ms

(77) Benzidine

12.833min (-0.023) 14508.03 ng m

response 797805

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.86
183.00	10.30	11.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2023	BNA_F	<u>BF132810.D</u>
Compound Name	Response	Retention Time
DDT	610531	13.657
DDD	12577	13.386
DDE	646	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13223	623754	2.12

Instrument :
BNA_F
ClientSampleId :
DFTPP