


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031715\
 Data File : BF077767.D
 Acq On : 17 Mar 2015 12:45
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE031615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 17 12:51:08 2015

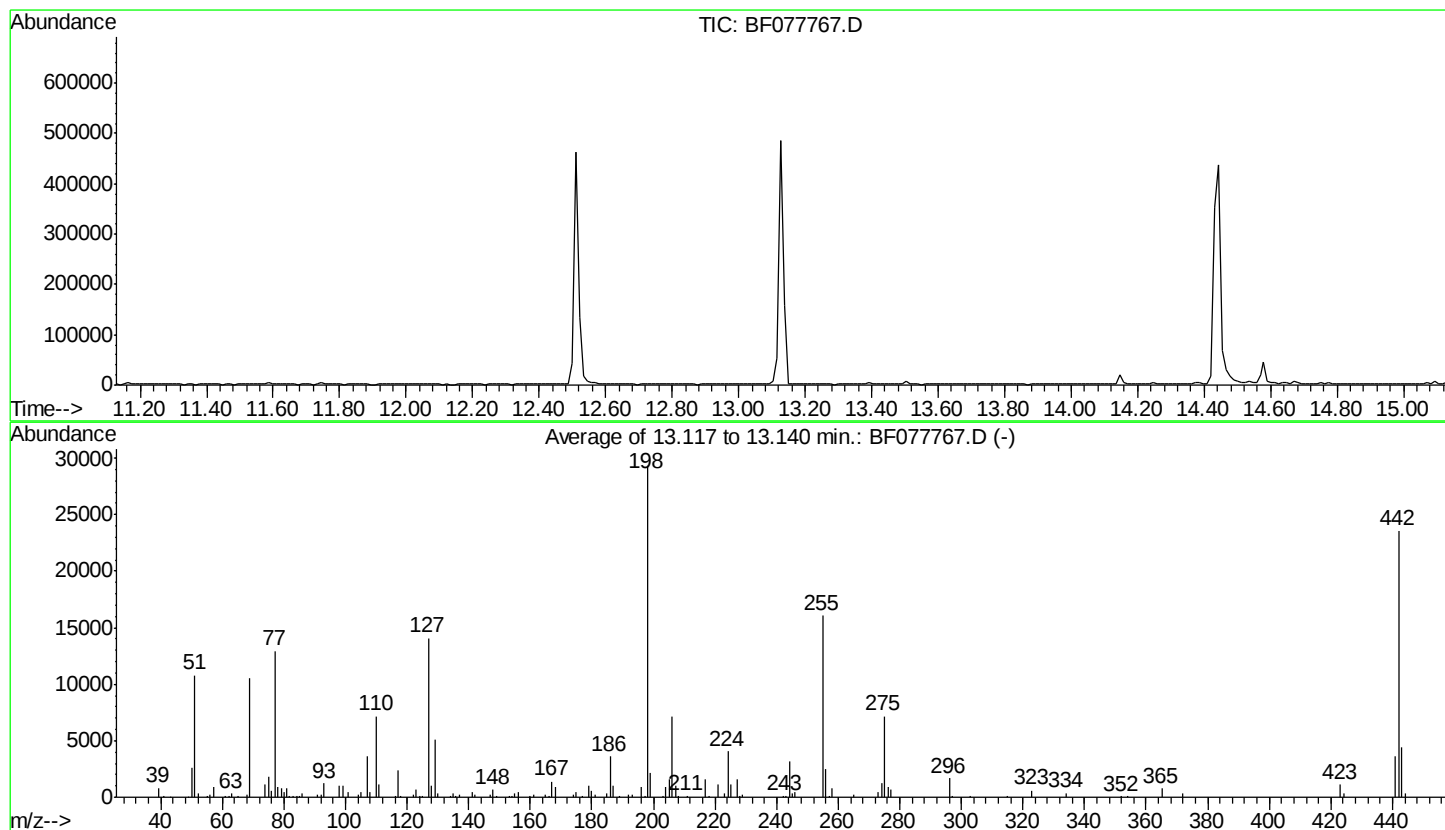

AutoFind: Scans 1070, 1071, 1072; Background Corrected with Scan 1067

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	10794	PASS
68	69	0.00	2	1.8	185	PASS
69	198	0.00	100	36.0	10562	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	14101	PASS
197	198	0.00	2	0.5	145	PASS
198	198	100	100	100.0	29336	PASS
199	198	5	9	7.2	2119	PASS
275	198	10	60	24.4	7167	PASS
365	198	1	100	2.6	751	PASS
441	442	0.01	24	15.6	3683	PASS
442	198	50	100	80.3	23571	PASS
443	442	15	24	18.9	4460	PASS