

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031715\
 Data File : BF077783.D
 Acq On : 17 Mar 2015 20:43
 Operator : TP/IZ
 Sample : G1544-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TW-8

Quant Time: Mar 18 02:20:32 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 18 00:52:09 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.16	152	39778	20.00	ng	0.00
21) Naphthalene-d8	8.74	136	154850	20.00	ng	0.00
38) Acenaphthene-d10	10.90	164	74648	20.00	ng	-0.01
63) Phenanthrene-d10	12.74	188	157517	20.00	ng	-0.01
75) Chrysene-d12	16.02	240	167461	20.00	ng	-0.01
86) Perylene-d12	17.71	264	161430	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	199752	87.65	ng	0.00
7) Phenol-d6	6.73	99	164905	58.57	ng	0.00
23) Nitrobenzene-d5	7.85	82	260223	110.16	ng	-0.01
41) 2,4,6-Tribromophenol	11.88	330	110653	154.93	ng	-0.01
44) 2-Fluorobiphenyl	10.09	172	581873	114.55	ng	0.00
78) Terphenyl-d14	14.74	244	664293	96.90	ng	0.00
Target Compounds						
49) Dimethylphthalate	10.59	163	12555	2.27	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031715\
Data File : BF077783.D
Acq On : 17 Mar 2015 20:43
Operator : TP/IZ
Sample : G1544-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-8

Quant Time: Mar 18 02:20:32 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 18 00:52:09 2015
Response via : Initial Calibration

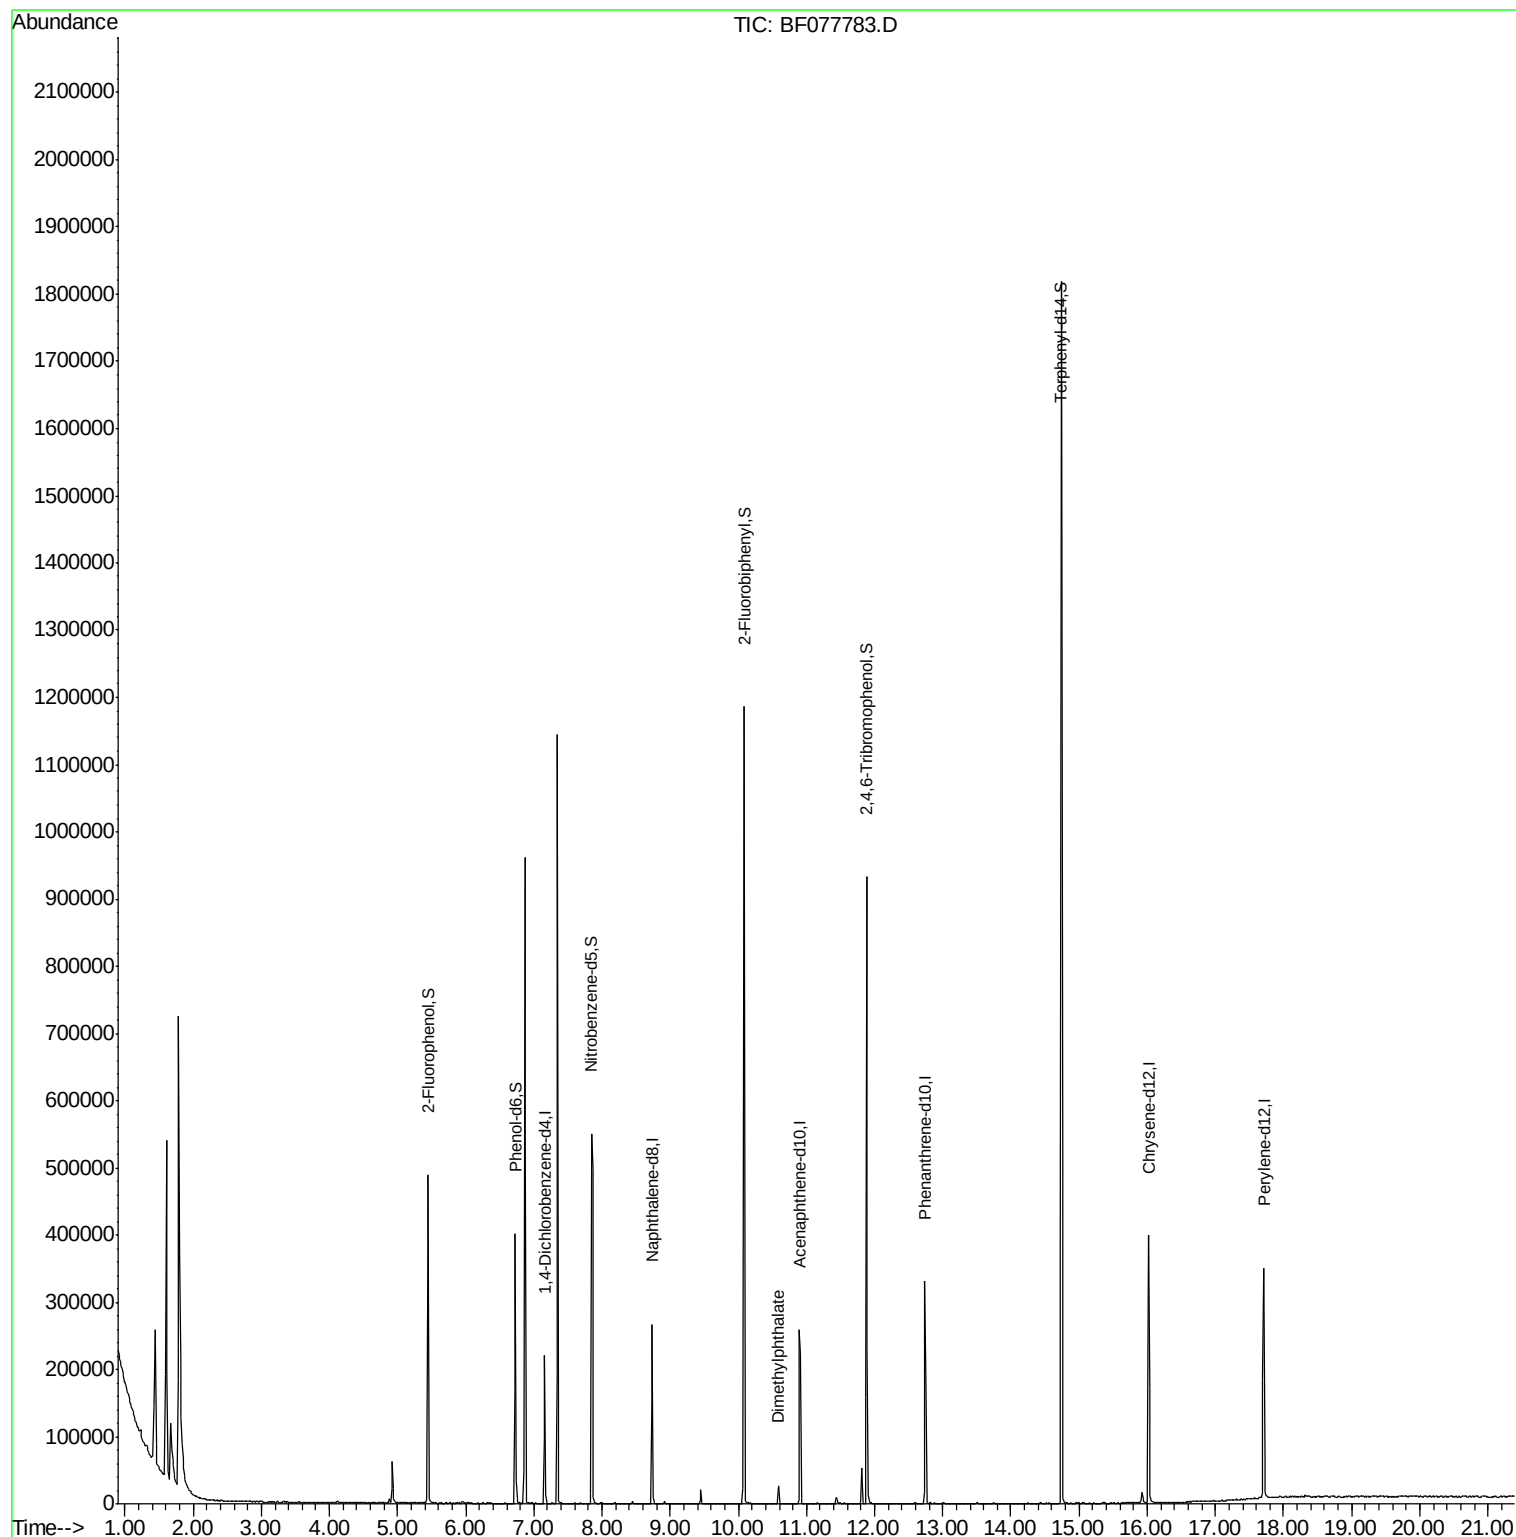

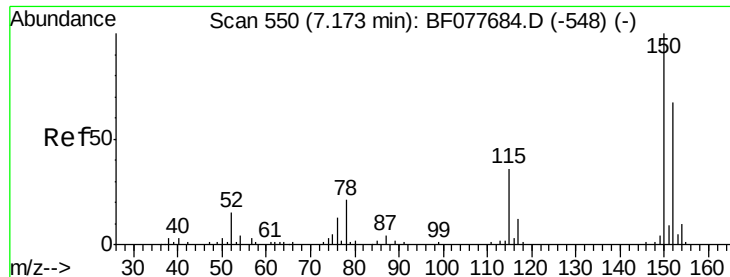


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.16 min Scan# 549
Delta R.T. -0.00 min
Lab File: BF077783.D
Acq: 17 Mar 2015 20:43

Instrument :
BNA_F
ClientSampleId :
TW-8

Tot Ion:152 Resp: 39778
Ion Ratio Lower Upper
152 100
150 158.3 119.5 179.3
115 53.6 43.0 64.4

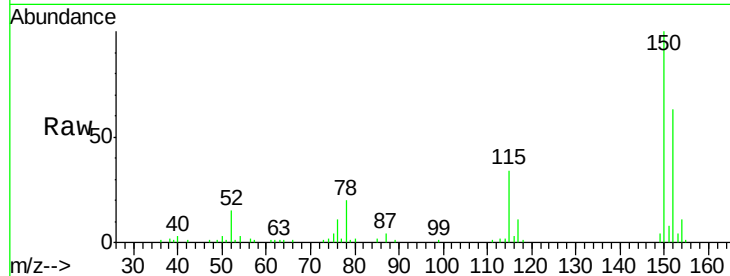


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

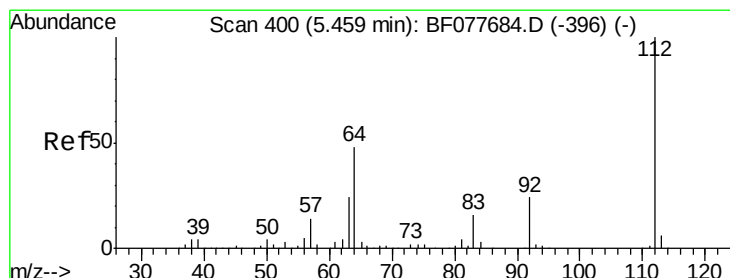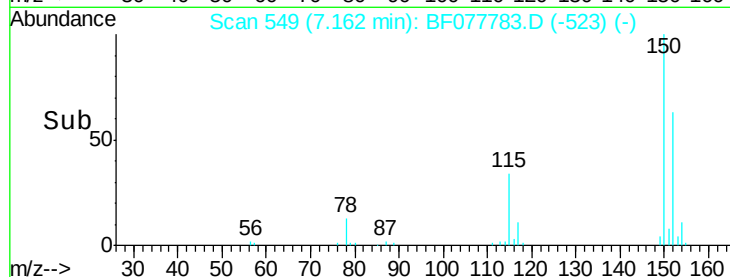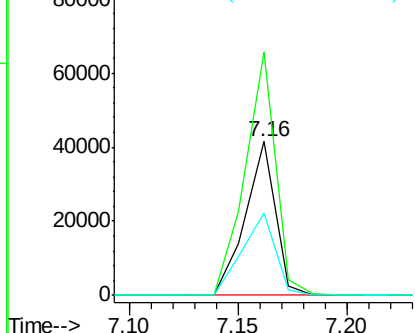



#5


2-Fluorophenol
Concen: 87.65 ng
RT: 5.45 min Scan# 399
Delta R.T. -0.00 min
Lab File: BF077783.D
Acq: 17 Mar 2015 20:43

Tgt Ion:112 Resp: 199752
Ion Ratio Lower Upper
112 100
64 50.4 38.6 57.8
63 25.5 19.3 28.9

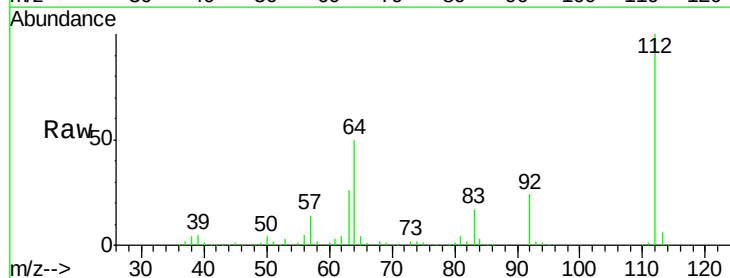

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

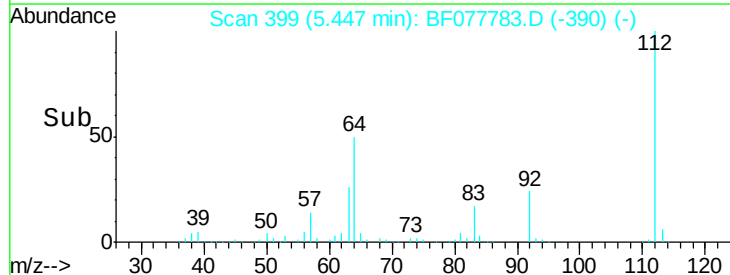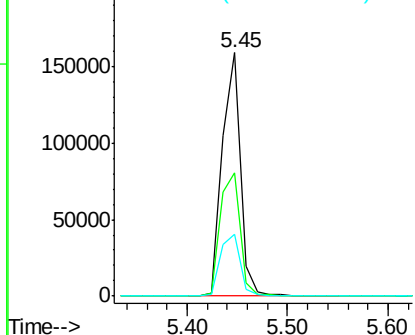

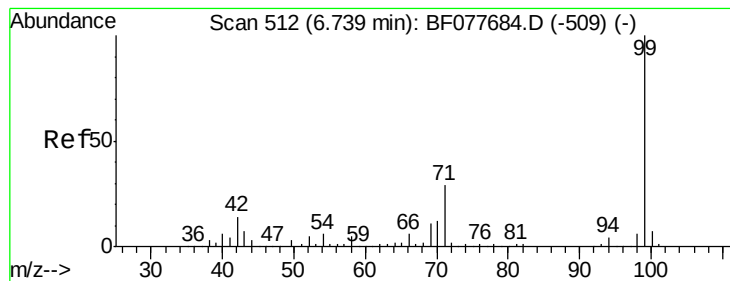

#7

Phenol-d6

Concen: 58.57 ng

RT: 6.73 min Scan# 511

Delta R.T. -0.00 min

Lab File: BF077783.D

Acq: 17 Mar 2015 20:43

Instrument :

BNA_F

ClientSampleId :

TW-8


Tot Ion: 99 Resp: 164905

Ion Ratio Lower Upper

99 100

42 14.0 11.0 16.4




71 29.0 23.4 35.2

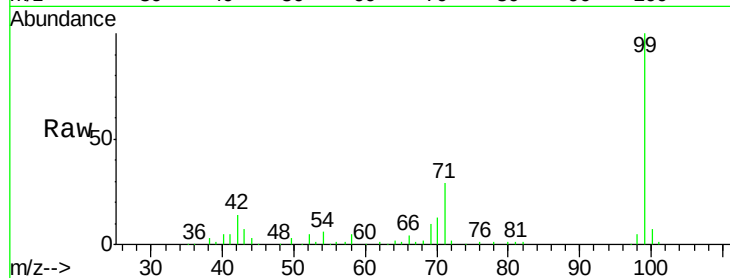

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

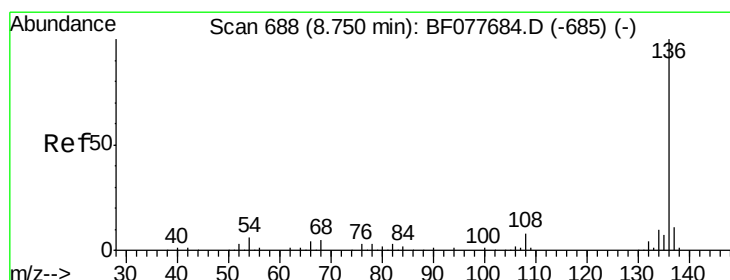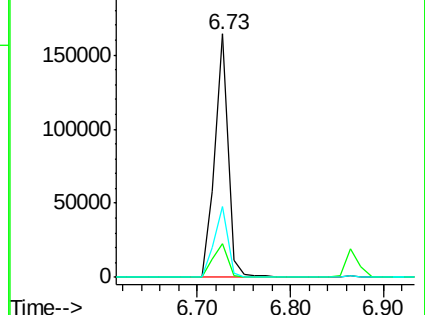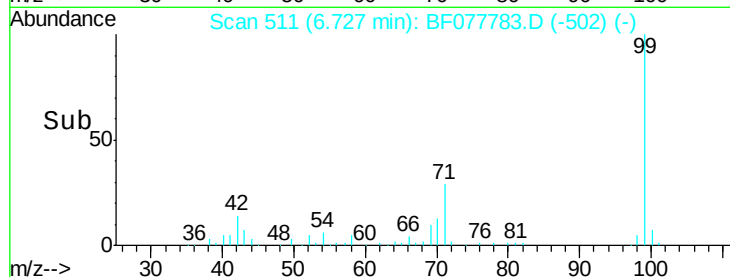

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.74 min Scan# 687

Delta R.T. -0.00 min

Lab File: BF077783.D

Acq: 17 Mar 2015 20:43

Tgt Ion: 136 Resp: 154850


Ion Ratio Lower Upper

136 100

137 10.3 8.7 13.1

54 6.0 4.6 6.8

68 4.9 3.7 5.5


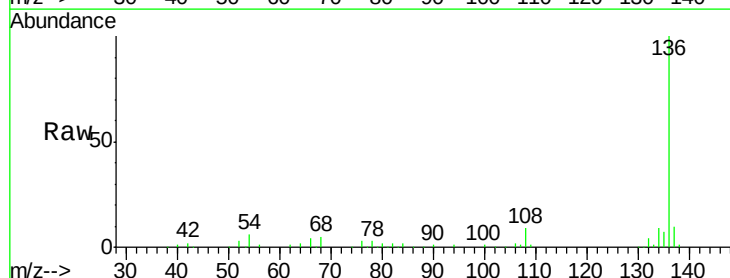



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

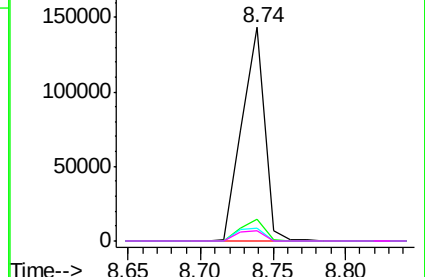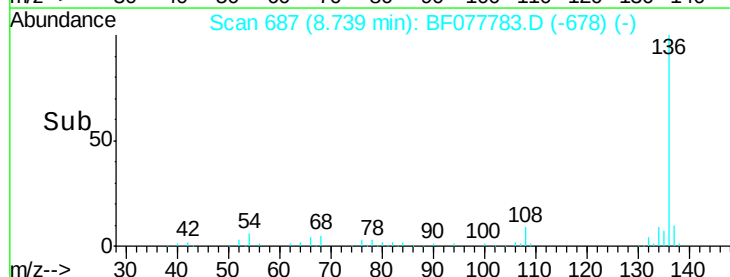


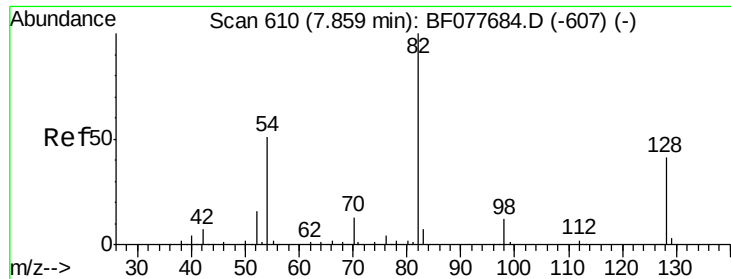




#23
 Nitrobenzene-d5
 Concen: 110.16 ng
 RT: 7.85 min Scan# 609
 Delta R.T. -0.01 min
 Lab File: BF077783.D
 Acq: 17 Mar 2015 20:43

Instrument :
 BNA_F
 ClientSampleId :
 TW-8

Tot Ion: 82 Resp: 260223
 Ion Ratio Lower Upper
 82 100
 128 38.8 32.8 49.2
 54 51.3 40.6 60.8

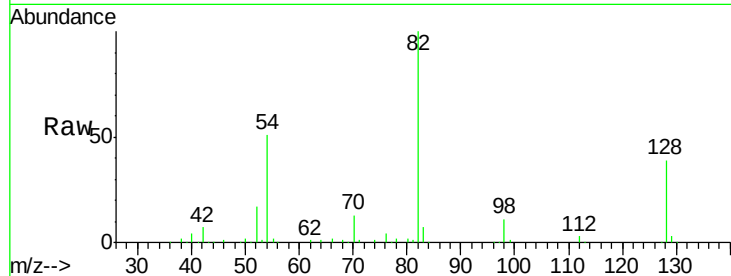


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

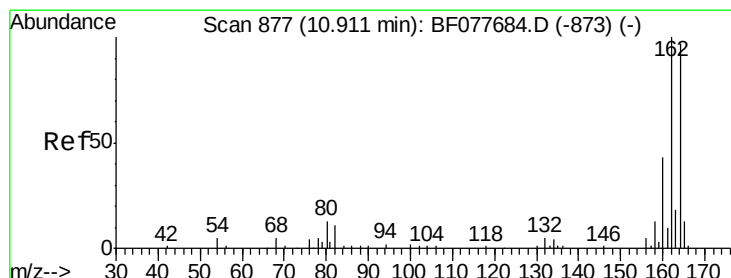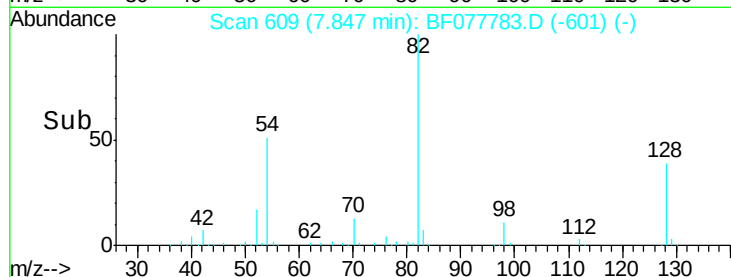
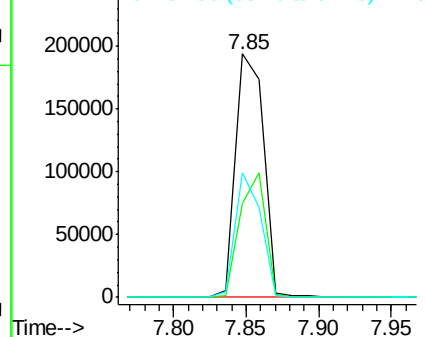



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.90 min Scan# 876
 Delta R.T. -0.01 min
 Lab File: BF077783.D
 Acq: 17 Mar 2015 20:43

Tgt Ion: 164 Resp: 74648
 Ion Ratio Lower Upper
 164 100
 162 101.0 82.4 123.6
 160 45.5 35.8 53.6

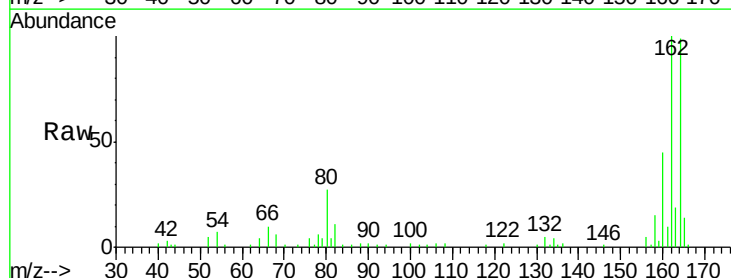

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



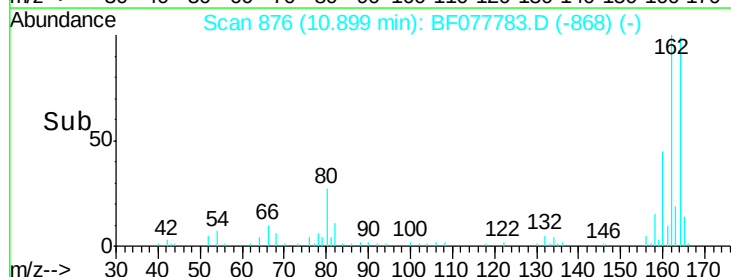
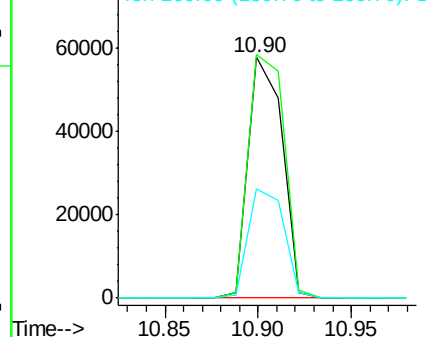


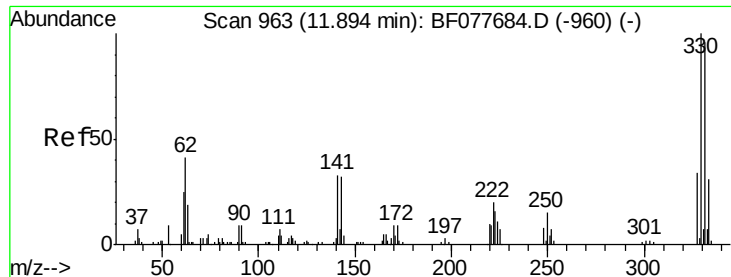

#41
 2,4,6-Tribromophenol
 Concen: 154.93 ng
 RT: 11.88 min Scan# 962
 Delta R.T. -0.01 min
 Lab File: BF077783.D
 Acq: 17 Mar 2015 20:43




Instrument :
 BNA_F
 ClientSampleId :
 TW-8


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	0.0	0.0#
141	38.9	0.0	0.0#

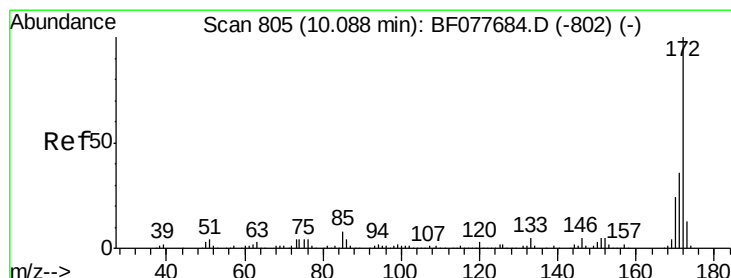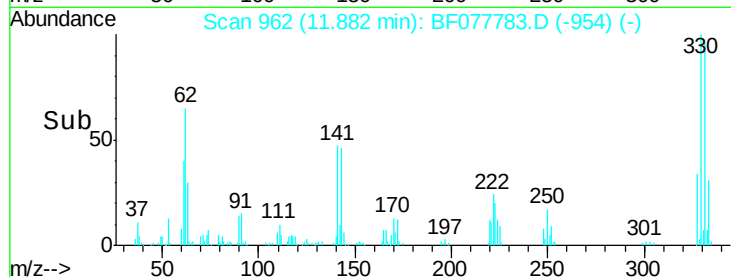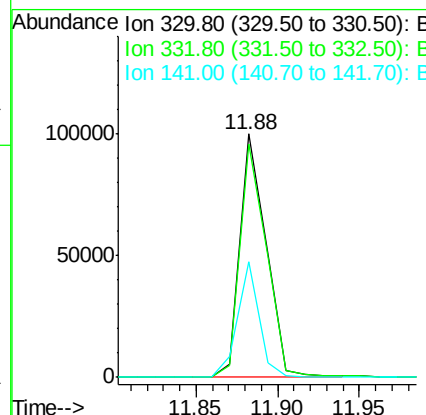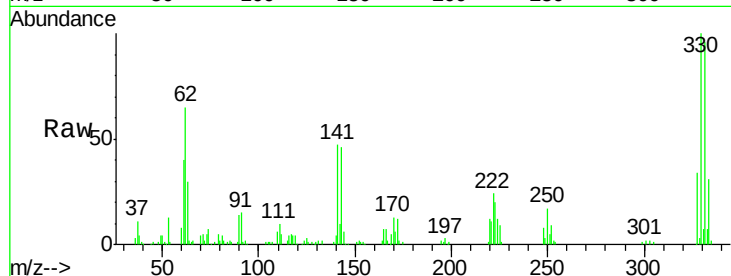

#44
 2-Fluorobiphenyl
 Concen: 114.55 ng
 RT: 10.09 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: BF077783.D
 Acq: 17 Mar 2015 20:43

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.8	28.5	42.7
170	23.0	18.8	28.2

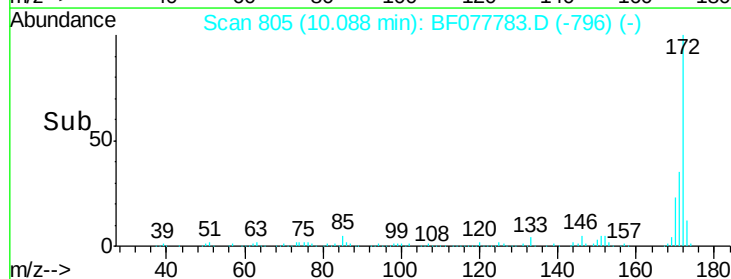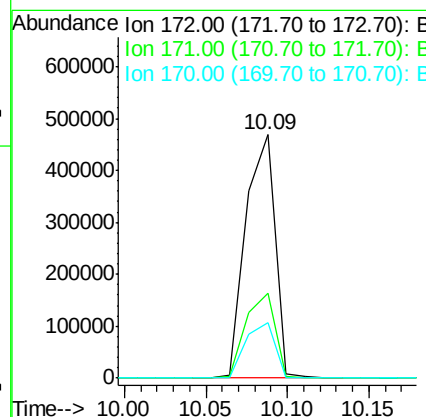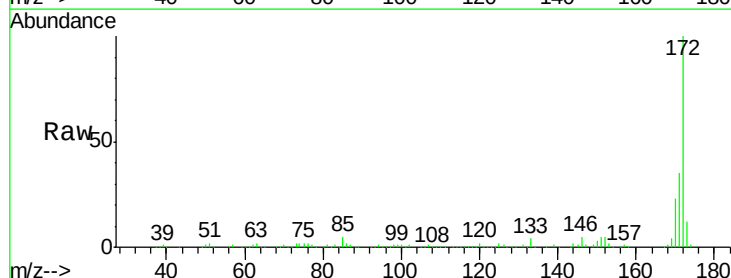

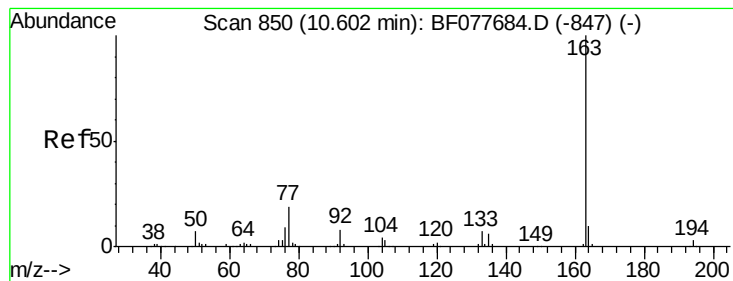

#49

Dimethylphthalate

Concen: 2.27 ng

RT: 10.59 min Scan# 849

Delta R.T. -0.01 min

Lab File: BF077783.D

Acq: 17 Mar 2015 20:43

Instrument :

BNA_F

ClientSampleId :

TW-8


Tot Ion:163 Resp: 12555

Ion Ratio Lower Upper

163 100

194 3.1 2.7 4.1




164 11.8 8.2 12.2

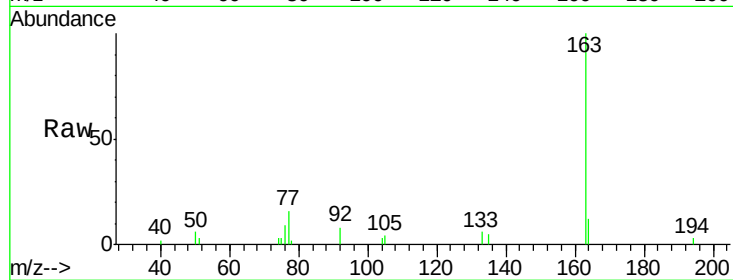

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

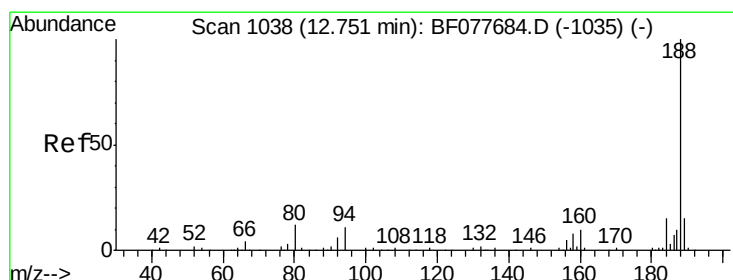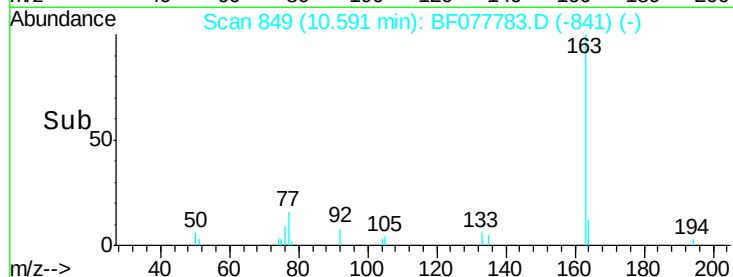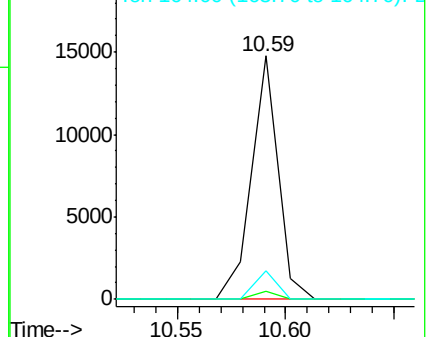

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.74 min Scan# 1037

Delta R.T. -0.01 min

Lab File: BF077783.D

Acq: 17 Mar 2015 20:43


Tgt Ion:188 Resp: 157517

Ion Ratio Lower Upper

188 100

94 12.0 8.7 13.1



80 12.8 9.3 13.9

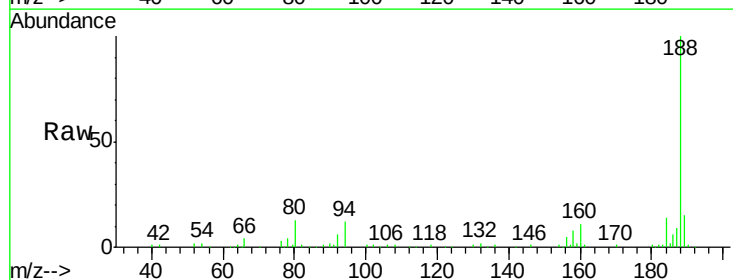


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



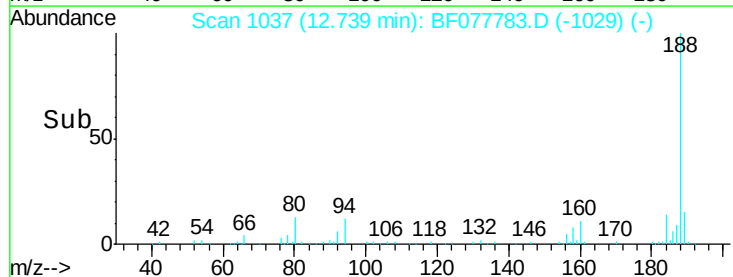
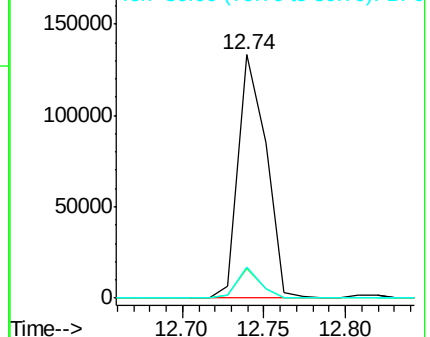


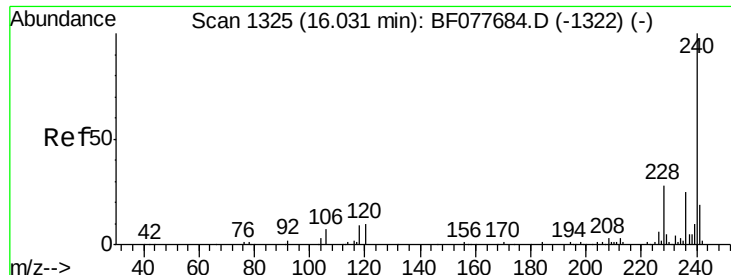

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 16.02 min Scan# 1324
 Delta R.T. -0.01 min
 Lab File: BF077783.D
 Acq: 17 Mar 2015 20:43




Instrument :
 BNA_F
 ClientSampleId :
 TW-8




Tot Ion:240 Resp: 167461
 Ion Ratio Lower Upper
 240 100
 120 13.6 8.2 12.2#
 236 24.8 20.0 30.0

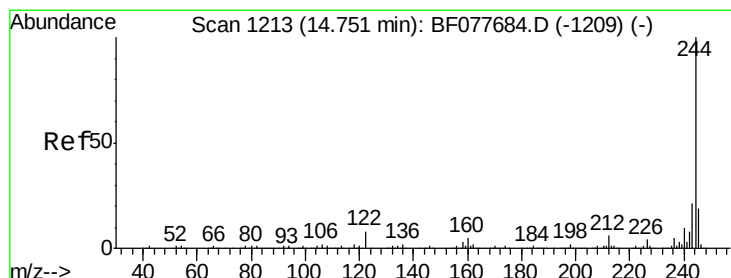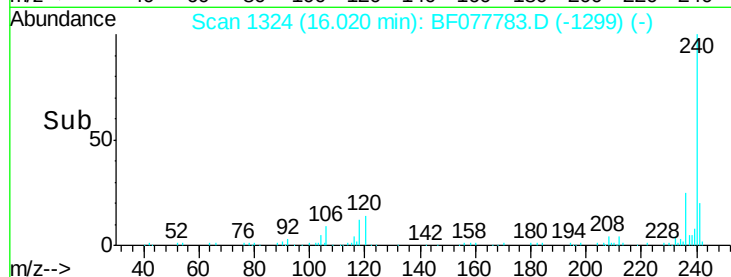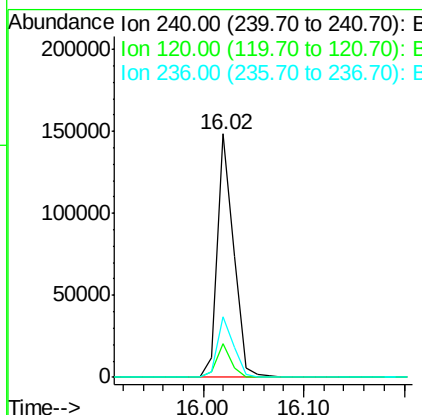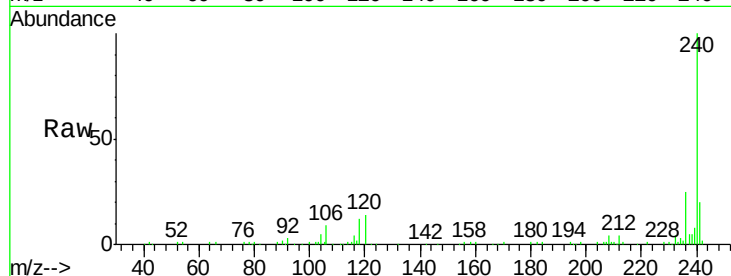

#78
 Terphenyl-d14
 Concen: 96.90 ng
 RT: 14.74 min Scan# 1212
 Delta R.T. -0.00 min
 Lab File: BF077783.D
 Acq: 17 Mar 2015 20:43

Tgt Ion:244 Resp: 664293
 Ion Ratio Lower Upper
 244 100
 212 6.8 4.9 7.3
 122 13.7 6.2 9.4#

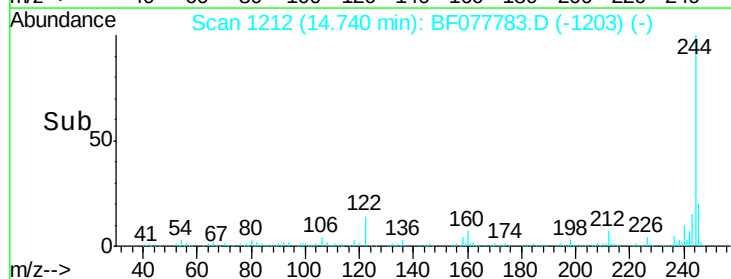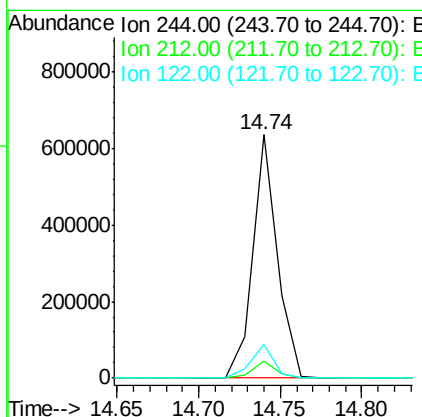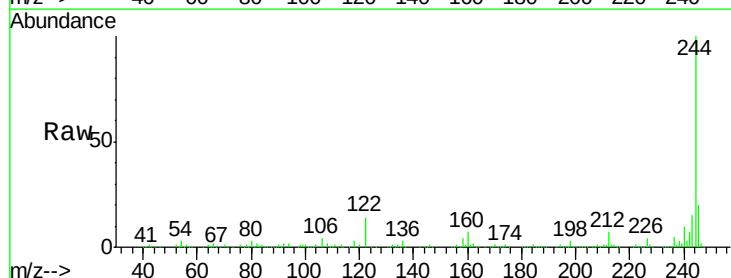

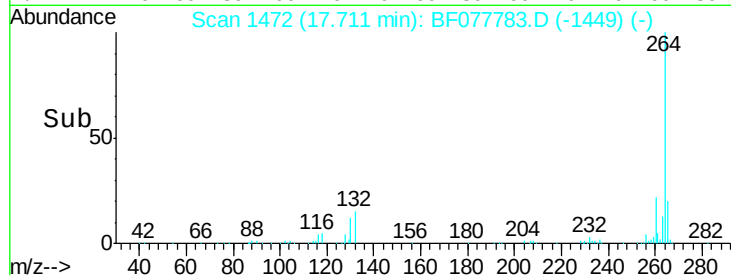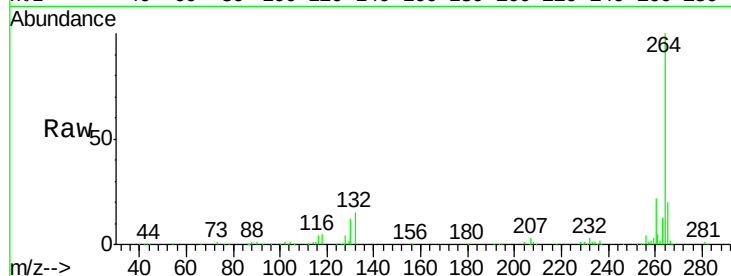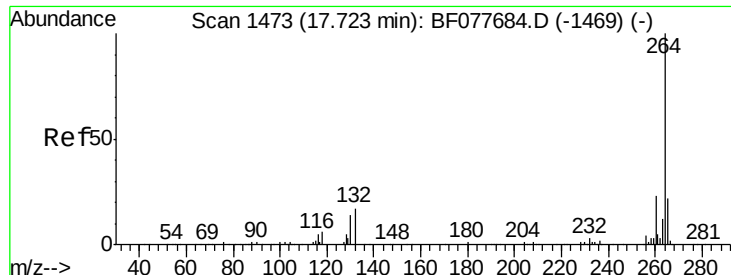

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 17.71 min Scan# 1472
 Delta R.T. -0.03 min
 Lab File: BF077783.D
 Acq: 17 Mar 2015 20:43

Instrument :
 BNA_F
 ClientSampleId :
 TW-8

Tot Ion:	264	Resp:	161430
Ion	Ratio	Lower	Upper
264	100		
260	22.2	18.6	27.8
265	20.3	17.3	25.9

