

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF031715\  
Data File : BF077773.D  
Acq On : 17 Mar 2015 15:37  
Operator : TP/IZ  
Sample : G1536-05  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031115.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.435       | 46            | 48          | 50           | rVB      | 38661          | 52633         | 7.29%           | 1.515%        |
| 2         | 1.790       | 77            | 79          | 106          | rVB      | 425133         | 721622        | 100.00%         | 20.776%       |
| 3         | 7.162       | 547           | 549         | 551          | rBV      | 286244         | 271771        | 37.66%          | 7.824%        |
| 4         | 8.739       | 685           | 687         | 689          | rBV      | 405832         | 389118        | 53.92%          | 11.203%       |
| 5         | 10.911      | 875           | 877         | 879          | rVB      | 397119         | 454254        | 62.95%          | 13.078%       |
| 6         | 12.751      | 1035          | 1038        | 1040         | rBV      | 377674         | 485151        | 67.23%          | 13.968%       |
| 7         | 14.442      | 1184          | 1186        | 1188         | rBV      | 6303           | 8892          | 1.23%           | 0.256%        |
| 8         | 16.031      | 1323          | 1325        | 1328         | rBV      | 476354         | 538733        | 74.66%          | 15.510%       |
| 9         | 17.791      | 1476          | 1479        | 1485         | rBV      | 373884         | 540790        | 74.94%          | 15.570%       |
| 10        | 20.031      | 1672          | 1675        | 1680         | rBV5     | 2674           | 10390         | 1.44%           | 0.299%        |


Sum of corrected areas: 3473354

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF031715\  
Data File : BF077773.D  
Acq On : 17 Mar 2015 15:37  
Operator : TP/IZ  
Sample : G1536-05  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

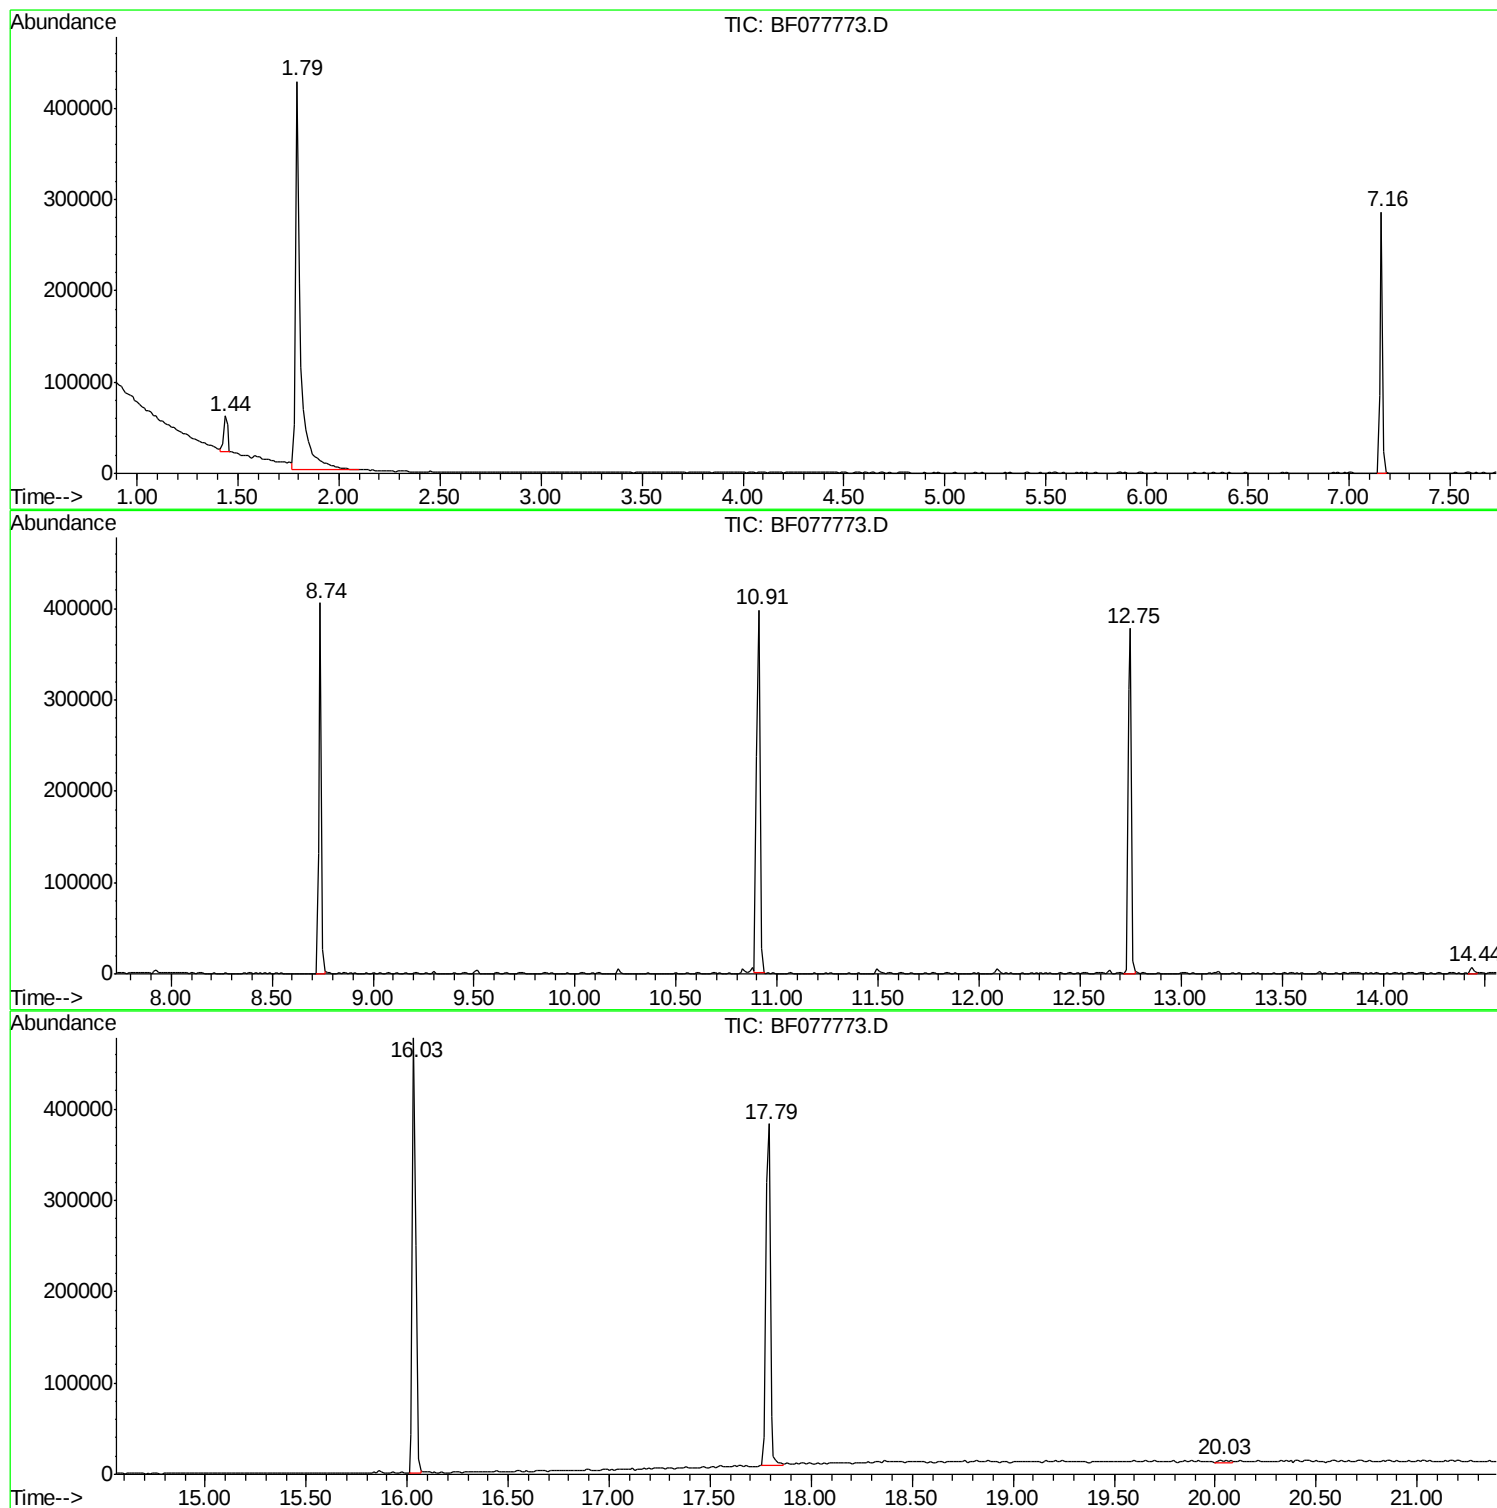

Data\_Path : Z:\HPCHEM1\BNA\_F\DATA\BF031715\  
Data\_File : BF077773.D  
Acq\_On : 17 Mar 2015 15:377  
Operator : TP/IZZ  
Sample : G1536-055  
Misc :  
ALS\_Vial : 7 Sample\_Multiplier: 11

Instrument :  
BNA\_F  
ClientSampleId :  
SVOC-GPC-BLANK

Quant\_Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031115.MM  
Quant\_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC\_Library : C:\DATABASE\NIST02.LL  
TIC\_Integration\_Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       | #        | RT Resp Conc            |

No Library Search Compounds Detected

\*\*\*\*\*