
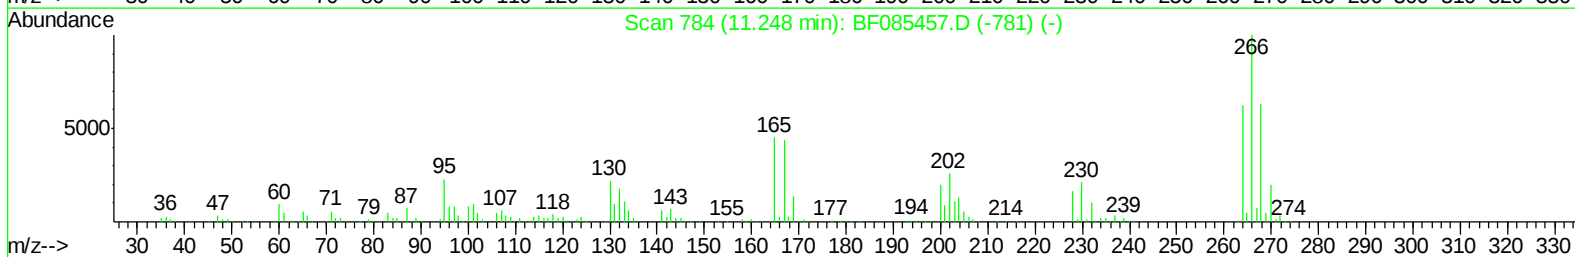
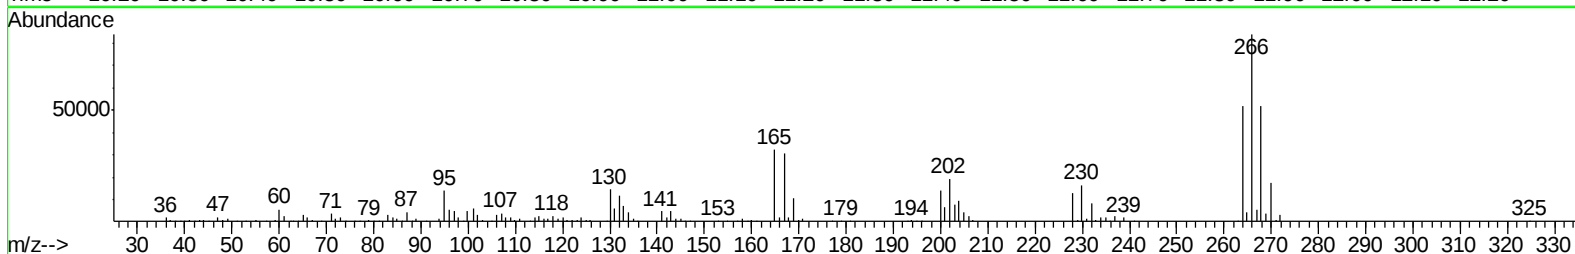


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031716\
Data File : BF085497.D
Acq On : 17 Mar 2016 11:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 03:33:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

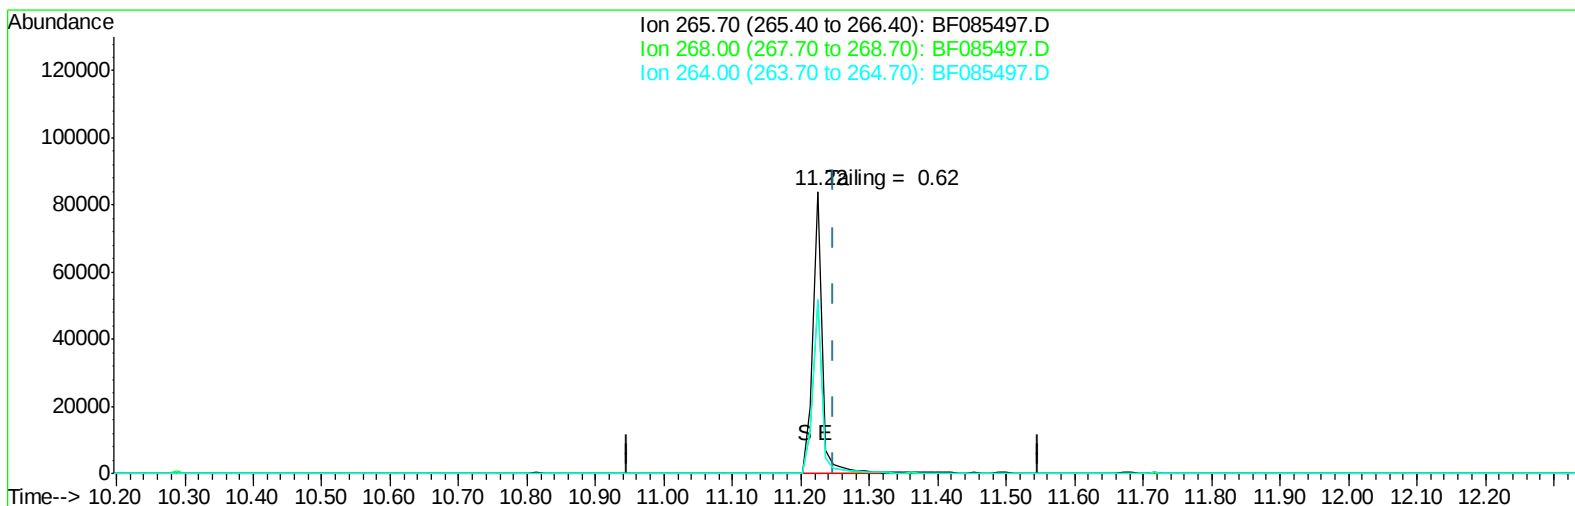

TIC: BF085497.D

(69) Pentachlorophenol (C)




11.225min (-0.023) 17050.67ng

response 81925

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	61.53
264.00	64.30	61.74
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031716\
Data File : BF085497.D
Acq On : 17 Mar 2016 11:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 03:33:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

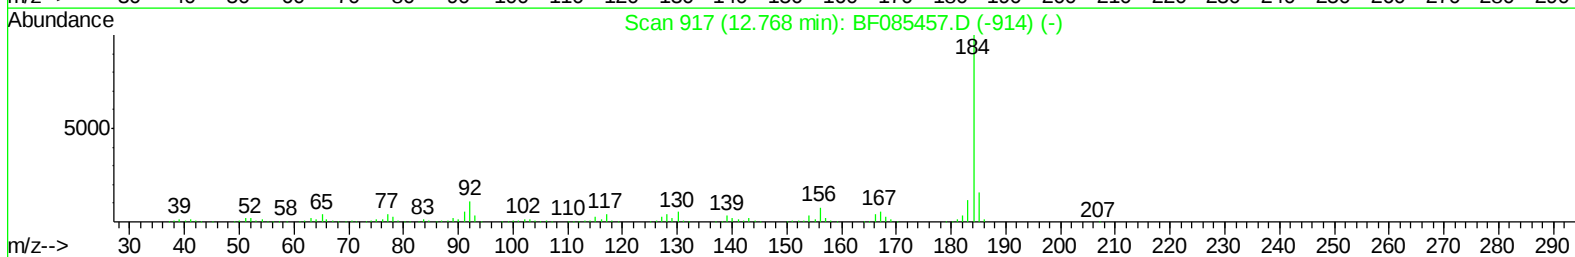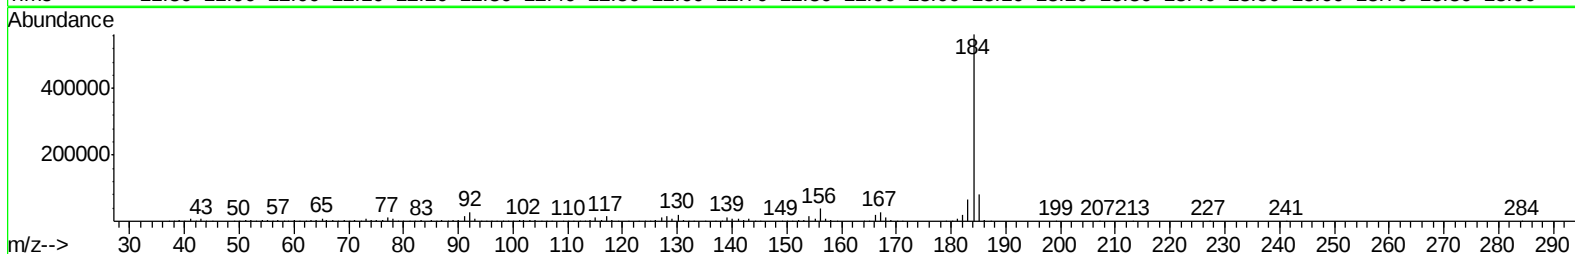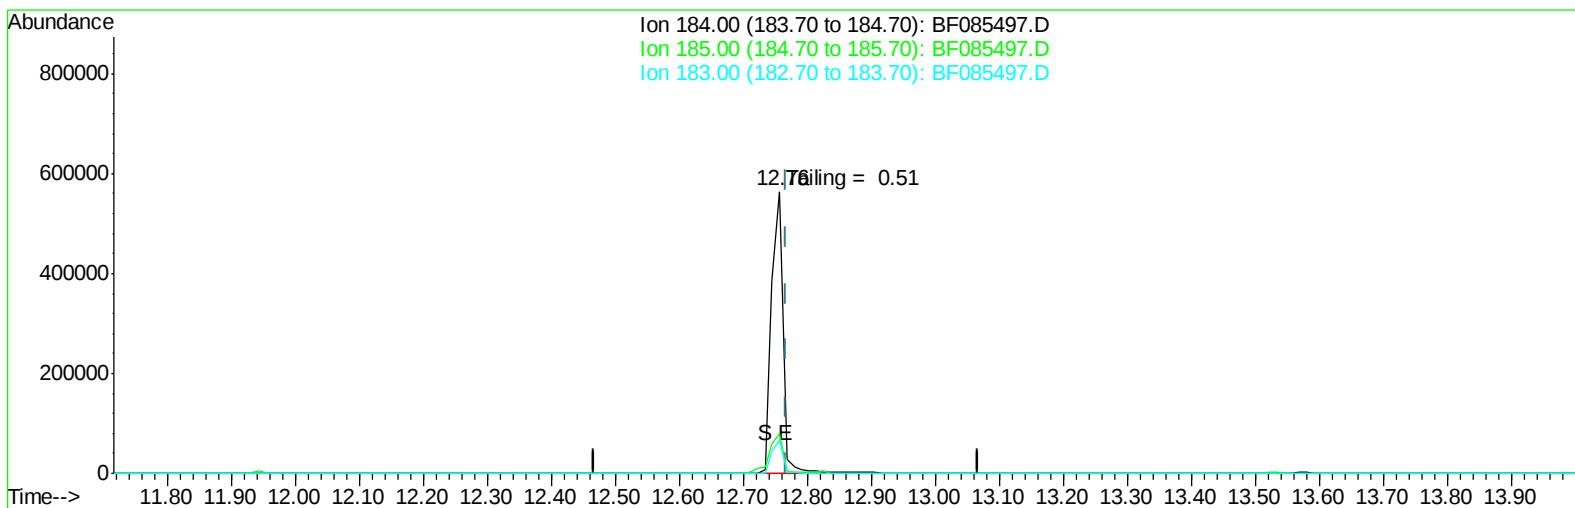

TIC: BF085497.D

(76) Benzidine

12.757min (-0.011) 0.00ng

response 713751

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.23
183.00	11.80	11.72
0.00	0.00	0.00