
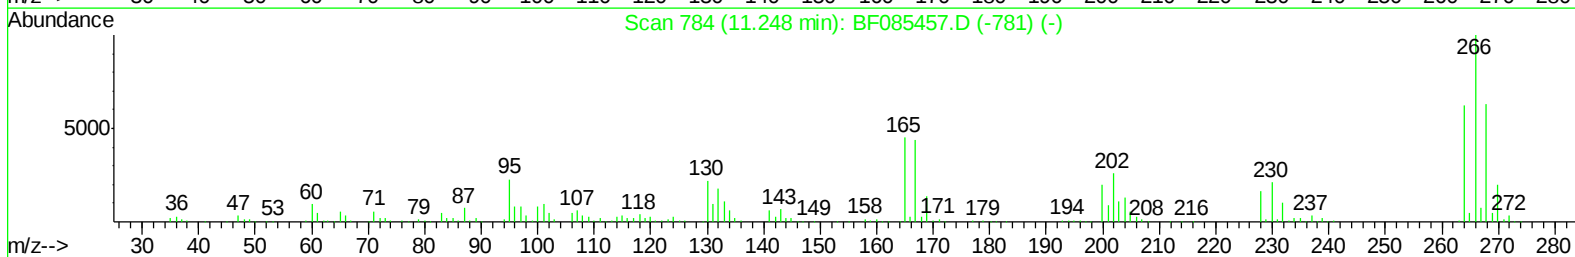
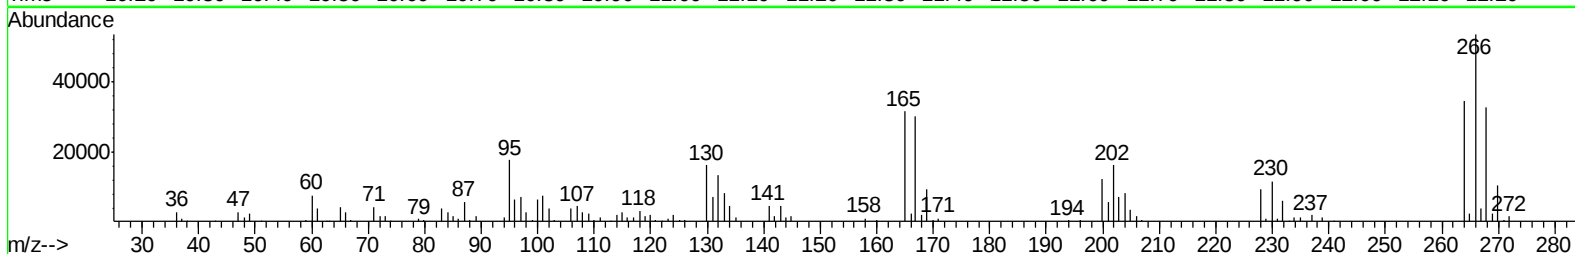


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031716\
Data File : BF085519.D
Acq On : 18 Mar 2016 4:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 03:51:17 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 18:57:05 2016
Response via : Initial Calibration

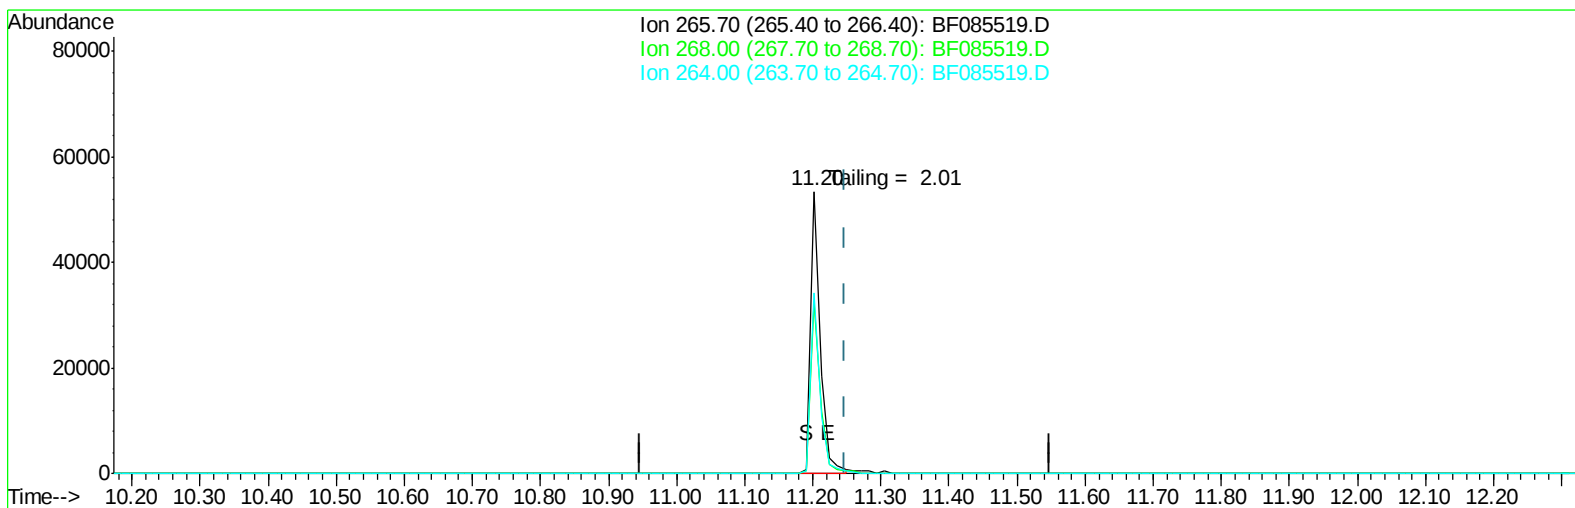

TIC: BF085519.D

(69) Pentachlorophenol (C)




11.202min (-0.046) 45955.88ng

response 54439

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	60.89
264.00	64.30	64.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031716\
 Data File : BF085519.D
 Acq On : 18 Mar 2016 4:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 03:51:17 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 18:57:05 2016
 Response via : Initial Calibration

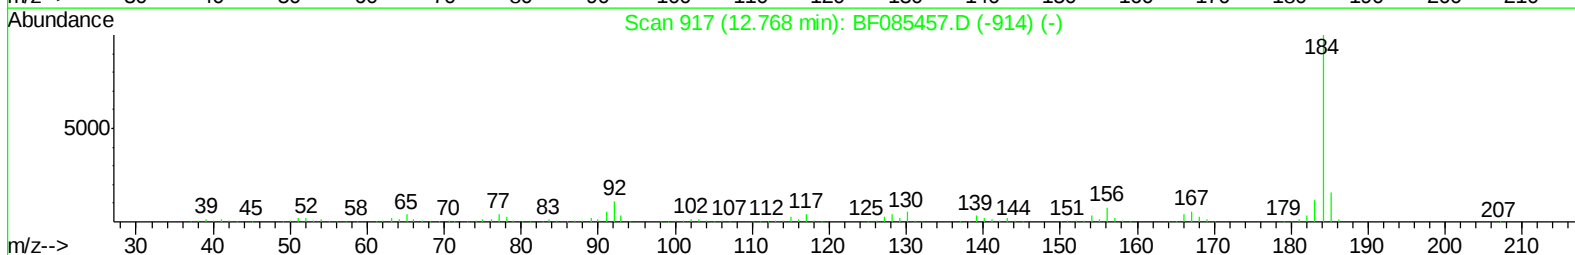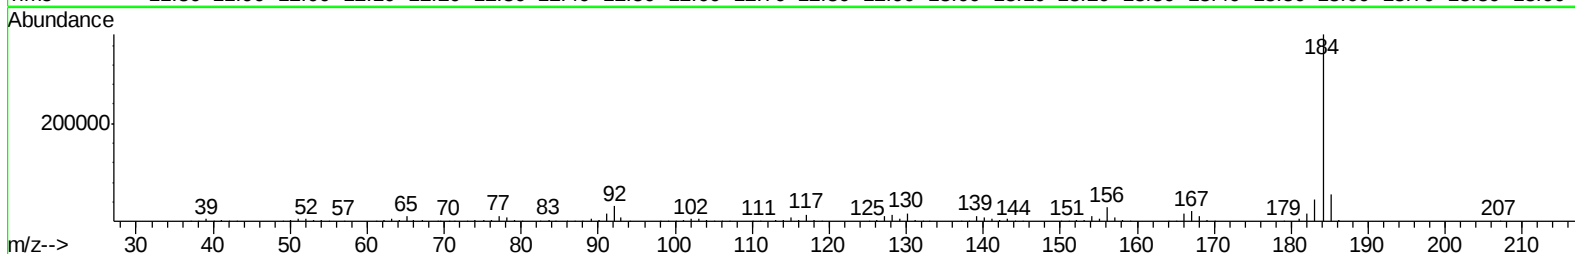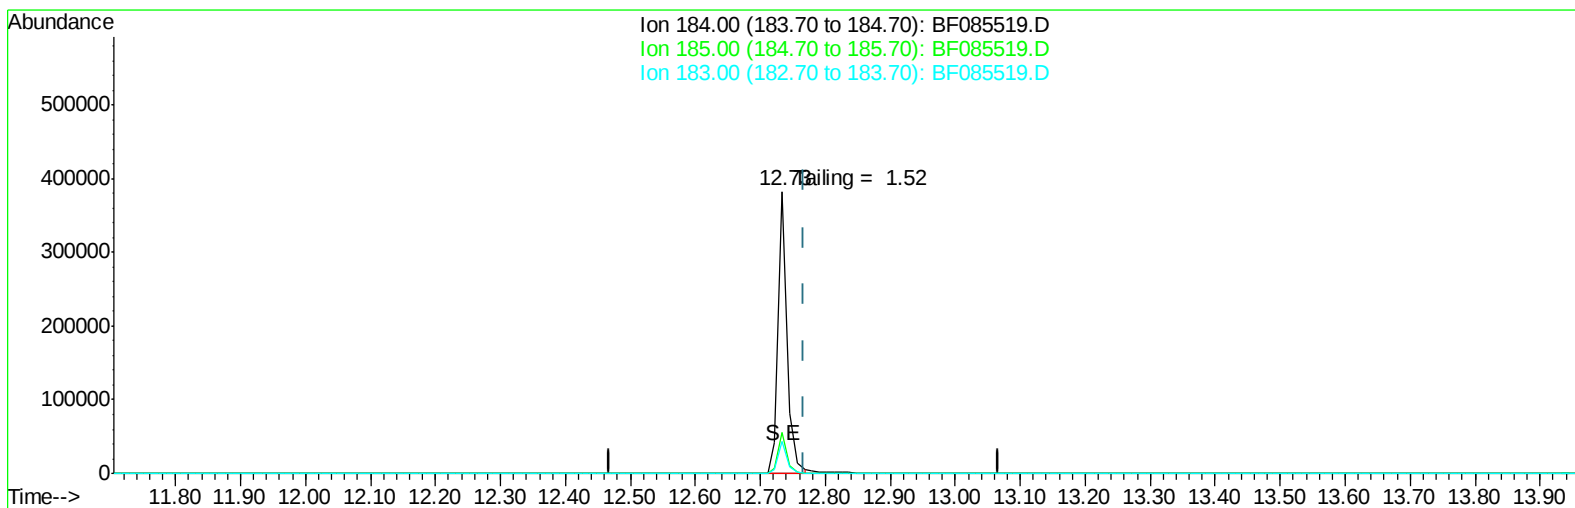

TIC: BF085519.D

(76) Benzidine

12.734min (-0.034) 14243.23ng

response 372069

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.38
183.00	11.80	11.59
0.00	0.00	0.00