

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF031716\  
 Data File : BF085503.D  
 Acq On : 17 Mar 2016 20:51  
 Operator : UM/SJ  
 Sample : PB88925BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB88925BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031516.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.087       | 242           | 245         | 249          | rBV      | 33309          | 61956         | 1.91%           | 0.231%        |
| 2         | 5.476       | 276           | 279         | 282          | rBV      | 2382348        | 2656633       | 81.93%          | 9.917%        |
| 3         | 6.504       | 366           | 369         | 371          | rBV      | 2609329        | 2657978       | 81.97%          | 9.922%        |
| 4         | 6.642       | 378           | 381         | 383          | rBV      | 2995555        | 2854333       | 88.03%          | 10.655%       |
| 5         | 6.870       | 399           | 401         | 404          | rBV      | 813099         | 821457        | 25.33%          | 3.066%        |
| 6         | 7.030       | 412           | 415         | 417          | rBV      | 2634838        | 2324817       | 71.70%          | 8.678%        |
| 7         | 7.442       | 448           | 451         | 453          | rBV      | 1803796        | 2068384       | 63.79%          | 7.721%        |
| 8         | 8.162       | 511           | 514         | 516          | rBV      | 1241343        | 1171497       | 36.13%          | 4.373%        |
| 9         | 9.236       | 605           | 608         | 611          | rBV      | 3144100        | 3242527       | 100.00%         | 12.104%       |
| 10        | 9.910       | 665           | 667         | 670          | rBV      | 861032         | 1167345       | 36.00%          | 4.357%        |
| 11        | 10.699      | 734           | 736         | 739          | rBV2     | 1477551        | 1887505       | 58.21%          | 7.046%        |
| 12        | 11.396      | 795           | 797         | 800          | rBV      | 1249649        | 1141151       | 35.19%          | 4.260%        |
| 13        | 12.985      | 933           | 936         | 938          | rBV      | 3263283        | 3015779       | 93.01%          | 11.257%       |
| 14        | 14.037      | 1025          | 1028        | 1030         | rBV      | 700201         | 836493        | 25.80%          | 3.122%        |
| 15        | 15.465      | 1150          | 1153        | 1156         | rBV      | 548357         | 702793        | 21.67%          | 2.623%        |
| 16        | 16.563      | 1247          | 1249        | 1250         | rBV2     | 47113          | 32666         | 1.01%           | 0.122%        |
| 17        | 17.031      | 1289          | 1290        | 1294         | rBV4     | 54144          | 103499        | 3.19%           | 0.386%        |
| 18        | 17.454      | 1325          | 1327        | 1330         | rVB3     | 33697          | 43062         | 1.33%           | 0.161%        |


Sum of corrected areas: 26789875

Data Path : Z:\HPCHEM1\BNA F\Data\BF031716\  
Data File : BF085503.D  
Acq On : 17 Mar 2016 20:51  
Operator : UM/SJ  
Sample : PB88925BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB88925BL

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031516.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

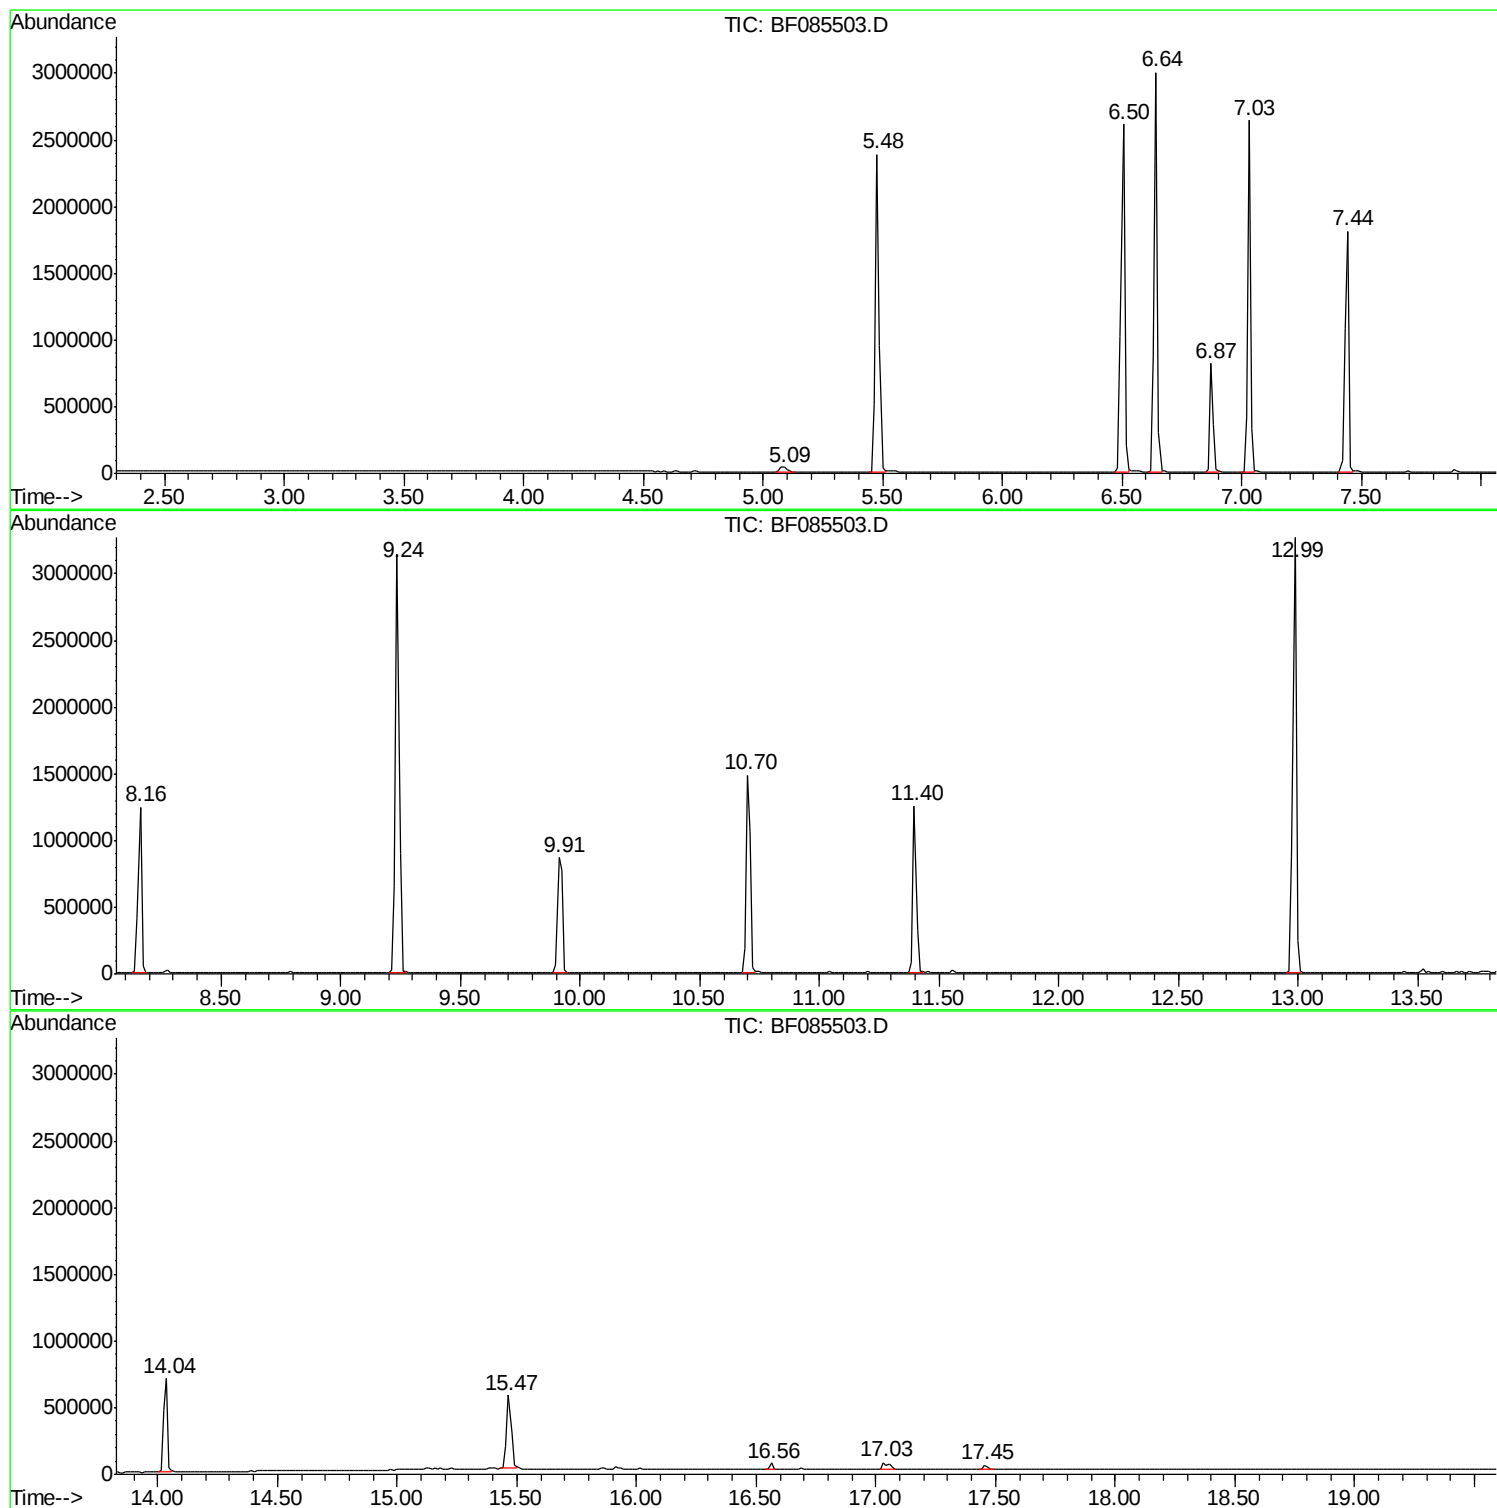

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF031716\  
Data File : BF085503.D  
Acq On : 17 Mar 2016 20:51  
Operator : UM/SJ  
Sample : PB88925BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB88925BL

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031516.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF031716\  
Data File : BF085503.D  
Acq On : 17 Mar 2016 20:51  
Operator : UM/SJ  
Sample : PB88925BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB88925BL

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031516.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |