


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF031716\  
 Data File : BF085497.D  
 Acq On : 17 Mar 2016 11:39  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031516.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Mar 15 18:57:05 2016

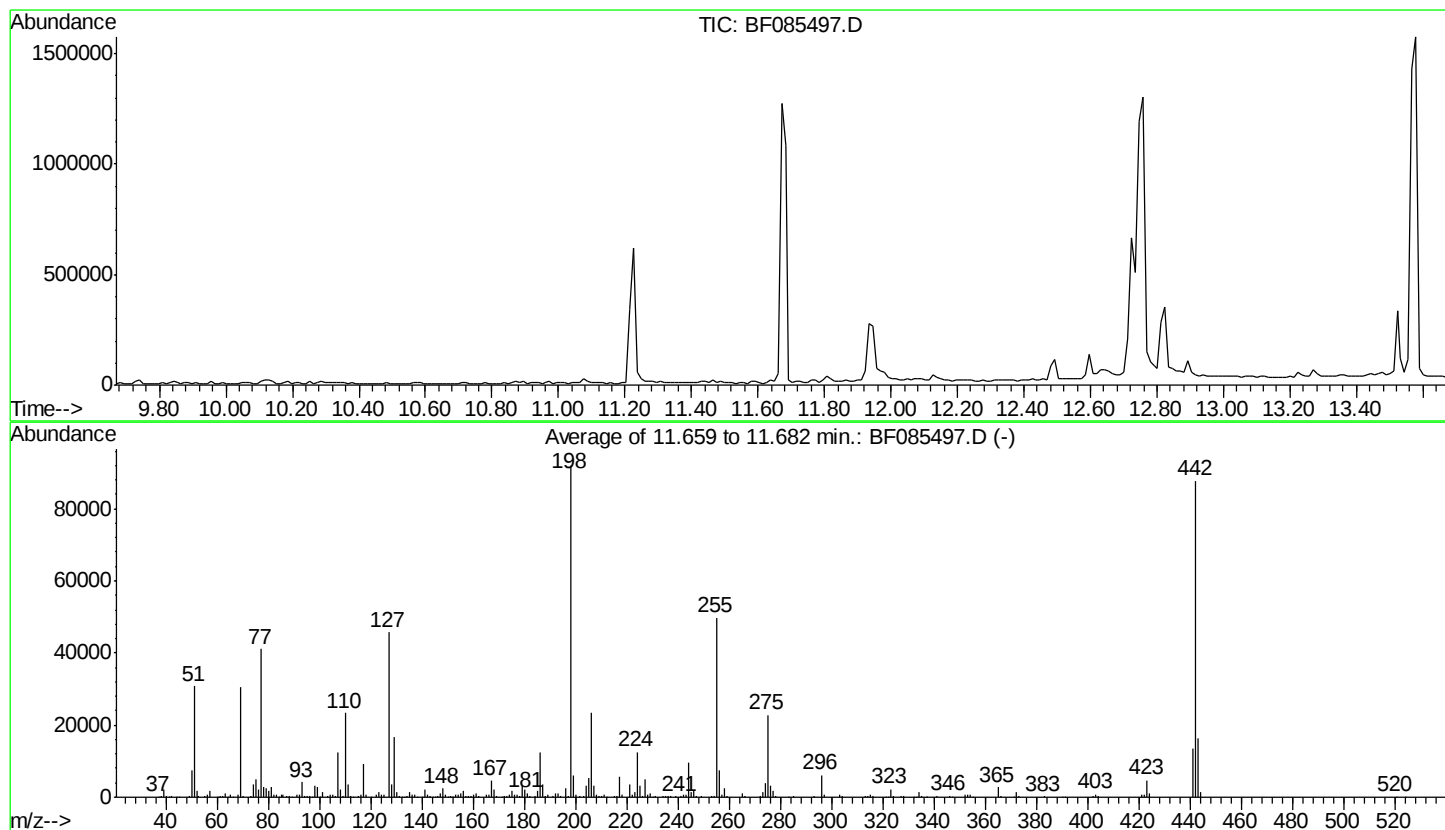

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 33.4      | 30730   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 567     | PASS             |
| 69          | 198          | 0.00         | 100          | 33.4      | 30672   | PASS             |
| 70          | 69           | 0.00         | 2            | 1.0       | 306     | PASS             |
| 127         | 198          | 10           | 80           | 49.7      | 45674   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 270     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 91948   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 6121    | PASS             |
| 275         | 198          | 10           | 60           | 24.9      | 22856   | PASS             |
| 365         | 198          | 1            | 100          | 3.1       | 2805    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.2      | 13334   | PASS             |
| 442         | 198          | 50           | 100          | 95.4      | 87752   | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 16474   | PASS             |