


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031716\
Data File : BF085497.D
Acq On : 17 Mar 2016 11:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 15 18:57:05 2016

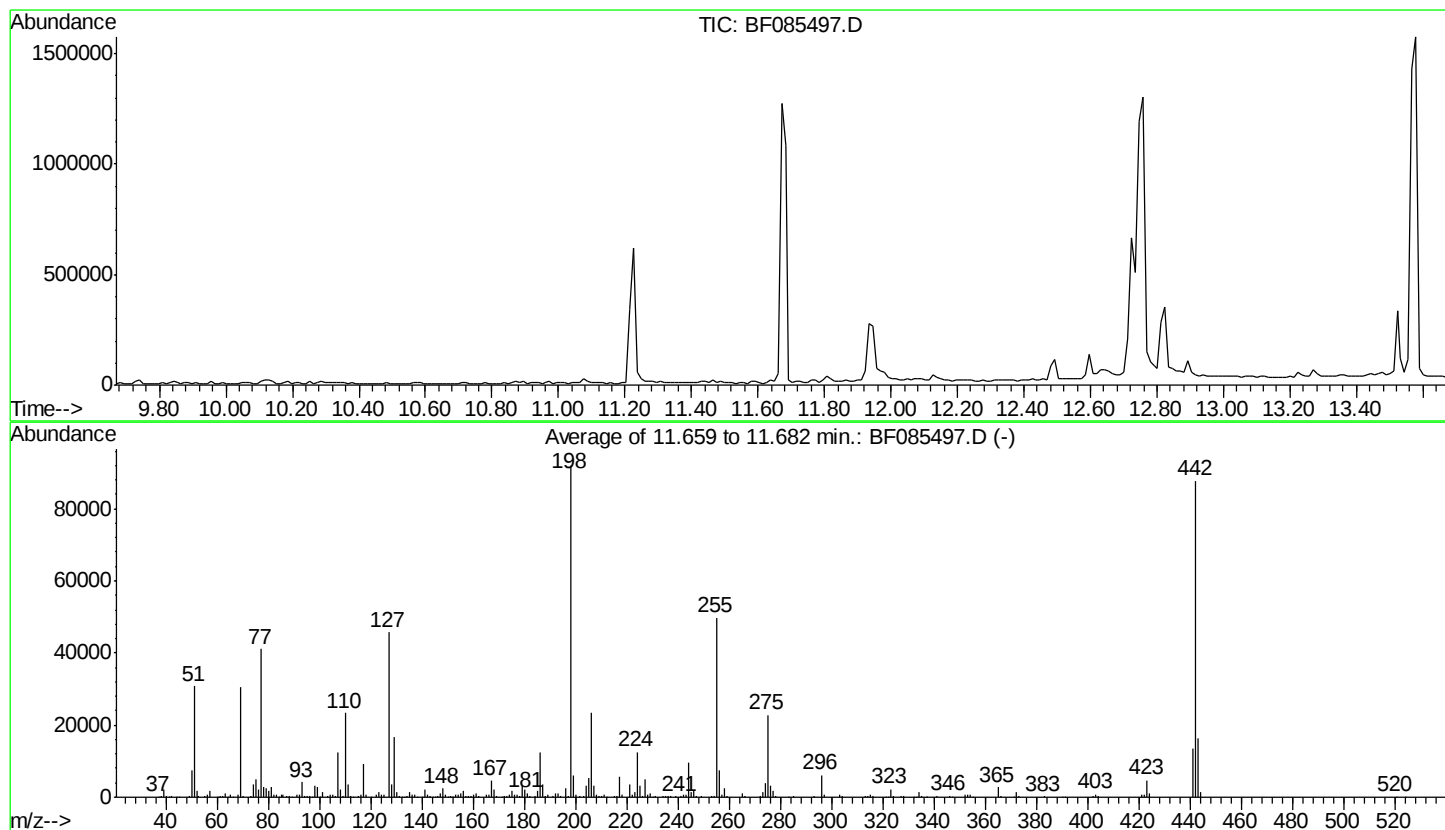

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	30730	PASS
68	69	0.00	2	1.8	567	PASS
69	198	0.00	100	33.4	30672	PASS
70	69	0.00	2	1.0	306	PASS
127	198	10	80	49.7	45674	PASS
197	198	0.00	2	0.3	270	PASS
198	198	100	100	100.0	91948	PASS
199	198	5	9	6.7	6121	PASS
275	198	10	60	24.9	22856	PASS
365	198	1	100	3.1	2805	PASS
441	442	0.01	24	15.2	13334	PASS
442	198	50	100	95.4	87752	PASS
443	442	15	24	18.8	16474	PASS