


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031716\
 Data File : BF085519.D
 Acq On : 18 Mar 2016 4:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 15 18:57:05 2016

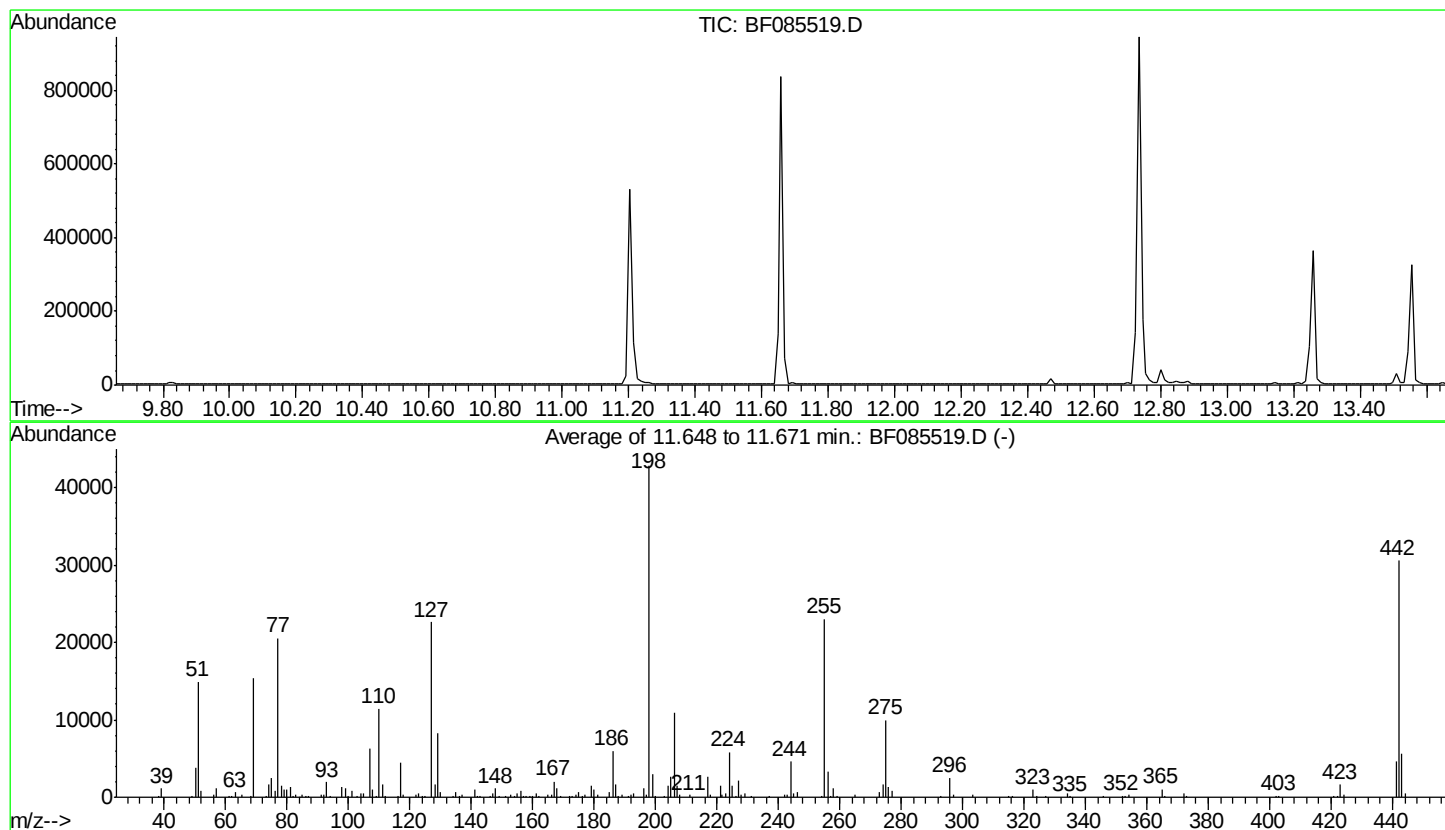

AutoFind: Scans 819, 820, 821; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	14891	PASS
68	69	0.00	2	1.3	202	PASS
69	198	0.00	100	36.0	15429	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	22586	PASS
197	198	0.00	2	0.6	254	PASS
198	198	100	100	100.0	42832	PASS
199	198	5	9	6.9	2955	PASS
275	198	10	60	23.3	9992	PASS
365	198	1	100	2.4	1016	PASS
441	442	0.01	24	15.4	4714	PASS
442	198	50	100	71.4	30570	PASS
443	442	15	24	18.6	5697	PASS