

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
 Data File : BF127368.D
 Acq On : 17 Mar 2022 11:12
 Operator : CG\JU
 Sample : PB143399BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143399BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	543	548	551	rBV	3278183	3394907	78.38%	12.999%
2	6.504	711	717	720	rBV	2900830	3495576	80.70%	13.384%
3	6.863	775	778	782	rBV	877389	761033	17.57%	2.914%
4	7.433	869	875	878	rBV	2068738	2487444	57.43%	9.524%
5	8.145	991	996	1000	rBV	980901	990226	22.86%	3.792%
6	9.227	1173	1180	1183	rBV	4089850	4114547	94.99%	15.754%
7	9.904	1289	1295	1299	rBV	1248179	1166102	26.92%	4.465%
8	10.704	1426	1431	1434	rBV	2550036	2423374	55.95%	9.279%
9	11.398	1545	1549	1556	rBV	1420176	1189333	27.46%	4.554%
10	12.992	1814	1820	1823	rBV	4164194	4331529	100.00%	16.585%
11	14.045	1995	1999	2009	rBV	1089375	976126	22.54%	3.738%
12	15.533	2246	2252	2269	rBV	506317	741603	17.12%	2.840%
13	17.239	2533	2542	2544	rBV8	21054	44911	1.04%	0.172%




Sum of corrected areas: 26116711

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127368.D
Acq On : 17 Mar 2022 11:12
Operator : CG\JU
Sample : PB143399BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143399BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

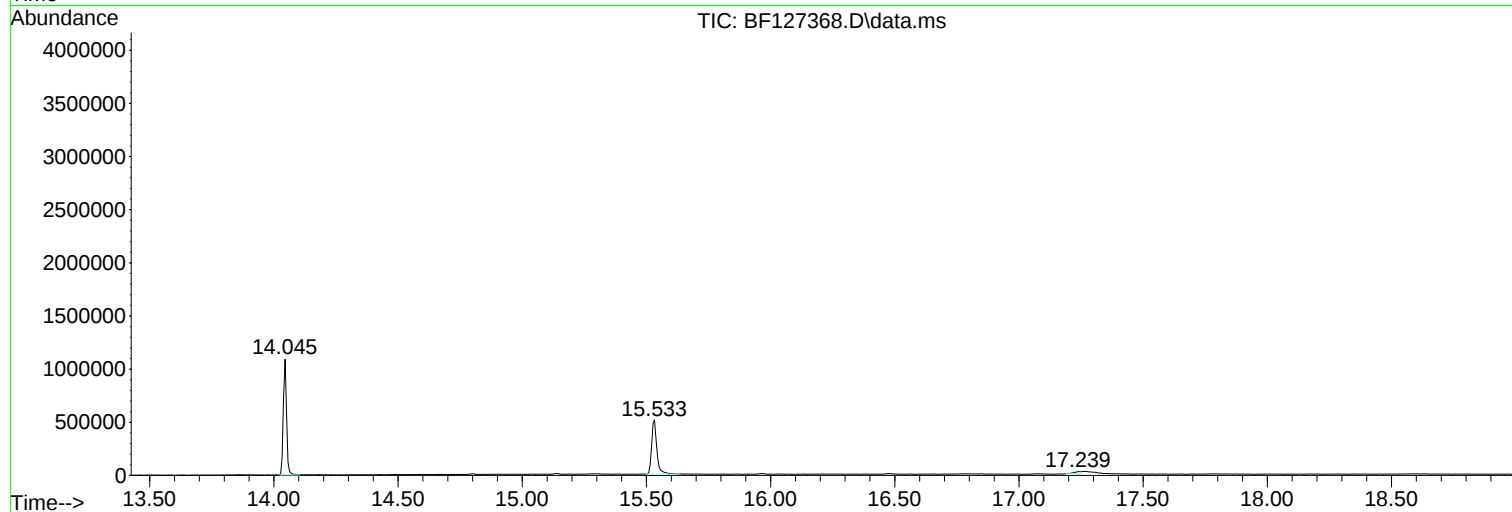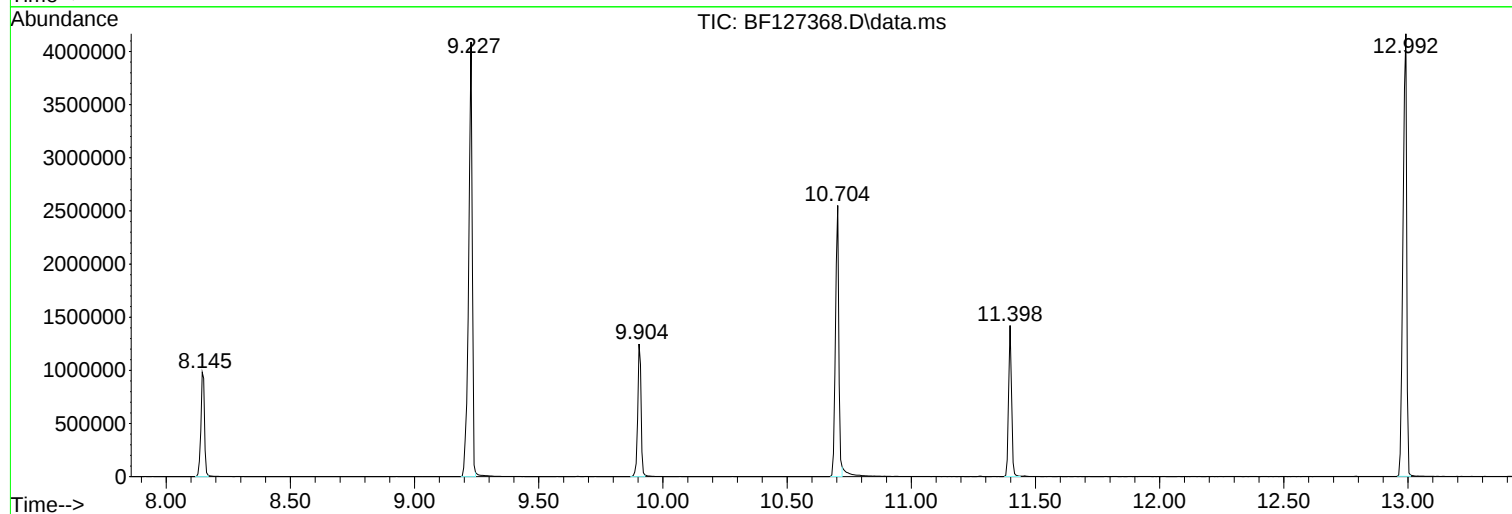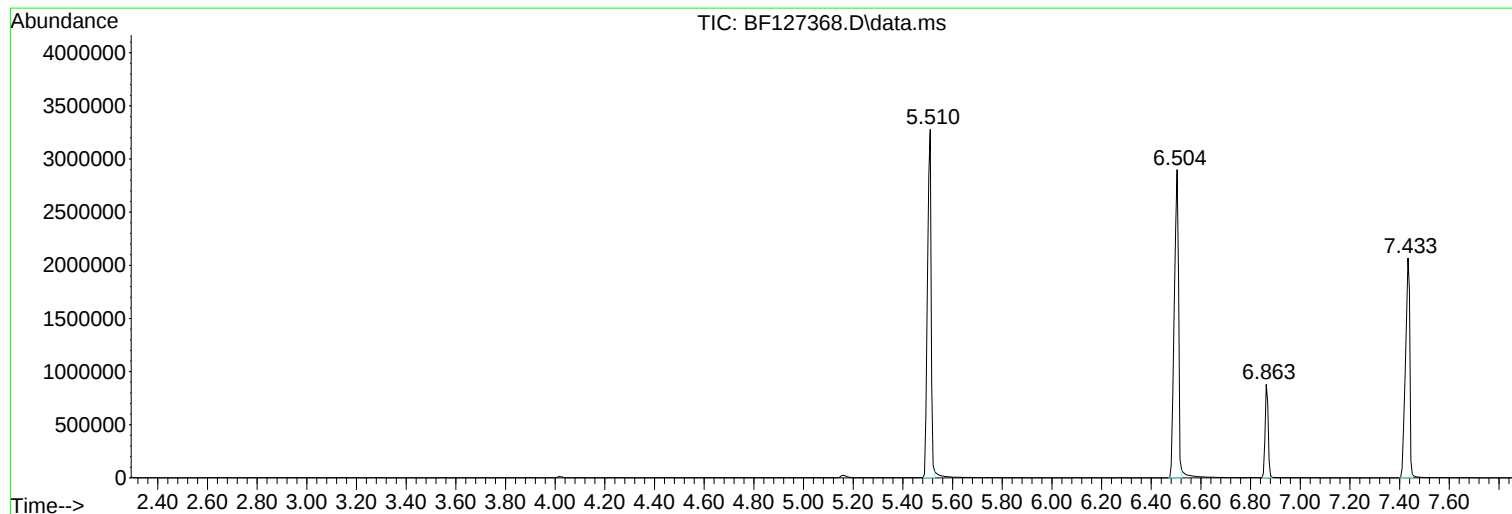

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127368.D
Acq On : 17 Mar 2022 11:12
Operator : CG\JU
Sample : PB143399BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143399BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127368.D
Acq On : 17 Mar 2022 11:12
Operator : CG\JU
Sample : PB143399BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143399BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------