

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
 Data File : BF127384.D
 Acq On : 17 Mar 2022 19:12
 Operator : CG\JU
 Sample : N1954-01 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-031522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	540	544	557	rBV	1138711	1079213	100.00%	7.657%
2	6.498	712	716	728	rBV	1108473	1060457	98.26%	7.524%
3	6.863	775	778	782	rBV	805023	696794	64.57%	4.944%
4	7.428	871	874	882	rBV	782012	686287	63.59%	4.869%
5	8.116	988	991	993	rBV	16486	14339	1.33%	0.102%
6	8.151	993	997	999	rVV	1015683	860647	79.75%	6.106%
7	8.169	999	1000	1007	rVB	76645	69313	6.42%	0.492%
8	8.727	1093	1095	1100	rVB2	25684	18898	1.75%	0.134%
9	8.863	1115	1118	1121	rVB	40811	30616	2.84%	0.217%
10	8.963	1130	1135	1138	rBV2	38395	36179	3.35%	0.257%
11	9.222	1175	1179	1182	rBV	1316598	1032557	95.68%	7.326%
12	9.292	1188	1191	1194	rVB	38654	29234	2.71%	0.207%
13	9.492	1221	1225	1229	rBV	18062	24343	2.26%	0.173%
14	9.563	1229	1237	1240	rBV3	27242	35864	3.32%	0.254%
15	9.610	1243	1245	1248	rVB3	15765	13578	1.26%	0.096%
16	9.680	1254	1257	1262	rVB2	15805	16350	1.51%	0.116%
17	9.769	1266	1272	1276	rBV2	19009	21824	2.02%	0.155%
18	9.822	1276	1281	1284	rVV	31162	25768	2.39%	0.183%
19	9.904	1292	1295	1299	rBV	960692	808069	74.88%	5.733%
20	9.939	1299	1301	1308	rVB	97434	79774	7.39%	0.566%
21	10.110	1327	1330	1333	rVV2	52494	45912	4.25%	0.326%
22	10.145	1333	1336	1340	rVB2	19781	20310	1.88%	0.144%
23	10.222	1345	1349	1352	rBV3	13363	17262	1.60%	0.122%
24	10.322	1360	1366	1370	rBV2	36666	42082	3.90%	0.299%
25	10.457	1383	1389	1394	rBV	92318	92265	8.55%	0.655%
26	10.521	1394	1400	1401	rBV2	12924	17184	1.59%	0.122%
27	10.539	1401	1403	1406	rVB	24742	22244	2.06%	0.158%
28	10.610	1413	1415	1421	rVB	20445	19778	1.83%	0.140%
29	10.698	1426	1430	1444	rVB	499470	473465	43.87%	3.359%
30	10.798	1444	1447	1451	rBV3	34314	48760	4.52%	0.346%
31	11.004	1477	1482	1484	rBV2	24862	25240	2.34%	0.179%
32	11.127	1498	1503	1505	rBV4	12042	19190	1.78%	0.136%
33	11.245	1520	1523	1526	rBV2	36789	33679	3.12%	0.239%
34	11.274	1526	1528	1530	rVV	21089	21107	1.96%	0.150%
35	11.292	1530	1531	1536	rVB	28519	23339	2.16%	0.166%
36	11.398	1545	1549	1551	rBV	847542	722810	66.98%	5.128%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
 Data File : BF127384.D
 Acq On : 17 Mar 2022 19:12
 Operator : CG\JU
 Sample : N1954-01 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-031522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.421	1551	1553	1557	rVV	517680	396753	36.76%	2.815%
38	11.474	1559	1562	1565	rVB	151254	120776	11.19%	0.857%
39	11.633	1584	1589	1593	rBV	36554	50271	4.66%	0.357%
40	11.674	1593	1596	1597	rVV	20702	15172	1.41%	0.108%
41	11.733	1603	1606	1610	rVB4	12146	16017	1.48%	0.114%
42	11.898	1631	1634	1637	rBV	57118	57658	5.34%	0.409%
43	11.927	1637	1639	1643	rVB	82756	67219	6.23%	0.477%
44	11.974	1643	1647	1650	rBV	40354	38492	3.57%	0.273%
45	12.016	1650	1654	1656	rBV	105313	116904	10.83%	0.829%
46	12.080	1662	1665	1668	rBV2	26745	22364	2.07%	0.159%
47	12.192	1681	1684	1687	rBV	39800	37753	3.50%	0.268%
48	12.227	1687	1690	1694	rVB4	15669	15369	1.42%	0.109%
49	12.451	1724	1728	1729	rBV	33840	35101	3.25%	0.249%
50	12.545	1740	1744	1747	rBV4	23409	31866	2.95%	0.226%
51	12.615	1752	1756	1759	rBV	714427	604245	55.99%	4.287%
52	12.768	1779	1782	1784	rBV2	18549	17949	1.66%	0.127%
53	12.786	1784	1785	1788	rVB3	16269	12712	1.18%	0.090%
54	12.827	1788	1792	1793	rBV2	132445	134827	12.49%	0.957%
55	12.845	1793	1795	1801	rVB	633612	518180	48.01%	3.677%
56	12.892	1801	1803	1807	rVB2	32651	32080	2.97%	0.228%
57	12.980	1811	1818	1821	rBV	976797	848476	78.62%	6.020%
58	13.010	1821	1823	1827	rVB	23966	21869	2.03%	0.155%
59	13.063	1827	1832	1836	rBV2	40360	75922	7.03%	0.539%
60	13.174	1843	1851	1854	rBV	98532	150298	13.93%	1.066%
61	13.239	1859	1862	1864	rVV	89305	72839	6.75%	0.517%
62	13.274	1864	1868	1871	rVV2	55674	64503	5.98%	0.458%
63	13.368	1882	1884	1887	rBV	24367	22129	2.05%	0.157%
64	13.398	1887	1889	1895	rVV4	31533	49957	4.63%	0.354%
65	13.686	1936	1938	1941	rBV2	25276	20131	1.87%	0.143%
66	13.792	1954	1956	1959	rVB	33646	30295	2.81%	0.215%
67	13.821	1959	1961	1963	rVB	50645	33172	3.07%	0.235%
68	13.845	1963	1965	1967	rBV	35126	32832	3.04%	0.233%
69	14.045	1994	1999	2002	rBV2	758071	885979	82.09%	6.286%
70	14.068	2002	2003	2009	rVB	222128	183785	17.03%	1.304%
71	14.151	2015	2017	2019	rVB	58836	41480	3.84%	0.294%
72	15.098	2174	2178	2181	rBV	157912	230503	21.36%	1.635%
73	15.404	2228	2230	2236	rVB	86278	104734	9.70%	0.743%
74	15.468	2238	2241	2247	rVV	131574	181316	16.80%	1.286%
75	15.533	2248	2252	2256	rVV	339933	417370	38.67%	2.961%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127384.D
Acq On : 17 Mar 2022 19:12
Operator : CG\JU
Sample : N1954-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-031522

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 14094029

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127384.D
Acq On : 17 Mar 2022 19:12
Operator : CG\JU
Sample : N1954-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-031522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

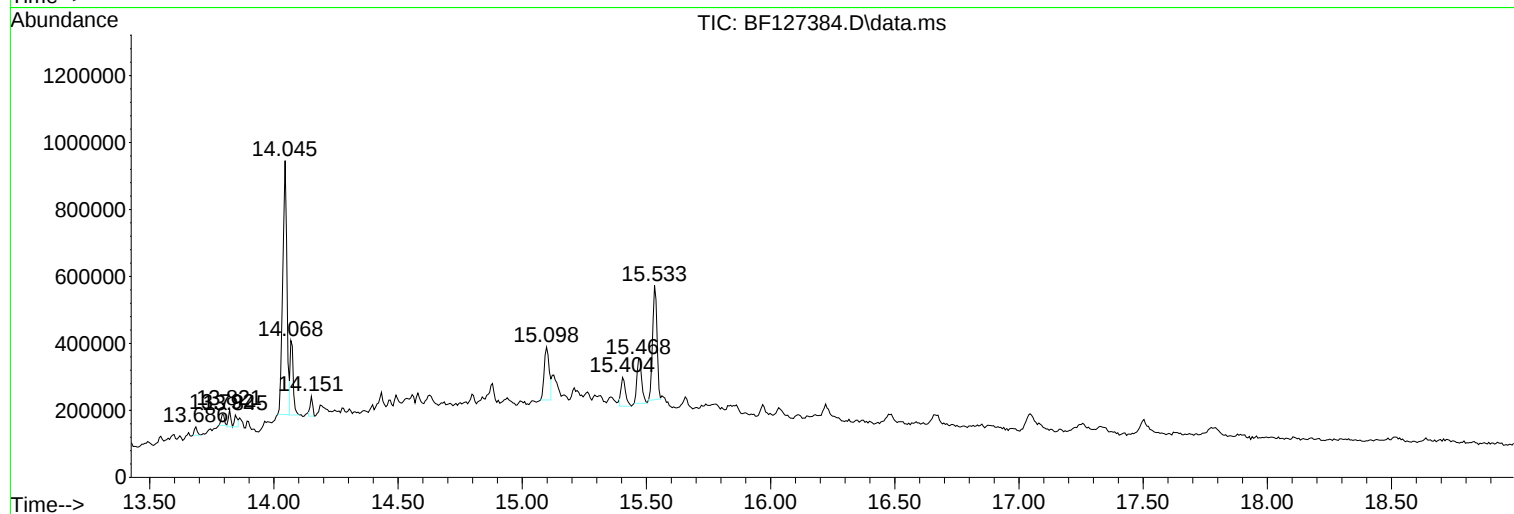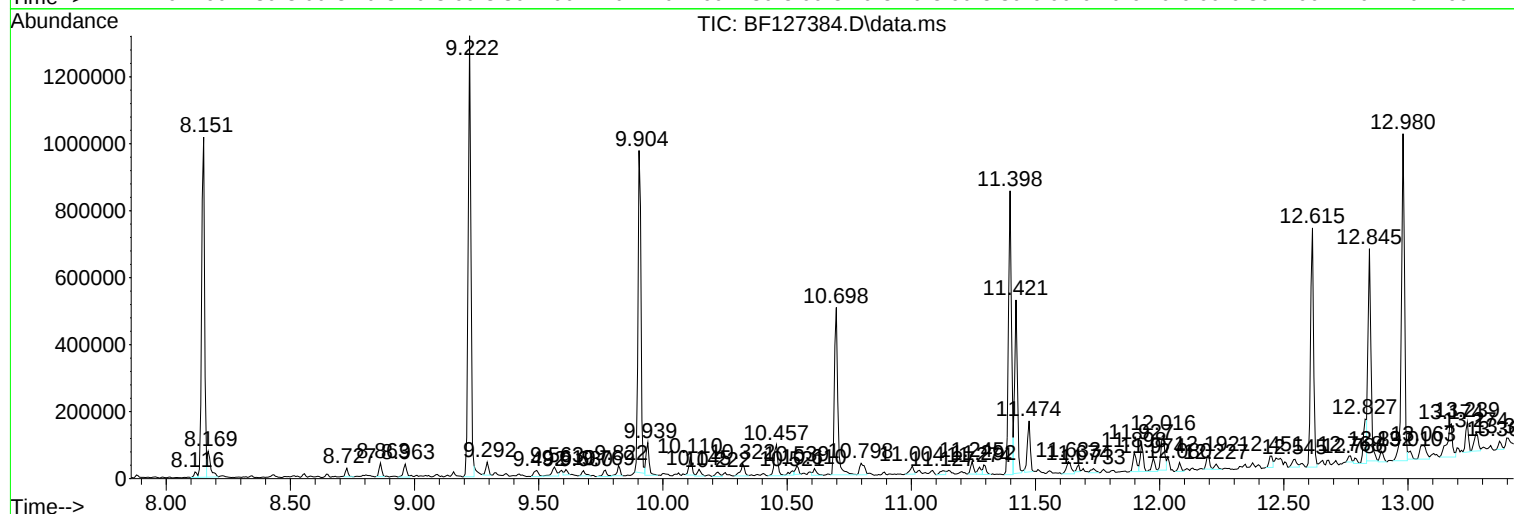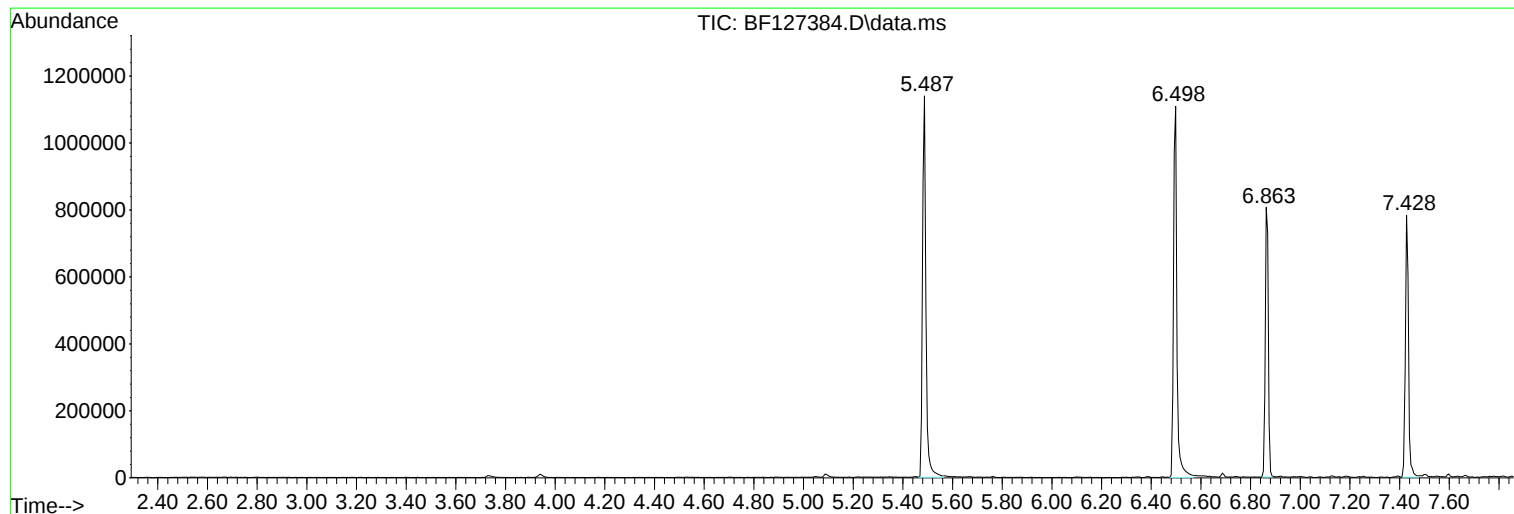

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127384.D
Acq On : 17 Mar 2022 19:12
Operator : CG\JU
Sample : N1954-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-031522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127384.D
Acq On : 17 Mar 2022 19:12
Operator : CG\JU
Sample : N1954-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-031522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------