

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
 Data File : BF127387.D
 Acq On : 17 Mar 2022 20:39
 Operator : CG\JU
 Sample : N1993-01 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-04-03162022

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.934	272	280	288	rVB2	7312	11214	1.25%	0.150%
2	5.081	471	475	482	rVB3	7762	13455	1.51%	0.180%
3	5.275	501	508	511	rBV5	10447	14551	1.63%	0.195%
4	5.487	541	544	553	rBV	826746	788915	88.29%	10.566%
5	5.551	553	555	560	rVB4	9623	11800	1.32%	0.158%
6	5.763	588	591	597	rBV	15857	14772	1.65%	0.198%
7	6.498	712	716	731	rBV	852123	794304	88.89%	10.638%
8	6.687	745	748	751	rVB	20050	17346	1.94%	0.232%
9	6.869	775	779	782	rBV	483190	433038	48.46%	5.800%
10	7.428	871	874	882	rBV	545840	524045	58.64%	7.019%
11	8.151	993	997	1000	rBV	600811	482678	54.02%	6.465%
12	8.728	1090	1095	1100	rVB	17295	13224	1.48%	0.177%
13	9.222	1176	1179	1183	rBV	1057964	825668	92.40%	11.059%
14	9.292	1189	1191	1195	rVB	28172	24164	2.70%	0.324%
15	9.610	1240	1245	1248	rBV2	22081	25145	2.81%	0.337%
16	9.822	1277	1281	1284	rBV3	16555	16772	1.88%	0.225%
17	9.910	1292	1296	1299	rBV	578379	506914	56.73%	6.789%
18	10.322	1359	1366	1369	rBV2	17274	23039	2.58%	0.309%
19	10.545	1398	1404	1407	rBV	19762	25138	2.81%	0.337%
20	10.698	1427	1430	1439	rBV	540032	474576	53.11%	6.356%
21	10.810	1444	1449	1452	rBV	42570	49272	5.51%	0.660%
22	11.245	1520	1523	1525	rBV	15044	13102	1.47%	0.175%
23	11.275	1525	1528	1531	rVB2	19496	19925	2.23%	0.267%
24	11.398	1545	1549	1553	rBV	639229	544033	60.88%	7.286%
25	11.674	1593	1596	1598	rVB2	13287	11687	1.31%	0.157%
26	11.774	1611	1613	1616	rVB3	14307	12005	1.34%	0.161%
27	12.327	1705	1707	1711	rBV5	8383	11573	1.30%	0.155%
28	12.469	1726	1731	1733	rBV4	33117	43665	4.89%	0.585%
29	12.616	1754	1756	1758	rBV	12155	10701	1.20%	0.143%
30	12.845	1793	1795	1797	rBV	15070	11626	1.30%	0.156%
31	12.980	1815	1818	1822	rBV	974820	893594	100.00%	11.968%
32	14.045	1996	1999	2003	rBV	489739	454637	50.88%	6.089%
33	15.539	2249	2253	2258	rVB	282914	349772	39.14%	4.685%




Sum of corrected areas: 7466350

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127387.D
Acq On : 17 Mar 2022 20:39
Operator : CG\JU
Sample : N1993-01 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-04-03162022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

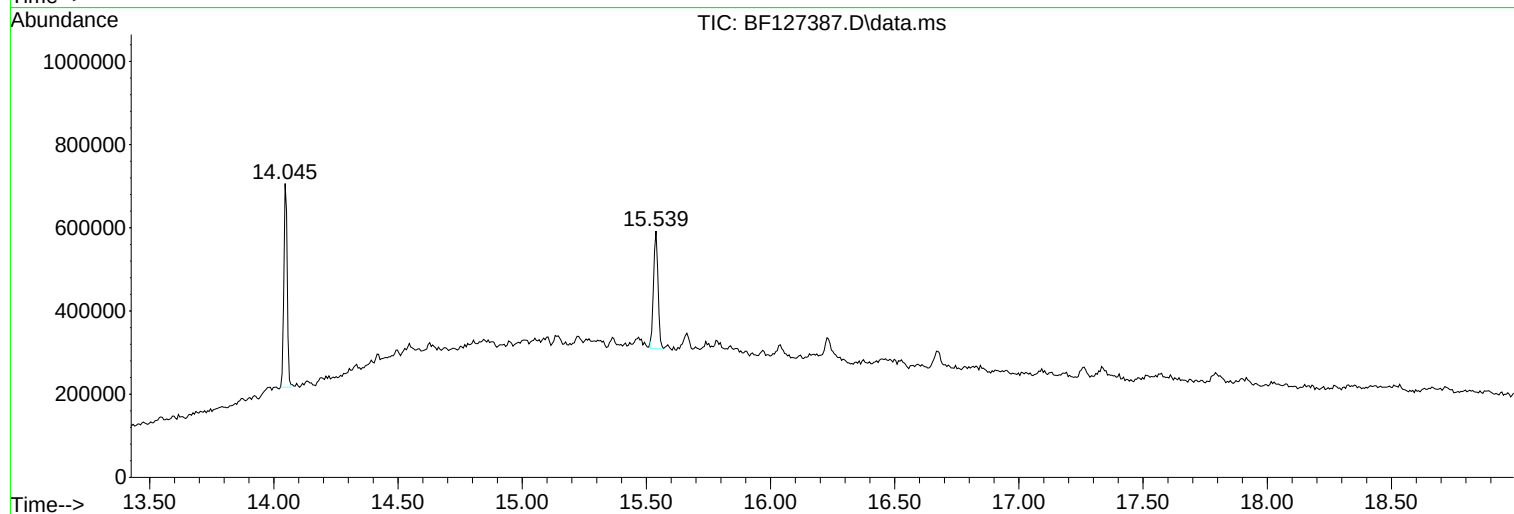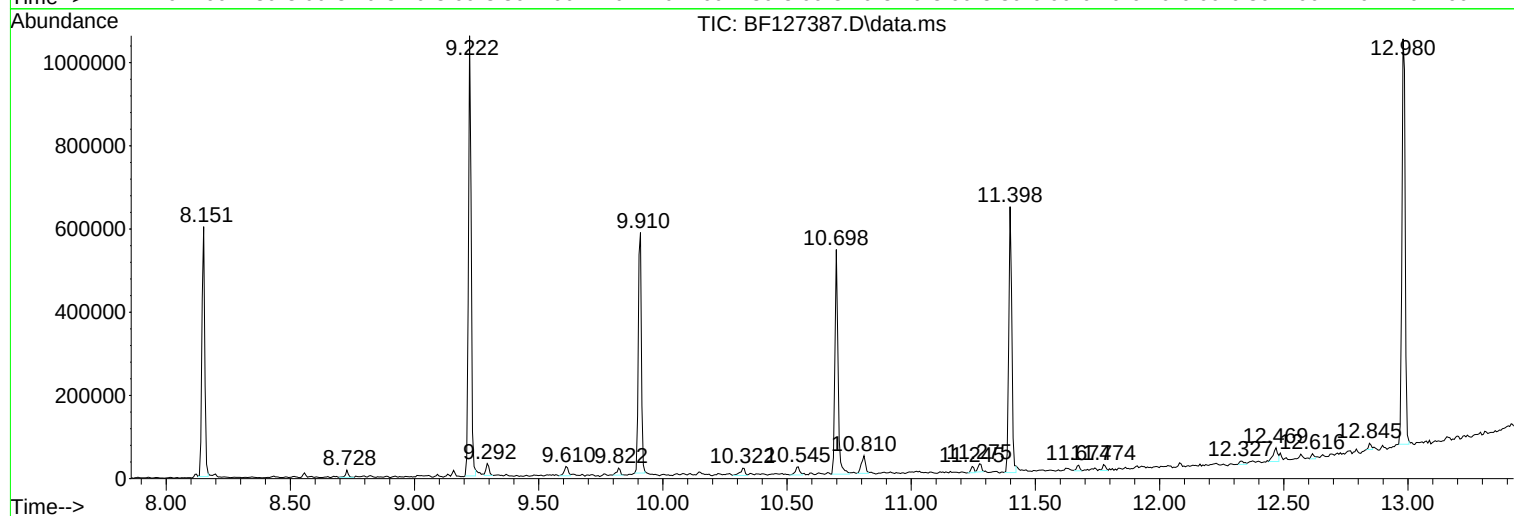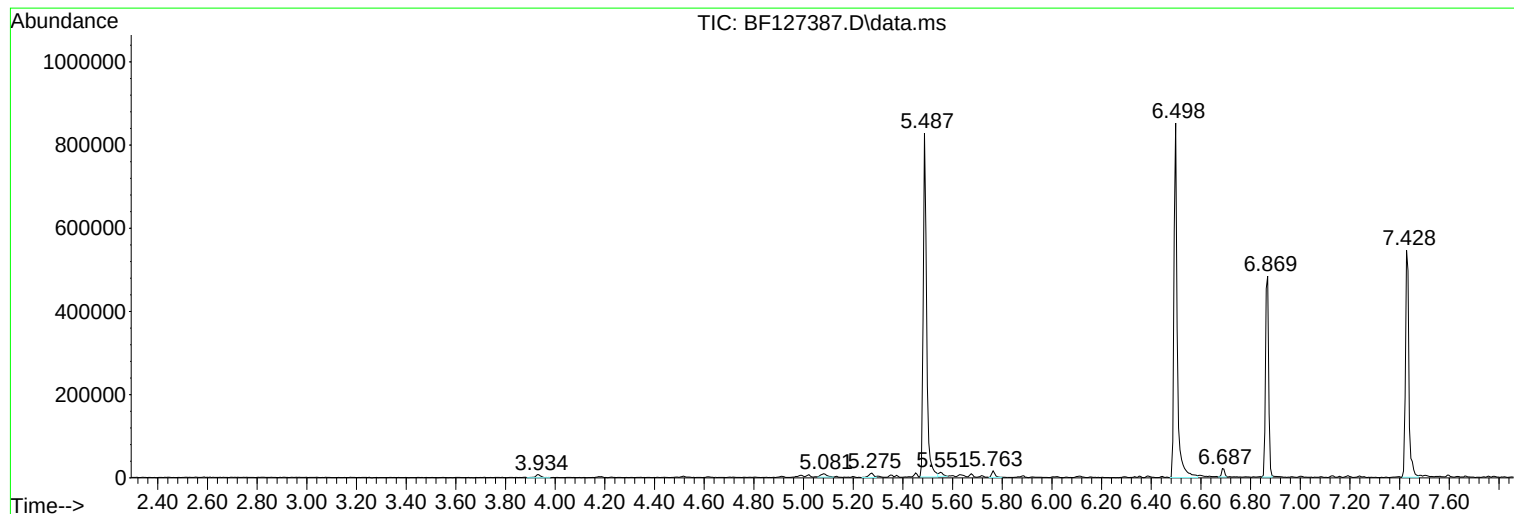

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127387.D
Acq On : 17 Mar 2022 20:39
Operator : CG\JU
Sample : N1993-01 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-04-03162022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127387.D
Acq On : 17 Mar 2022 20:39
Operator : CG\JU
Sample : N1993-01 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-04-03162022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------